
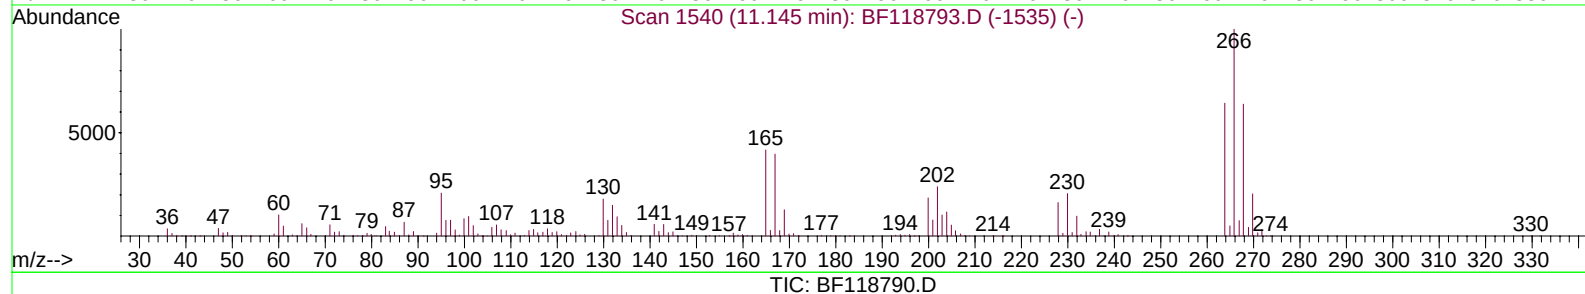
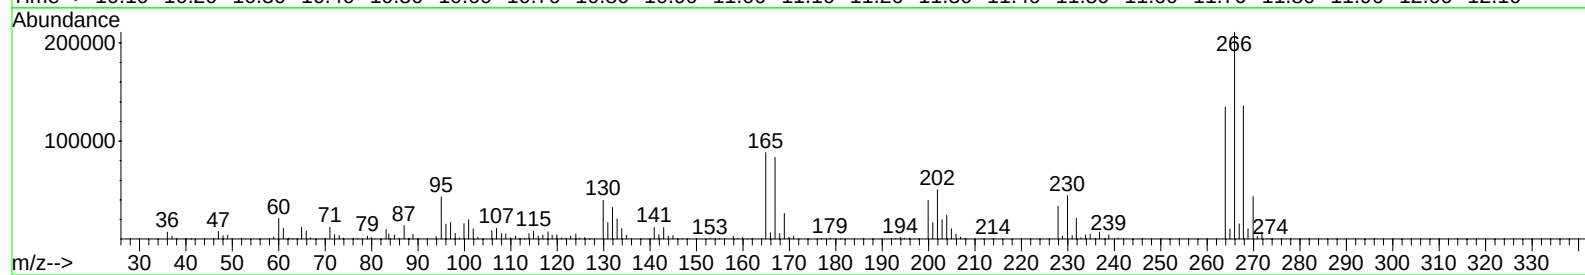


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF020320\
Data File : BF118790.D
Acq On : 3 Feb 2020 10:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 03 18:03:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF020320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 03 16:26:03 2020
Response via : Initial Calibration

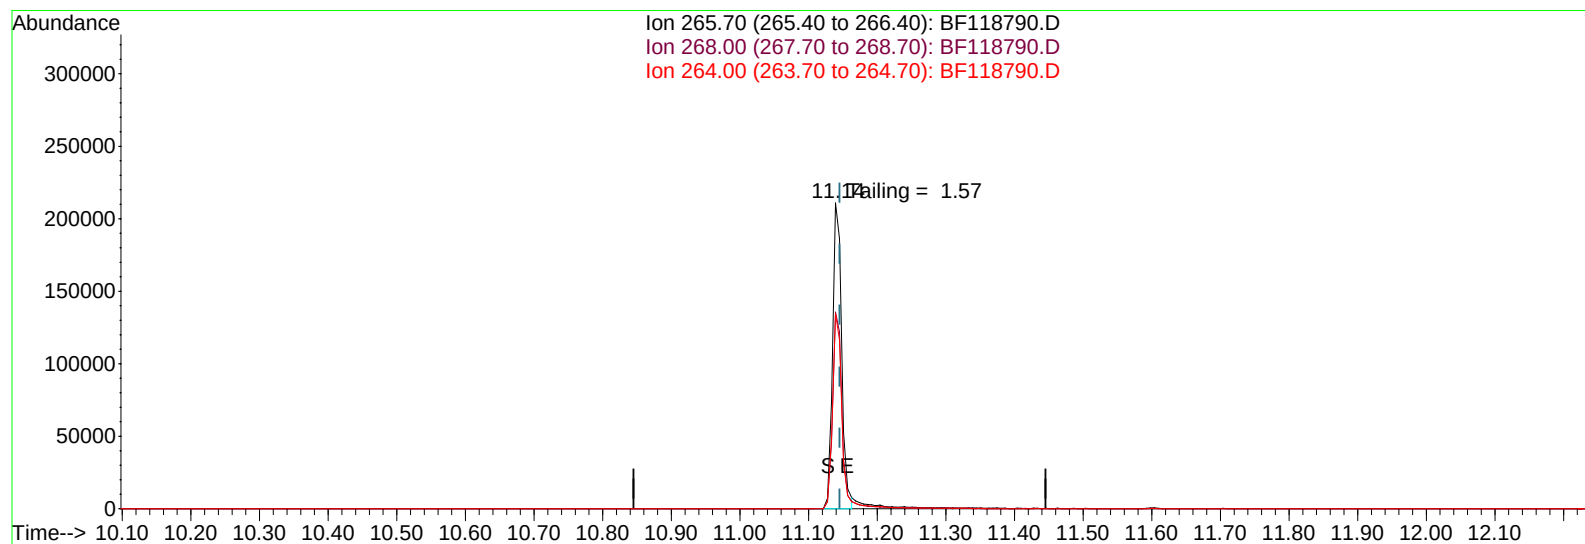

(70) Pentachlorophenol (C)




11.139min (-0.006) 35948.61ng

response 205267

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	64.34
264.00	64.30	63.88
0.00	0.00	0.00

```
Data Path   : Z:\svoasrv\HPCHEM1\BNA F\Data\BF020320\  
Data File   : BF118790.D  
Acq On      : 3 Feb 2020 10:55  
Operator    : CG/JU  
Sample      : DFTPP  
Misc        :  
ALS Vial    : 1      Sample Multiplier: 1
```

Quant Time: Feb 03 18:03:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF020320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 03 16:26:03 2020
Response via : Initial Calibration

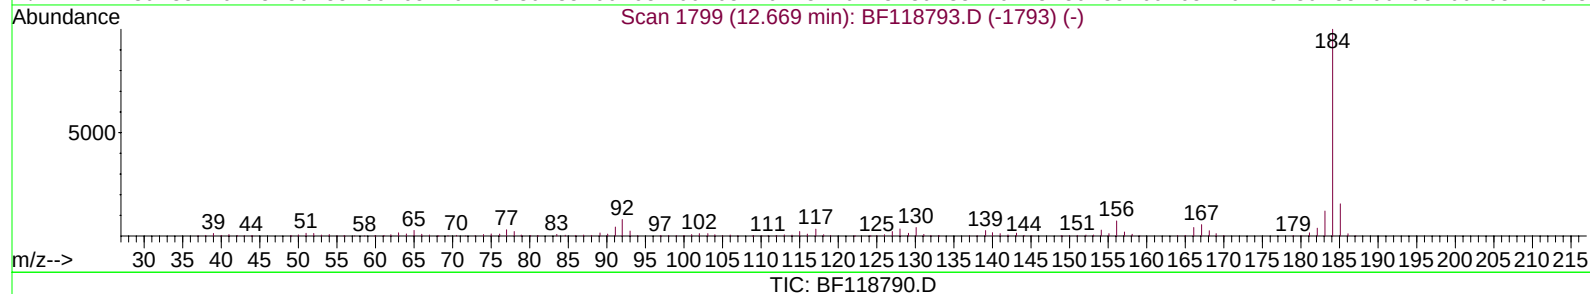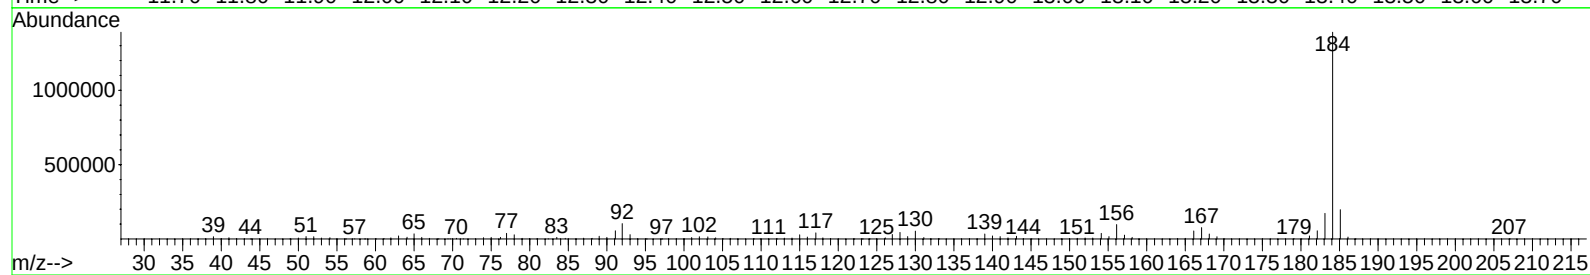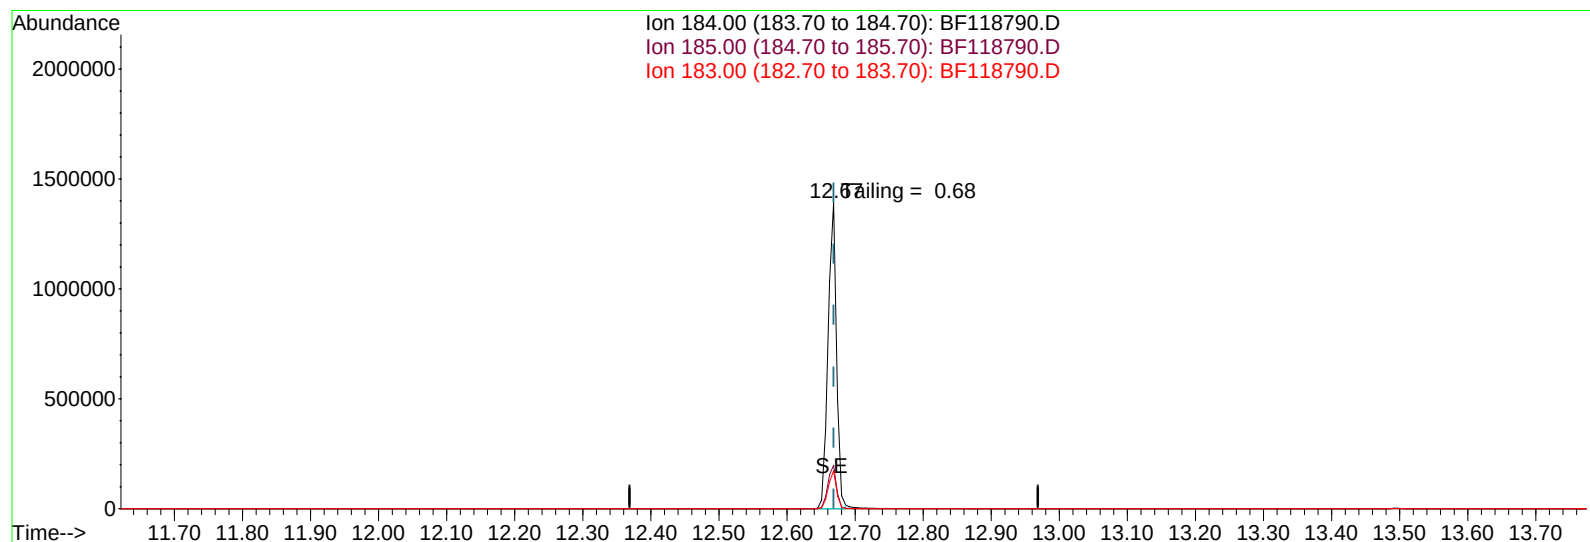

(77) Benzidine

12.668min (-0.000) 0.00ng m

response 1198947

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	14.22
183.00	12.10	12.39
0.00	0.00	0.00