
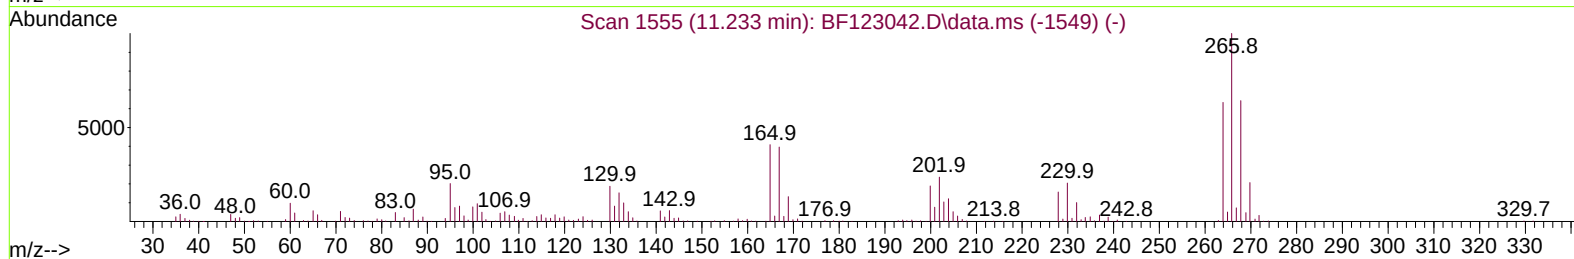
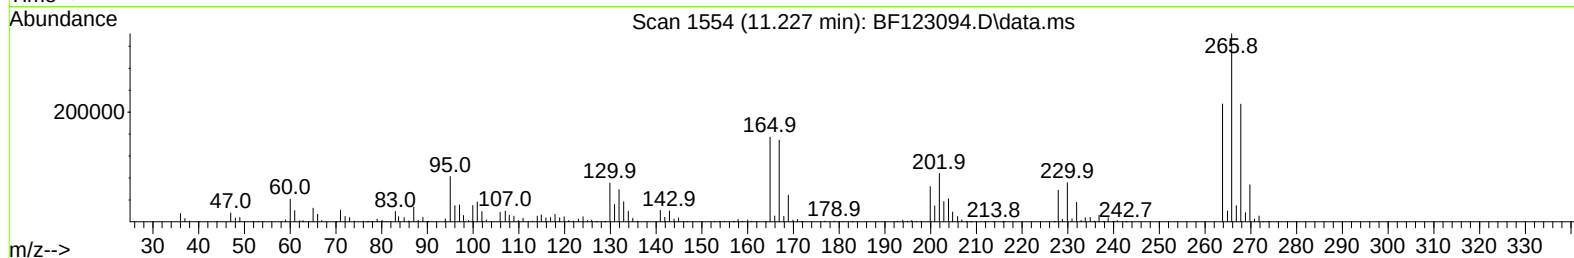


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020321\
Data File : BF123094.D
Acq On : 3 Feb 2021 9:33
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 04 02:00:41 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 29 12:29:00 2021
Response via : Initial Calibration

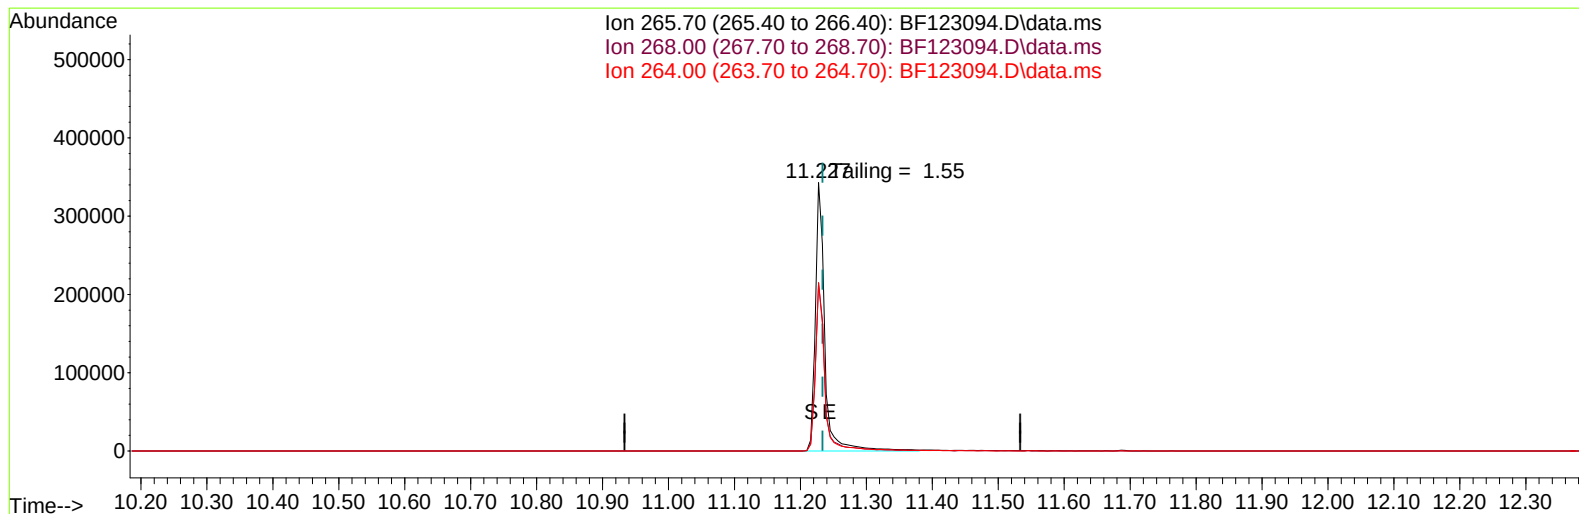

TIC: BF123094.D\data.ms

(70) Pentachlorophenol (C)




11.227min (-0.006) 33760.42 ng

response 338660

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.57
264.00	62.30	62.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020321\
Data File : BF123094.D
Acq On : 3 Feb 2021 9:33
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 04 02:00:41 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 29 12:29:00 2021
Response via : Initial Calibration

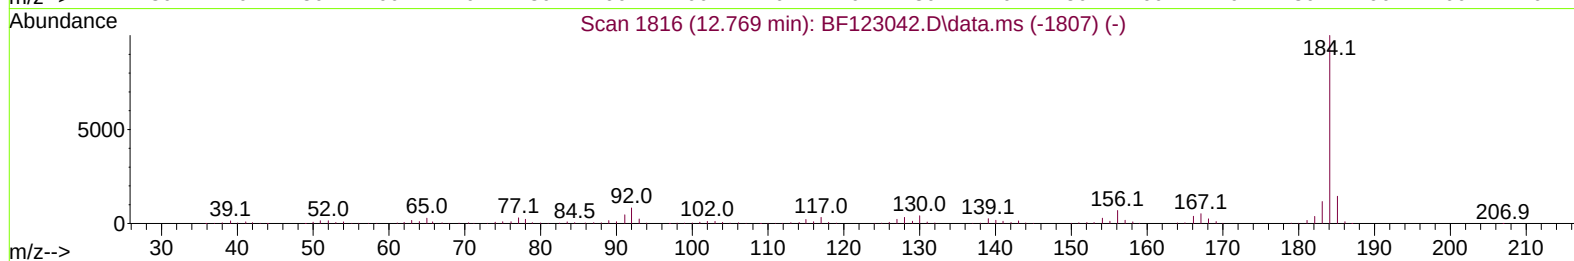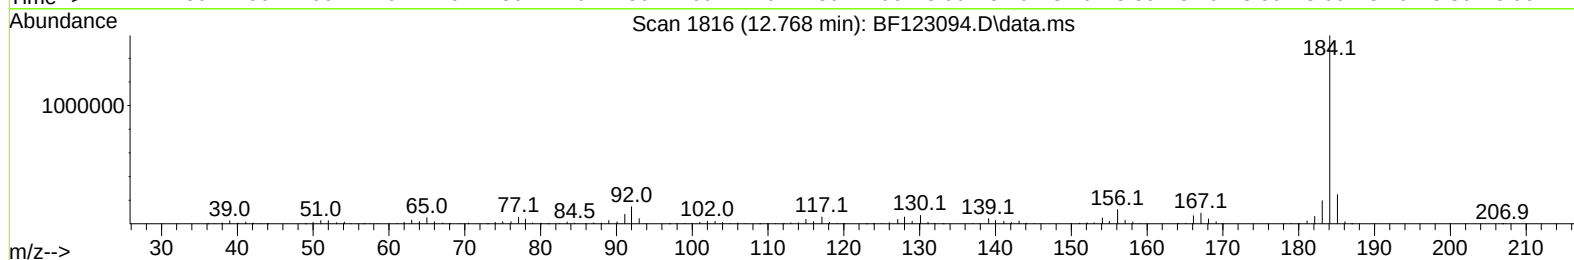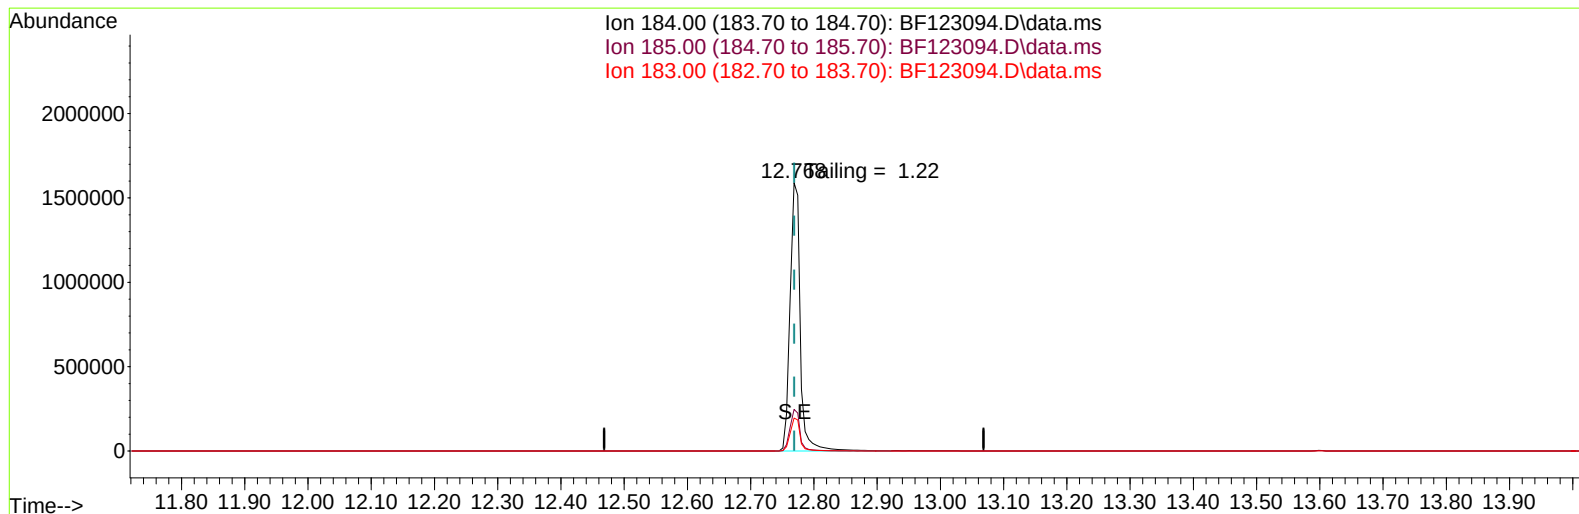

TIC: BF123094.D\data.ms

(77) Benzidine

12.768min (-0.000) 0.00 ng

response 1790154

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	15.53
183.00	12.10	12.29
0.00	0.00	0.00