

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF020321\  
 Data File : BF123096.D  
 Acq On : 3 Feb 2021 10:44  
 Operator : JU/CG  
 Sample : PB134433BL  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 PB134433BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF012721.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF123096.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.516       | 578           | 583         | 586          | rBV      | 5693746        | 6168740       | 68.55%          | 12.227%       |
| 2         | 6.516       | 747           | 753         | 756          | rBV      | 5421134        | 6136956       | 68.20%          | 12.164%       |
| 3         | 6.892       | 813           | 817         | 820          | rBV      | 1808615        | 1417780       | 15.76%          | 2.810%        |
| 4         | 7.451       | 907           | 912         | 915          | rBV      | 3810250        | 4141202       | 46.02%          | 8.208%        |
| 5         | 8.175       | 1030          | 1035        | 1039         | rBV      | 2102527        | 1865411       | 20.73%          | 3.697%        |
| 6         | 9.257       | 1213          | 1219        | 1222         | rBV      | 6959977        | 7438684       | 82.67%          | 14.744%       |
| 7         | 9.933       | 1329          | 1334        | 1338         | rBV      | 2373376        | 2195482       | 24.40%          | 4.352%        |
| 8         | 10.727      | 1463          | 1469        | 1472         | rBV      | 4938062        | 4916509       | 54.64%          | 9.745%        |
| 9         | 11.427      | 1583          | 1588        | 1591         | rBV      | 2638153        | 2285319       | 25.40%          | 4.530%        |
| 10        | 11.951      | 1671          | 1677        | 1688         | rBV      | 184536         | 247884        | 2.75%           | 0.491%        |
| 11        | 13.027      | 1854          | 1860        | 1863         | rBV      | 8360626        | 8998490       | 100.00%         | 17.836%       |
| 12        | 14.080      | 2030          | 2039        | 2051         | rBV      | 2282282        | 2354277       | 26.16%          | 4.666%        |
| 13        | 14.862      | 2155          | 2172        | 2183         | rBV6     | 71164          | 287720        | 3.20%           | 0.570%        |
| 14        | 15.562      | 2284          | 2291        | 2313         | rBV      | 1263397        | 1996275       | 22.18%          | 3.957%        |




Sum of corrected areas: 50450729

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF020321\  
Data File : BF123096.D  
Acq On : 3 Feb 2021 10:44  
Operator : JU/CG  
Sample : PB134433BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB134433BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF012721.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

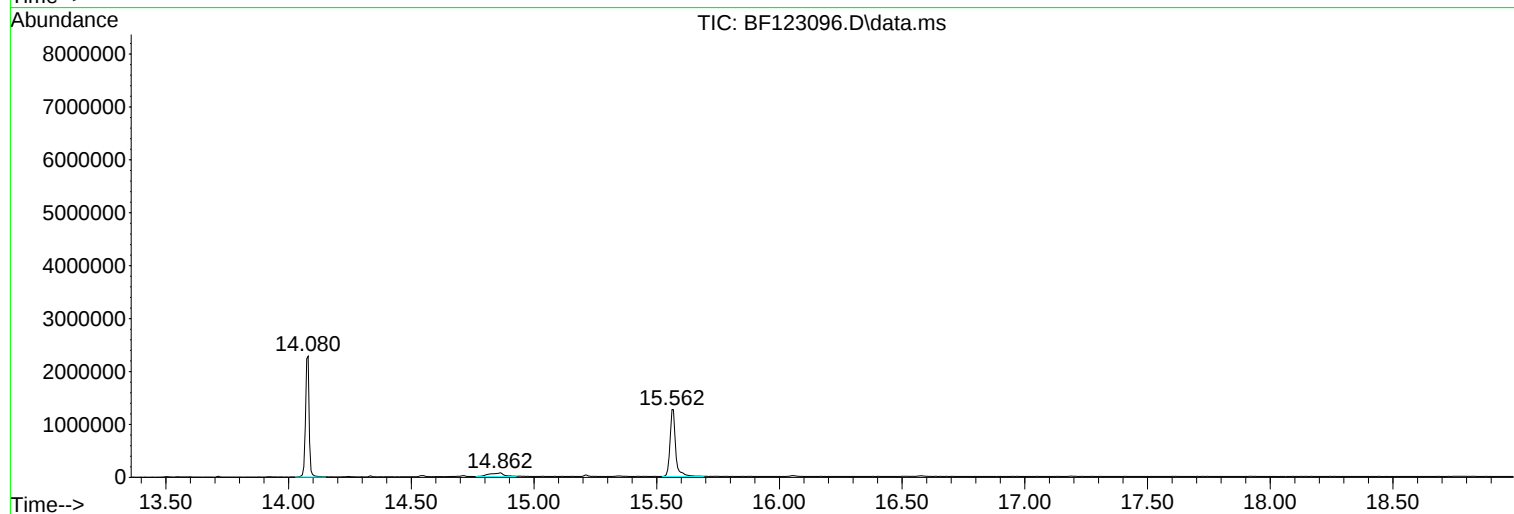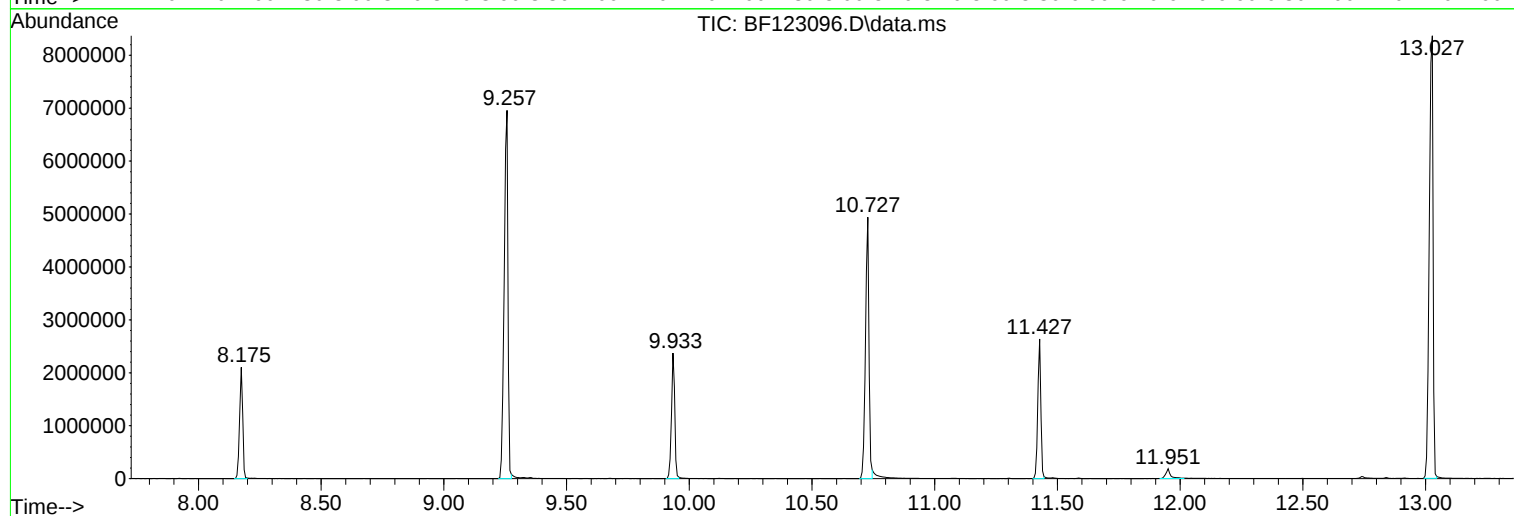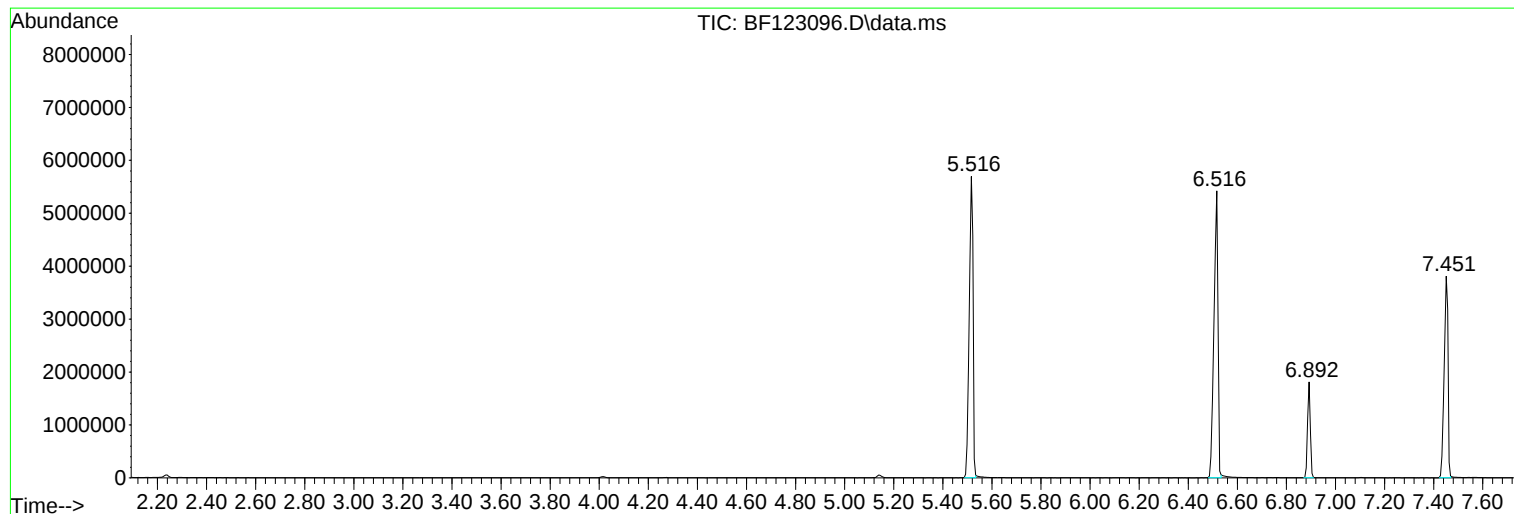

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF020321\  
Data File : BF123096.D  
Acq On : 3 Feb 2021 10:44  
Operator : JU/CG  
Sample : PB134433BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB134433BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF012721.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF020321\  
Data File : BF123096.D  
Acq On : 3 Feb 2021 10:44  
Operator : JU/CG  
Sample : PB134433BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB134433BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF012721.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|