

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020321\
 Data File : BF123100.D
 Acq On : 3 Feb 2021 13:02
 Operator : JU/CG
 Sample : M1292-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU421-009-0205

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF123100.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.175	7	15	20	rBV	525849	668948	10.92%	1.534%
2	5.110	507	514	521	rBV	352079	440031	7.19%	1.009%
3	5.510	577	582	585	rBV	4602260	4332017	70.74%	9.931%
4	6.516	747	753	770	rBV	4300904	4620089	75.44%	10.592%
5	6.892	813	817	820	rBV	1656090	1282610	20.94%	2.940%
6	7.451	907	912	915	rBV	3155923	2932360	47.88%	6.723%
7	8.175	1031	1035	1039	rBV	2046441	1696120	27.70%	3.888%
8	9.257	1214	1219	1222	rBV	5840495	5330693	87.05%	12.221%
9	9.369	1234	1238	1254	rVB	865531	1010716	16.50%	2.317%
10	9.527	1262	1265	1271	rBV	80168	67351	1.10%	0.154%
11	9.645	1281	1285	1289	rBV	172107	139831	2.28%	0.321%
12	9.933	1330	1334	1338	rBV	2156337	1990061	32.50%	4.562%
13	10.551	1433	1439	1452	rBV3	102330	354118	5.78%	0.812%
14	10.727	1464	1469	1484	rBV	3595780	3575427	58.38%	8.197%
15	11.427	1584	1588	1591	rBV	2394192	2043928	33.38%	4.686%
16	11.951	1671	1677	1682	rBV	333835	329279	5.38%	0.755%
17	12.680	1798	1801	1804	rVB	131111	107541	1.76%	0.247%
18	12.739	1808	1811	1819	rBV	68390	90623	1.48%	0.208%
19	13.021	1854	1859	1862	rBV	6327765	6123904	100.00%	14.039%
20	13.468	1930	1935	1937	rBV2	51707	75487	1.23%	0.173%
21	13.815	1974	1994	2009	rBV5	432594	2375393	38.79%	5.446%
22	14.004	2015	2026	2029	rBV7	245815	816232	13.33%	1.871%
23	14.080	2035	2039	2042	rBV	1701273	1595684	26.06%	3.658%
24	14.862	2170	2172	2179	rVB2	64778	75702	1.24%	0.174%
25	15.209	2228	2231	2235	rVB	76976	94861	1.55%	0.217%
26	15.568	2286	2292	2296	rBV	1012063	1367083	22.32%	3.134%
27	16.056	2371	2375	2379	rVB	56184	83170	1.36%	0.191%




Sum of corrected areas: 43619259

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020321\
Data File : BF123100.D
Acq On : 3 Feb 2021 13:02
Operator : JU/CG
Sample : M1292-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU421-009-0205

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

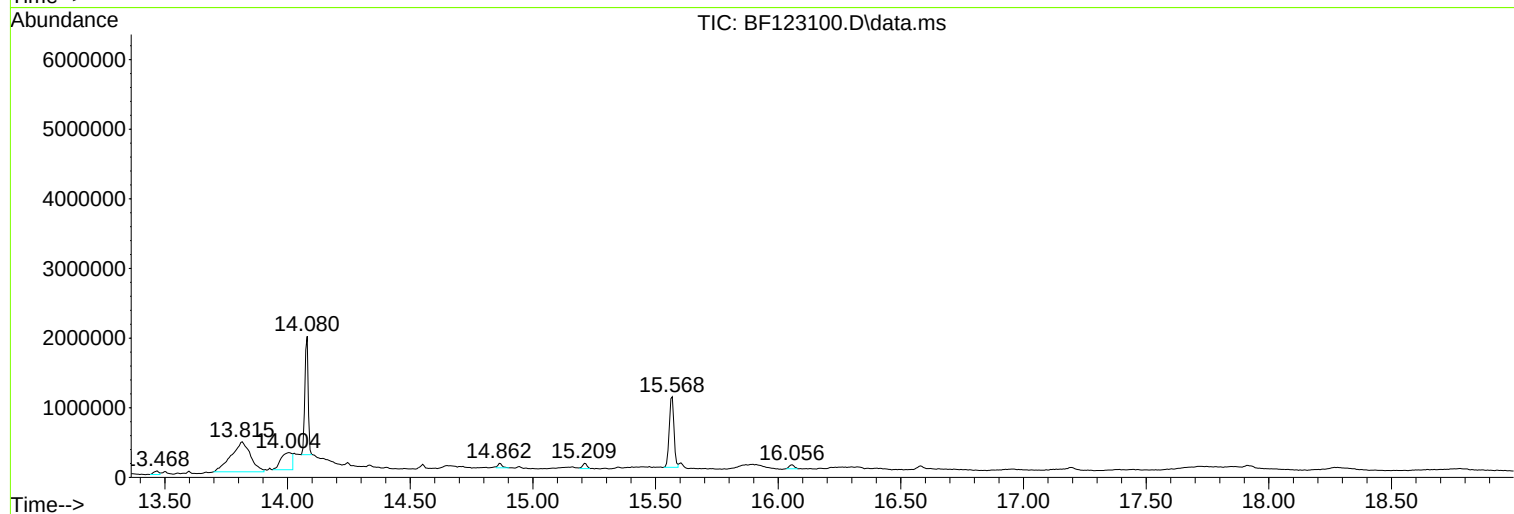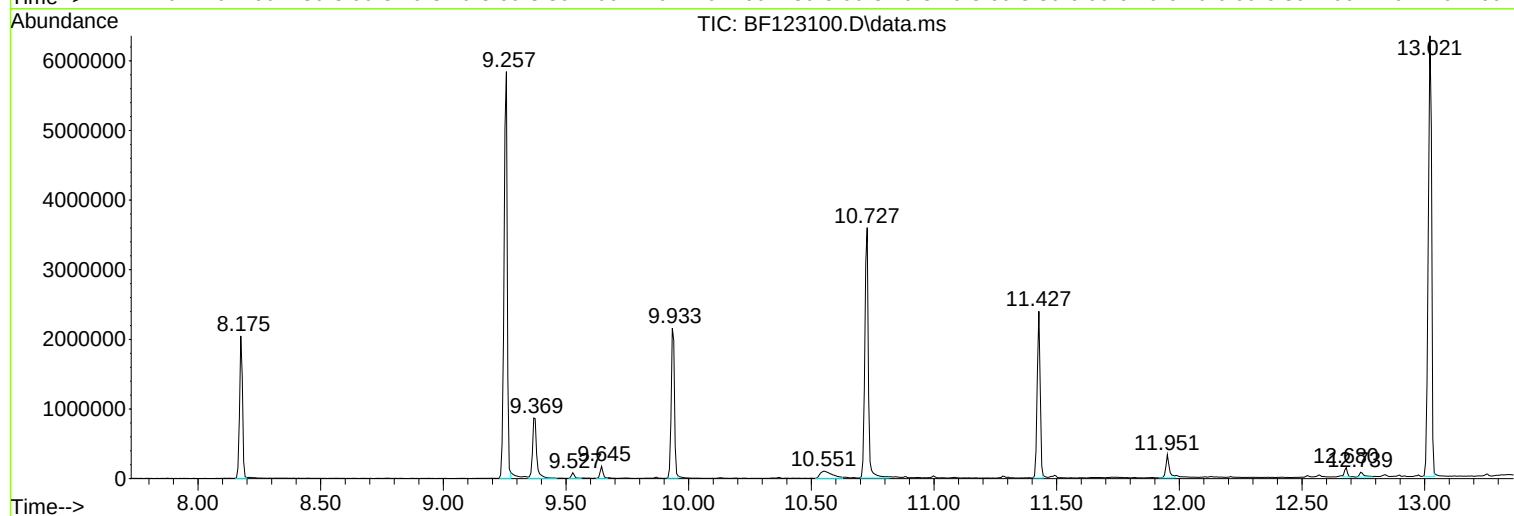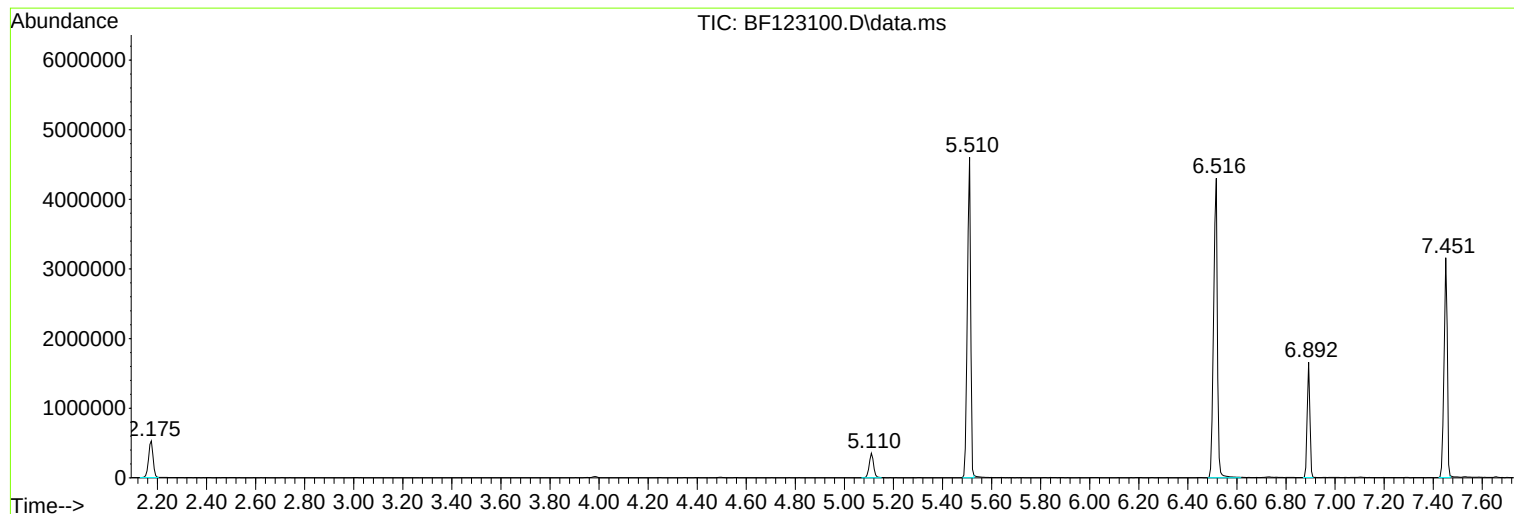

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020321\
Data File : BF123100.D
Acq On : 3 Feb 2021 13:02
Operator : JU/CG
Sample : M1292-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU421-009-0205

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020321\
Data File : BF123100.D
Acq On : 3 Feb 2021 13:02
Operator : JU/CG
Sample : M1292-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU421-009-0205

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------