

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020321\
 Data File : BF123101.D
 Acq On : 3 Feb 2021 13:35
 Operator : JU/CG
 Sample : M1292-11
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU421-009-0510

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF123101.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.163	6	13	20	rBV	490347	609179	10.20%	1.363%
2	5.110	507	514	521	rBV	110019	141835	2.37%	0.317%
3	5.510	577	582	585	rBV	4071733	4111361	68.84%	9.196%
4	6.516	747	753	767	rBV	3953979	4303218	72.05%	9.625%
5	6.892	813	817	820	rBV	1605472	1238903	20.74%	2.771%
6	7.451	907	912	915	rBV	3078863	2764597	46.29%	6.184%
7	8.175	1031	1035	1039	rBV	1939572	1632238	27.33%	3.651%
8	9.257	1214	1219	1222	rBV	5520669	5116725	85.67%	11.445%
9	9.645	1281	1285	1289	rBV	182821	148978	2.49%	0.333%
10	9.939	1330	1335	1338	rBV	2025401	1923839	32.21%	4.303%
11	10.727	1464	1469	1480	rBV	3498301	3526830	59.05%	7.888%
12	11.427	1584	1588	1591	rBV	2410708	2002787	33.53%	4.480%
13	11.951	1671	1677	1687	rBV2	505033	608821	10.19%	1.362%
14	12.739	1808	1811	1819	rBV	114841	121149	2.03%	0.271%
15	13.021	1854	1859	1862	rBV	6483943	5972623	100.00%	13.359%
16	13.780	1973	1988	1989	rBV5	285619	842574	14.11%	1.885%
17	13.810	1990	1993	2008	rVB5	362915	1041643	17.44%	2.330%
18	13.927	2008	2013	2015	rBV2	91170	88325	1.48%	0.198%
19	13.986	2017	2023	2035	rVV3	181999	725761	12.15%	1.623%
20	14.074	2035	2038	2042	rVB	1731928	1653405	27.68%	3.698%
21	14.551	2115	2119	2123	rBV	338071	302725	5.07%	0.677%
22	14.645	2128	2135	2139	rBV6	83536	237498	3.98%	0.531%
23	14.862	2167	2172	2177	rVB2	94709	128121	2.15%	0.287%
24	15.015	2194	2198	2202	rBV	298692	305463	5.11%	0.683%
25	15.209	2227	2231	2239	rVB	543436	638911	10.70%	1.429%
26	15.345	2248	2254	2257	rBV5	85897	200092	3.35%	0.448%
27	15.568	2286	2292	2296	rBV	1092063	1442851	24.16%	3.227%
28	15.604	2296	2298	2302	rVB	87377	94855	1.59%	0.212%
29	15.809	2328	2333	2341	rBV	622386	905371	15.16%	2.025%
30	16.056	2369	2375	2382	rVB	292975	460278	7.71%	1.029%
31	16.227	2399	2404	2405	rBV5	73981	111268	1.86%	0.249%
32	16.880	2509	2515	2523	rBV	317874	612905	10.26%	1.371%
33	17.121	2552	2556	2563	rVB4	67295	129332	2.17%	0.289%
34	17.192	2565	2568	2576	rVB3	51820	95929	1.61%	0.215%
35	18.356	2762	2766	2777	rVB4	75400	196972	3.30%	0.441%
36	18.745	2827	2832	2846	rVB6	86692	271582	4.55%	0.607%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020321\
Data File : BF123101.D
Acq On : 3 Feb 2021 13:35
Operator : JU/CG
Sample : M1292-11
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU421-009-0510

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION




Sum of corrected areas: 44708944

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020321\
Data File : BF123101.D
Acq On : 3 Feb 2021 13:35
Operator : JU/CG
Sample : M1292-11
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU421-009-0510

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

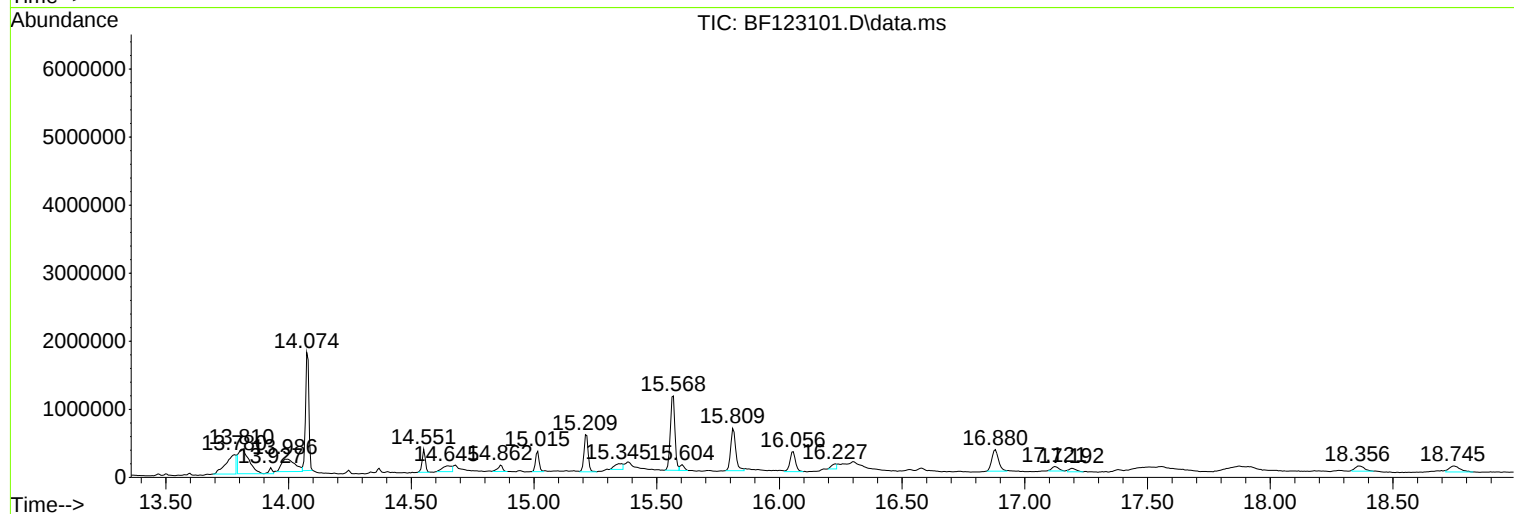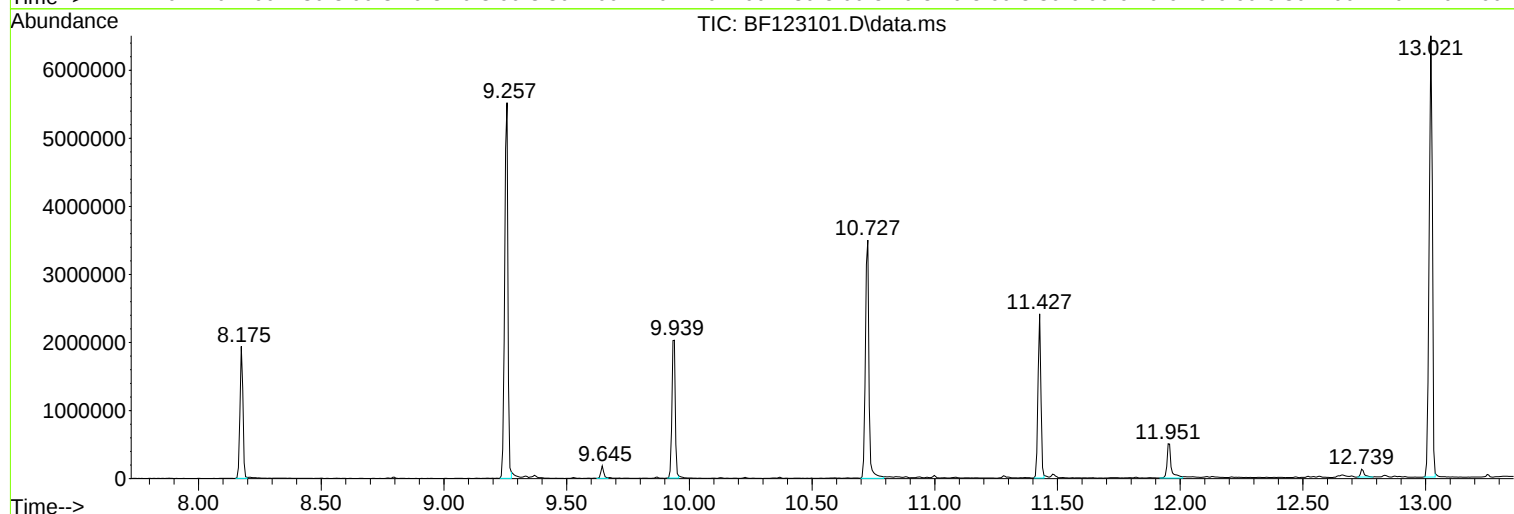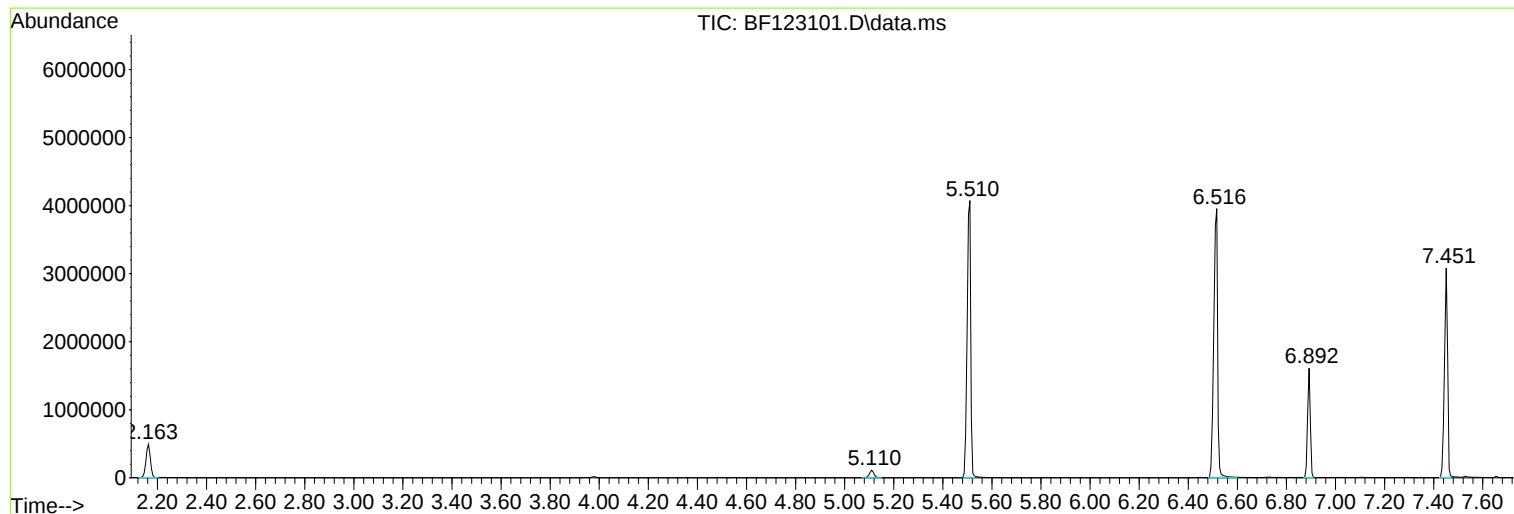

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020321\
Data File : BF123101.D
Acq On : 3 Feb 2021 13:35
Operator : JU/CG
Sample : M1292-11
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU421-009-0510

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020321\
Data File : BF123101.D
Acq On : 3 Feb 2021 13:35
Operator : JU/CG
Sample : M1292-11
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU421-009-0510

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------