

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020321\
 Data File : BF123102.D
 Acq On : 3 Feb 2021 14:07
 Operator : JU/CG
 Sample : M1292-17
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 2021-01-28-FD04

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF123102.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.163	7	13	21	rBV	476236	589048	10.59%	1.583%
2	5.104	508	513	519	rBV	258319	325465	5.85%	0.875%
3	5.504	577	581	585	rBV	3632605	3654295	65.69%	9.820%
4	6.510	747	752	764	rBV	3687660	3925859	70.57%	10.550%
5	6.892	813	817	820	rBV	1625922	1235340	22.21%	3.320%
6	7.451	907	912	915	rBV	2988845	2569910	46.19%	6.906%
7	8.175	1031	1035	1039	rBV	1959072	1630040	29.30%	4.380%
8	9.257	1214	1219	1222	rBV	5036376	4749482	85.37%	12.763%
9	9.645	1282	1285	1289	rBV	106106	84491	1.52%	0.227%
10	9.933	1330	1334	1338	rBV	1997303	1926642	34.63%	5.177%
11	10.721	1464	1468	1483	rBV	2725197	2835782	50.97%	7.620%
12	11.427	1584	1588	1592	rBV	2332447	1972327	35.45%	5.300%
13	11.951	1672	1677	1681	rBV	112205	110669	1.99%	0.297%
14	12.410	1752	1755	1759	rBV	157572	145910	2.62%	0.392%
15	12.668	1793	1799	1804	rBV3	62939	68962	1.24%	0.185%
16	13.021	1854	1859	1862	rBV	6054854	5563300	100.00%	14.950%
17	13.498	1937	1940	1945	rVB	72583	72018	1.29%	0.194%
18	13.639	1961	1964	1967	rBV	220599	198937	3.58%	0.535%
19	13.768	1979	1986	1990	rBV9	52023	137521	2.47%	0.370%
20	13.927	2008	2013	2015	rBV2	50075	58718	1.06%	0.158%
21	13.992	2015	2024	2035	rVV5	236680	1079490	19.40%	2.901%
22	14.074	2035	2038	2054	rVB	1731756	1831107	32.91%	4.921%
23	14.551	2115	2119	2123	rVB	118309	110154	1.98%	0.296%
24	14.709	2144	2146	2154	rVB	47926	58645	1.05%	0.158%
25	14.862	2166	2172	2176	rVB4	65385	92715	1.67%	0.249%
26	15.009	2194	2197	2205	rVB3	60700	69829	1.26%	0.188%
27	15.209	2227	2231	2239	rVB	157789	188397	3.39%	0.506%
28	15.568	2286	2292	2296	rBV	1063581	1412182	25.38%	3.795%
29	15.603	2296	2298	2306	rVB	66874	81814	1.47%	0.220%
30	15.809	2329	2333	2338	rBV	124766	183956	3.31%	0.494%
31	16.056	2369	2375	2380	rBV	90898	147035	2.64%	0.395%
32	16.874	2510	2514	2522	rVB4	53295	102936	1.85%	0.277%




Sum of corrected areas: 37212976

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020321\
Data File : BF123102.D
Acq On : 3 Feb 2021 14:07
Operator : JU/CG
Sample : M1292-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
2021-01-28-FD04

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

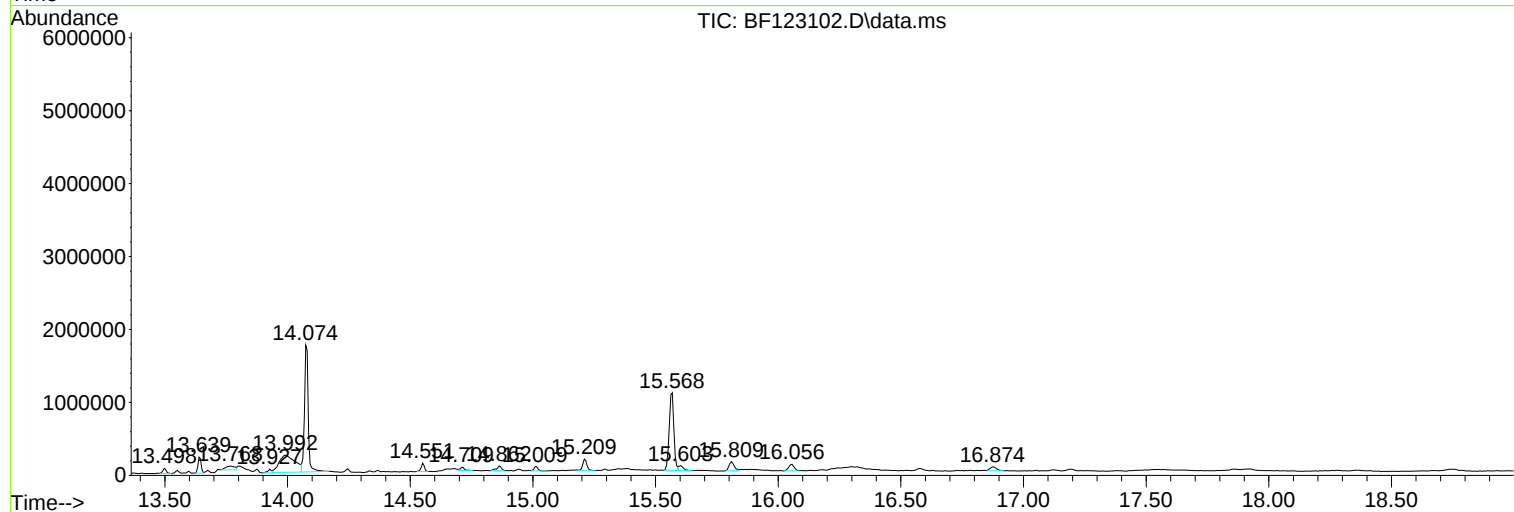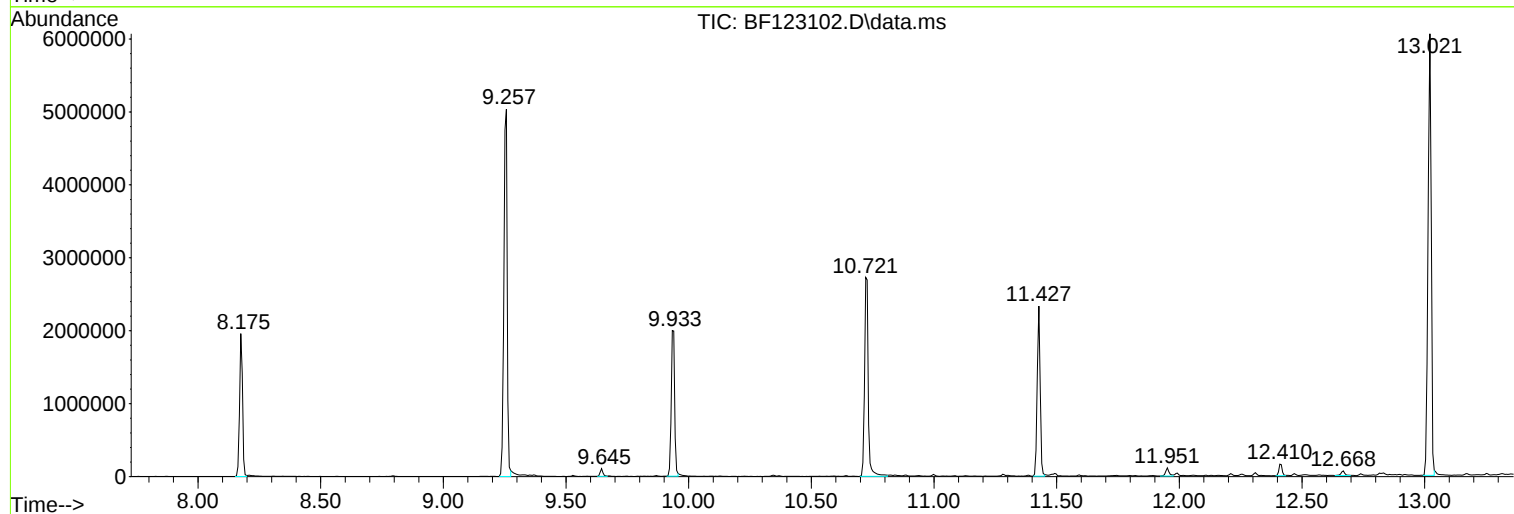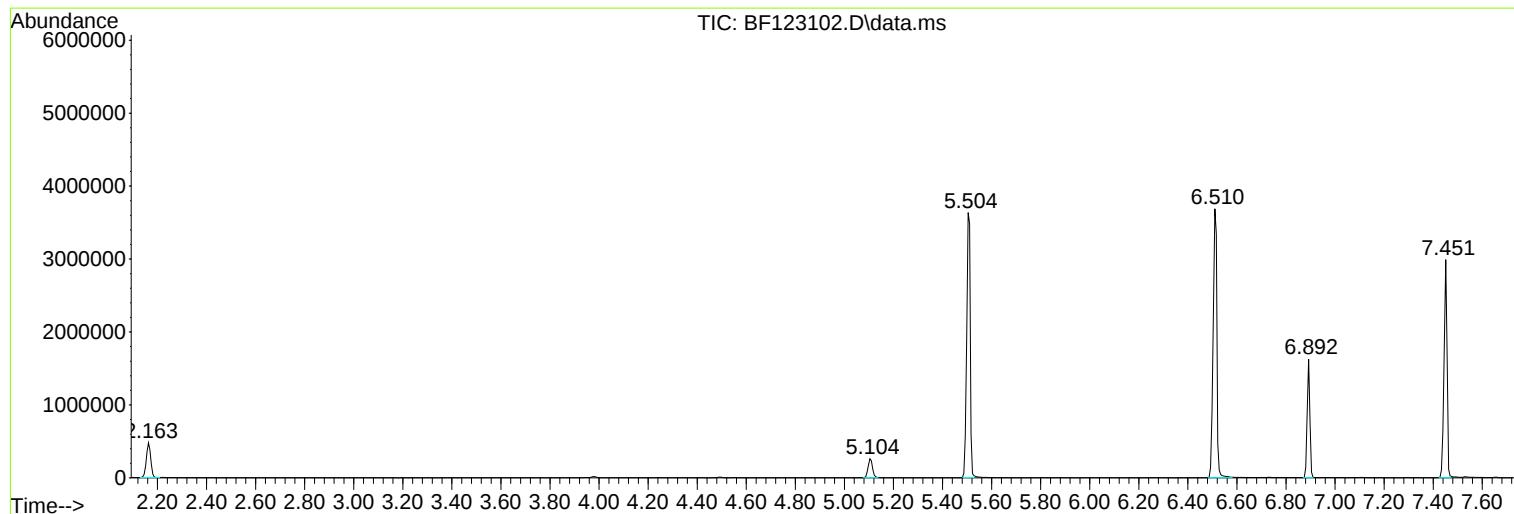

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020321\
Data File : BF123102.D
Acq On : 3 Feb 2021 14:07
Operator : JU/CG
Sample : M1292-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
2021-01-28-FD04

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020321\
Data File : BF123102.D
Acq On : 3 Feb 2021 14:07
Operator : JU/CG
Sample : M1292-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
2021-01-28-FD04

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------