

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020321\
 Data File : BF123103.D
 Acq On : 3 Feb 2021 14:39
 Operator : JU/CG
 Sample : M1292-08
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU421-003-1015

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF123103.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.169	8	14	19	rVB	551942	699730	11.41%	1.657%
2	5.510	577	582	585	rBV	4660752	4505970	73.50%	10.671%
3	6.516	747	753	756	rBV	4386632	4699200	76.65%	11.129%
4	6.892	813	817	820	rBV	1706285	1331023	21.71%	3.152%
5	7.451	907	912	915	rBV	3233180	3061059	49.93%	7.249%
6	8.175	1031	1035	1039	rBV	2129926	1753758	28.61%	4.153%
7	9.257	1214	1219	1222	rBV	5782197	5461614	89.08%	12.934%
8	9.645	1282	1285	1295	rBV	174174	176242	2.87%	0.417%
9	9.933	1330	1334	1338	rBV	2347796	2066621	33.71%	4.894%
10	10.727	1464	1469	1472	rBV	3953852	3722856	60.72%	8.817%
11	11.427	1584	1588	1591	rBV	2531032	2171833	35.42%	5.143%
12	11.957	1670	1678	1691	rBV	1101923	1093476	17.84%	2.590%
13	12.645	1791	1795	1796	rBV	77719	68558	1.12%	0.162%
14	12.663	1796	1798	1808	rVB4	68233	84987	1.39%	0.201%
15	12.745	1808	1812	1823	rBV	274101	335366	5.47%	0.794%
16	13.021	1854	1859	1862	rBV	6512541	6130916	100.00%	14.519%
17	13.927	2008	2013	2015	rBV3	46965	65889	1.07%	0.156%
18	13.998	2017	2025	2034	rVV4	243054	902282	14.72%	2.137%
19	14.074	2034	2038	2042	rVB	1820680	1800366	29.37%	4.264%
20	14.551	2114	2119	2122	rBV2	78503	86026	1.40%	0.204%
21	14.862	2170	2172	2176	rVB	60284	62604	1.02%	0.148%
22	14.945	2182	2186	2192	rBV	84147	93639	1.53%	0.222%
23	15.210	2228	2231	2237	rVB	95529	112818	1.84%	0.267%
24	15.562	2286	2291	2296	rBV	1132416	1545640	25.21%	3.660%
25	15.604	2296	2298	2304	rVB2	72721	81342	1.33%	0.193%
26	16.057	2370	2375	2380	rVB	75358	111662	1.82%	0.264%




Sum of corrected areas: 42225477

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020321\
Data File : BF123103.D
Acq On : 3 Feb 2021 14:39
Operator : JU/CG
Sample : M1292-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU421-003-1015

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

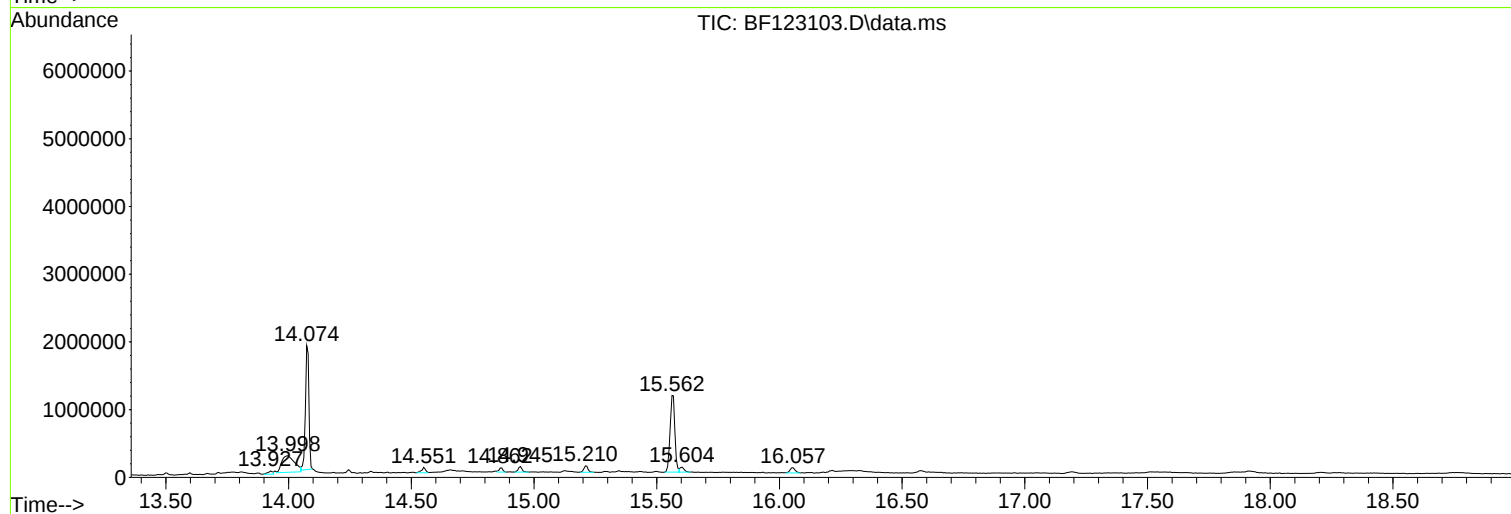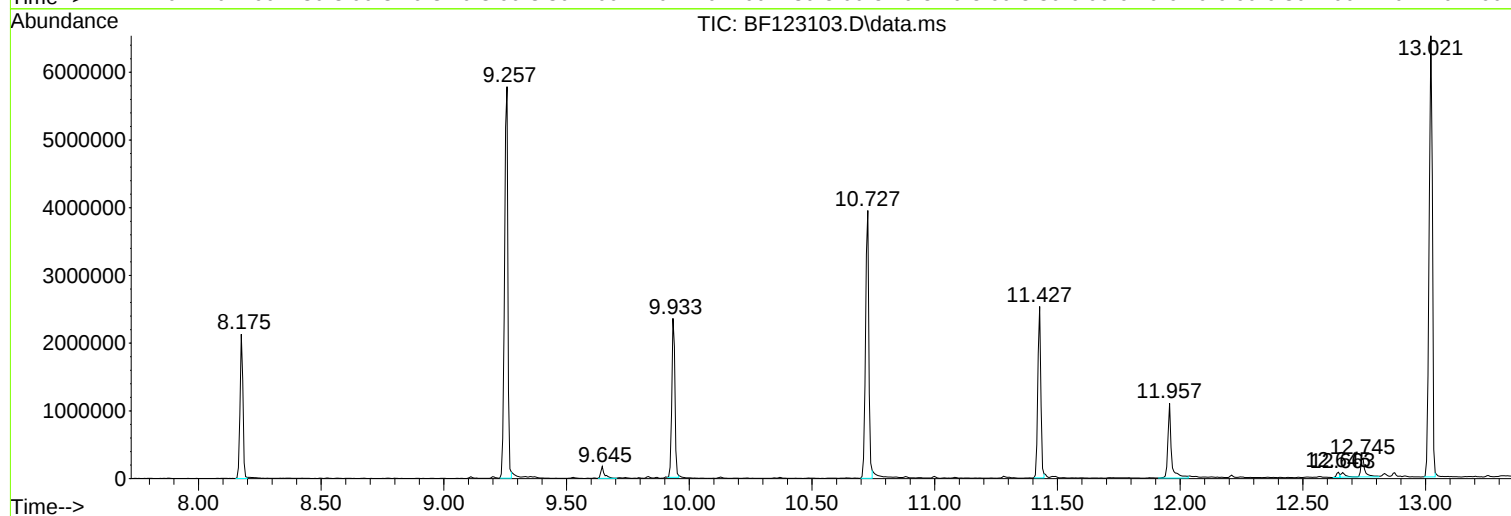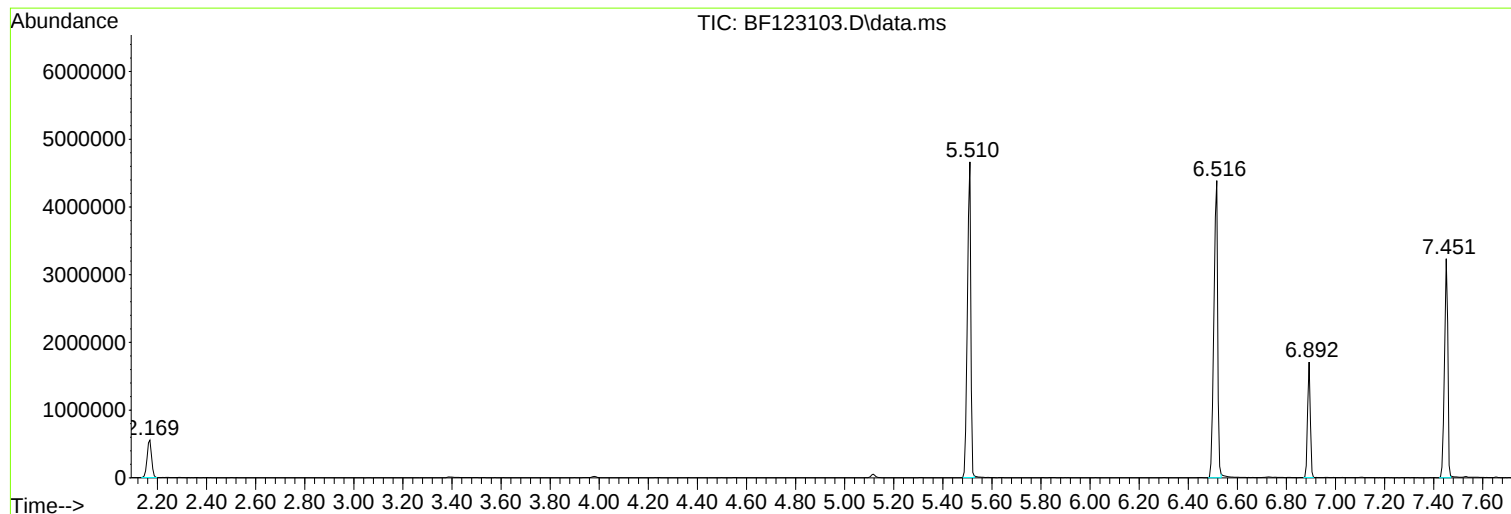

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020321\
Data File : BF123103.D
Acq On : 3 Feb 2021 14:39
Operator : JU/CG
Sample : M1292-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU421-003-1015

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020321\
Data File : BF123103.D
Acq On : 3 Feb 2021 14:39
Operator : JU/CG
Sample : M1292-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU421-003-1015

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc