

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020321\
 Data File : BF123104.D
 Acq On : 3 Feb 2021 15:14
 Operator : JU/CG
 Sample : M1292-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU421-003-0510

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF123104.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.157	5	12	18	rBV	602563	771187	11.92%	1.844%
2	5.116	510	515	521	rVB	63207	80646	1.25%	0.193%
3	5.510	576	582	585	rBV	4561120	4656495	72.00%	11.134%
4	6.516	747	753	756	rBV	4387151	4727367	73.09%	11.303%
5	6.892	813	817	820	rBV	1634523	1253631	19.38%	2.997%
6	7.451	907	912	915	rBV	3309770	3053842	47.22%	7.302%
7	8.175	1031	1035	1038	rBV	2046244	1649755	25.51%	3.945%
8	9.257	1214	1219	1222	rBV	5920398	5543641	85.71%	13.255%
9	9.645	1281	1285	1289	rBV	180052	148174	2.29%	0.354%
10	9.933	1330	1334	1338	rBV	2212006	1949579	30.14%	4.662%
11	10.728	1464	1469	1472	rBV	3983109	3689273	57.04%	8.821%
12	11.427	1584	1588	1591	rBV	2430760	2031940	31.42%	4.858%
13	11.957	1671	1678	1690	rBV	627164	694325	10.74%	1.660%
14	12.645	1791	1795	1802	rBV	51628	65517	1.01%	0.157%
15	12.739	1808	1811	1819	rBV	125403	147313	2.28%	0.352%
16	13.021	1854	1859	1862	rBV	6807737	6467725	100.00%	15.465%
17	13.998	2017	2025	2033	rBV3	177412	655735	10.14%	1.568%
18	14.074	2034	2038	2042	rVB	1774539	1718735	26.57%	4.110%
19	14.551	2114	2119	2124	rBV2	65346	81524	1.26%	0.195%
20	14.939	2182	2185	2193	rVB	93648	103972	1.61%	0.249%
21	15.210	2227	2231	2235	rBV	104301	118271	1.83%	0.283%
22	15.562	2286	2291	2296	rBV	1144950	1484624	22.95%	3.550%
23	15.604	2296	2298	2305	rVB2	64460	72046	1.11%	0.172%
24	16.051	2369	2374	2380	rVB	74585	118606	1.83%	0.284%
25	16.204	2395	2400	2406	rBV	148049	245729	3.80%	0.588%
26	17.909	2687	2690	2700	rVB5	62598	132625	2.05%	0.317%
27	18.292	2747	2755	2761	rBV8	56522	160375	2.48%	0.383%




Sum of corrected areas: 41822652

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020321\
Data File : BF123104.D
Acq On : 3 Feb 2021 15:14
Operator : JU/CG
Sample : M1292-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU421-003-0510

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

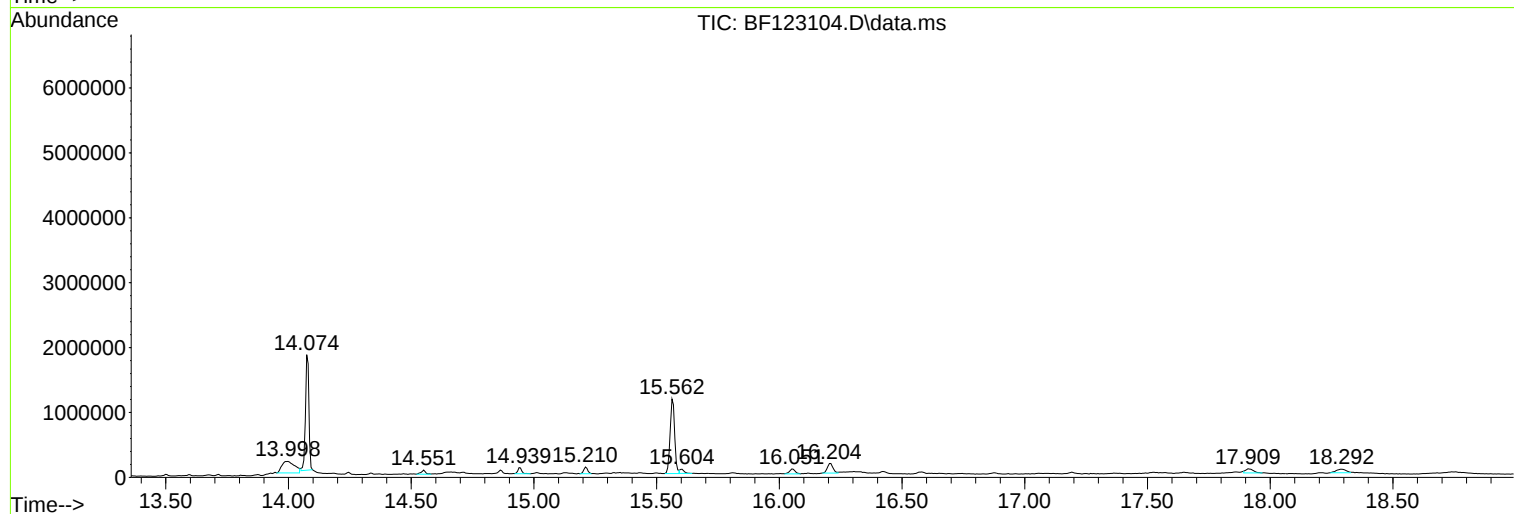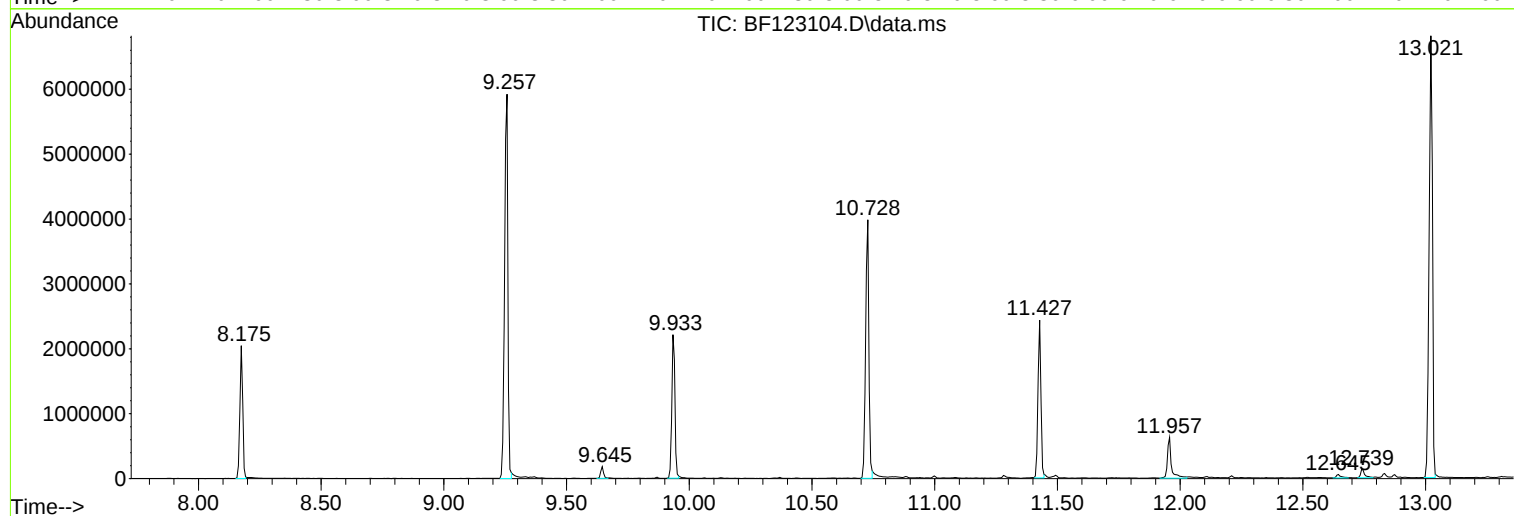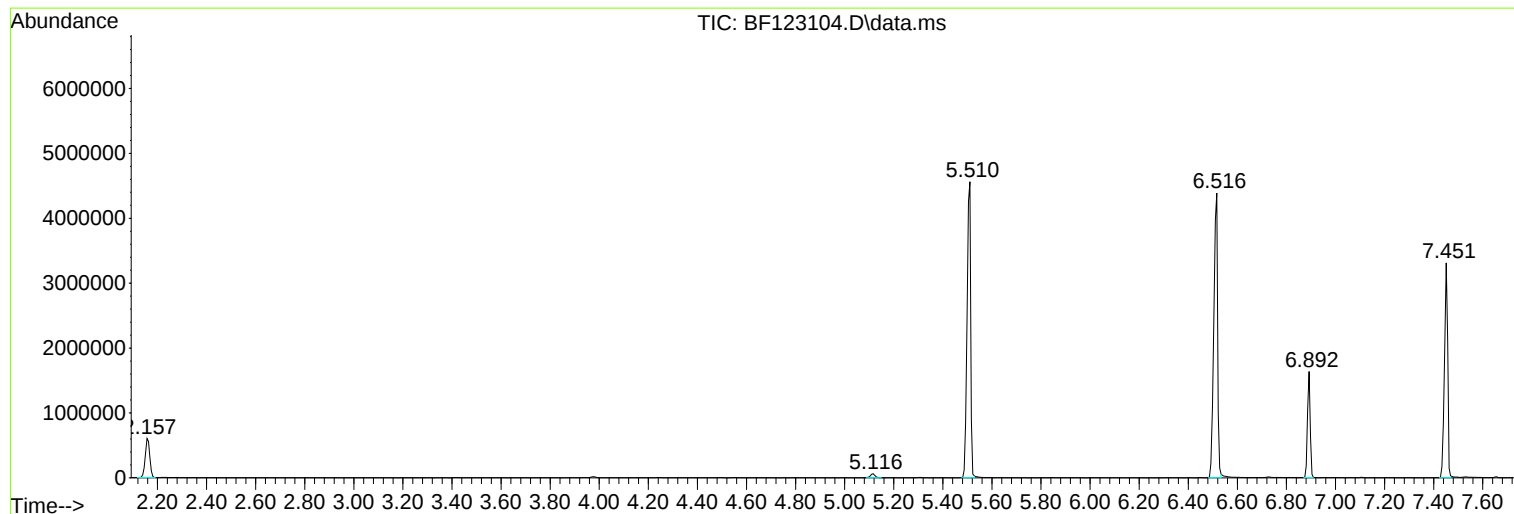

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020321\
Data File : BF123104.D
Acq On : 3 Feb 2021 15:14
Operator : JU/CG
Sample : M1292-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU421-003-0510

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020321\
Data File : BF123104.D
Acq On : 3 Feb 2021 15:14
Operator : JU/CG
Sample : M1292-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU421-003-0510

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------