
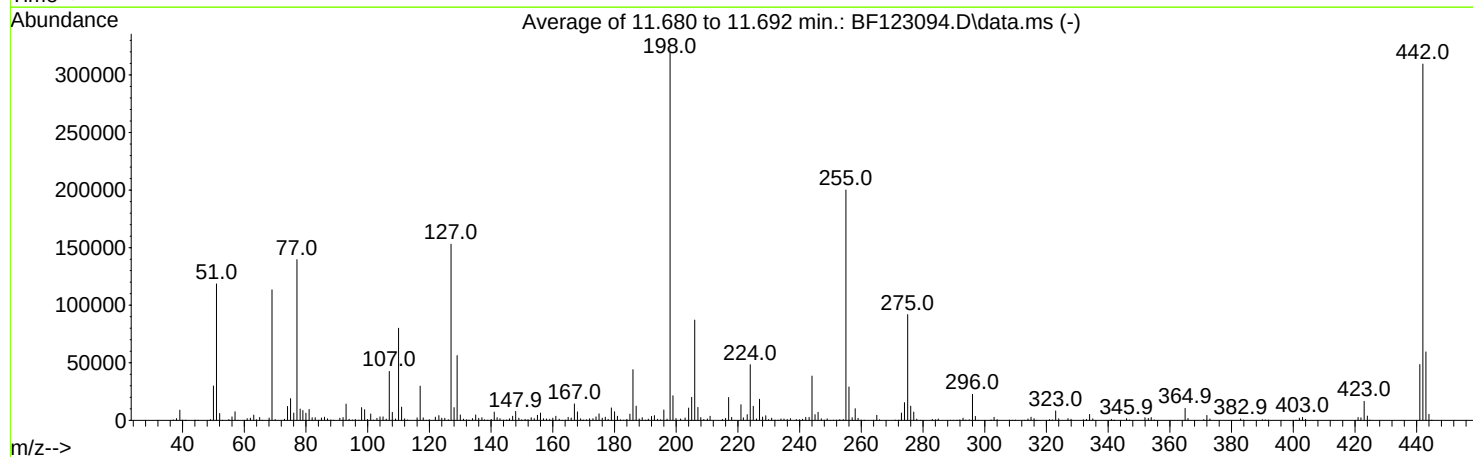


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020321\
 Data File : BF123094.D
 Acq On : 3 Feb 2021 9:33
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 29 12:29:00 2021

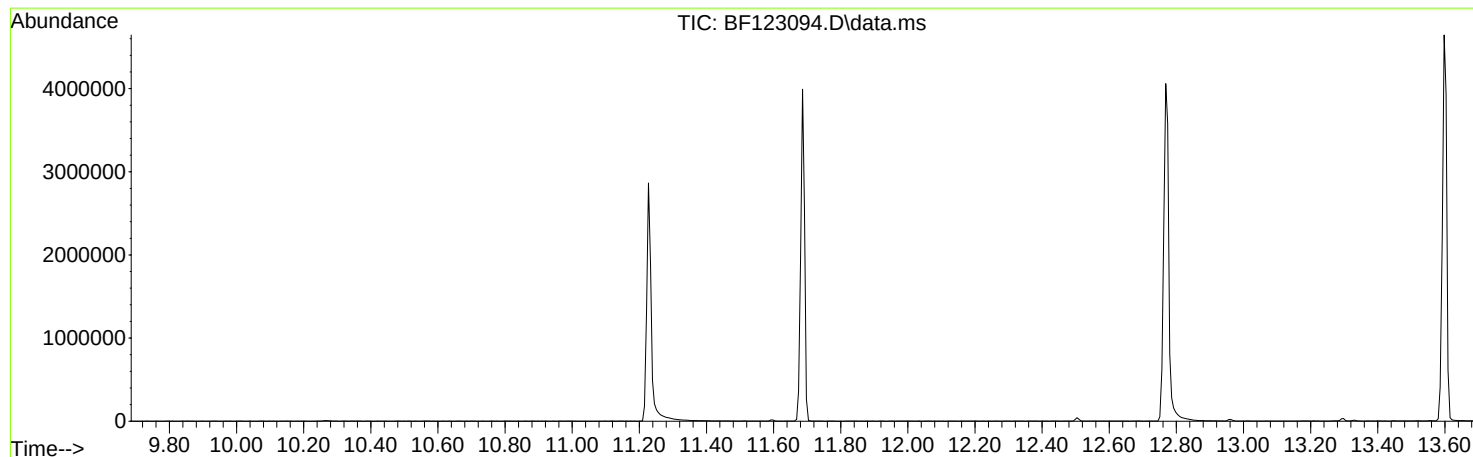

AutoFind: Scans 1631, 1632, 1633; Background Corrected with Scan 1626

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.1	118587	PASS
68	69	0.00	2	1.8	2061	PASS
69	198	0.00	100	35.5	113347	PASS
70	69	0.00	2	0.6	666	PASS
127	198	10	80	47.9	152949	PASS
197	198	0.00	2	0.4	1179	PASS
198	198	100	100	100.0	319467	PASS
199	198	5	9	6.7	21422	PASS
275	198	10	60	28.8	91923	PASS
365	198	1	100	3.3	10442	PASS
441	198	0.01	100	15.2	48531	PASS
442	442	50	100	100.0	309501	PASS
443	442	15	24	19.2	59456	PASS

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/3/2021	BNA_F	<u>BF123094.D</u>
Compound Name	Response	Retention Time
DDT	841305	13.598
DDD	9060	13.298
DDE	3447	12.957
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12507	853812	1.46

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020321\
 Data File : BF123094.D
 Acq On : 3 Feb 2021 9:33
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Feb 04 02:00:41 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 29 12:29:00 2021
 Response via : Initial Calibration

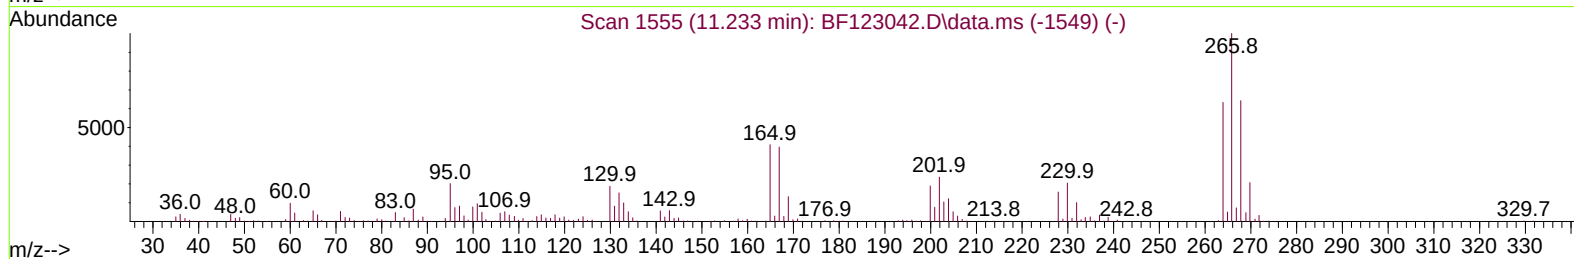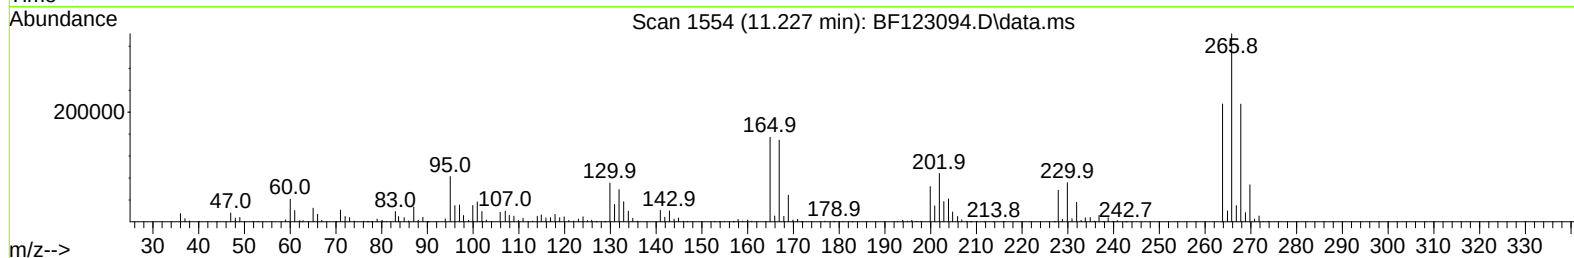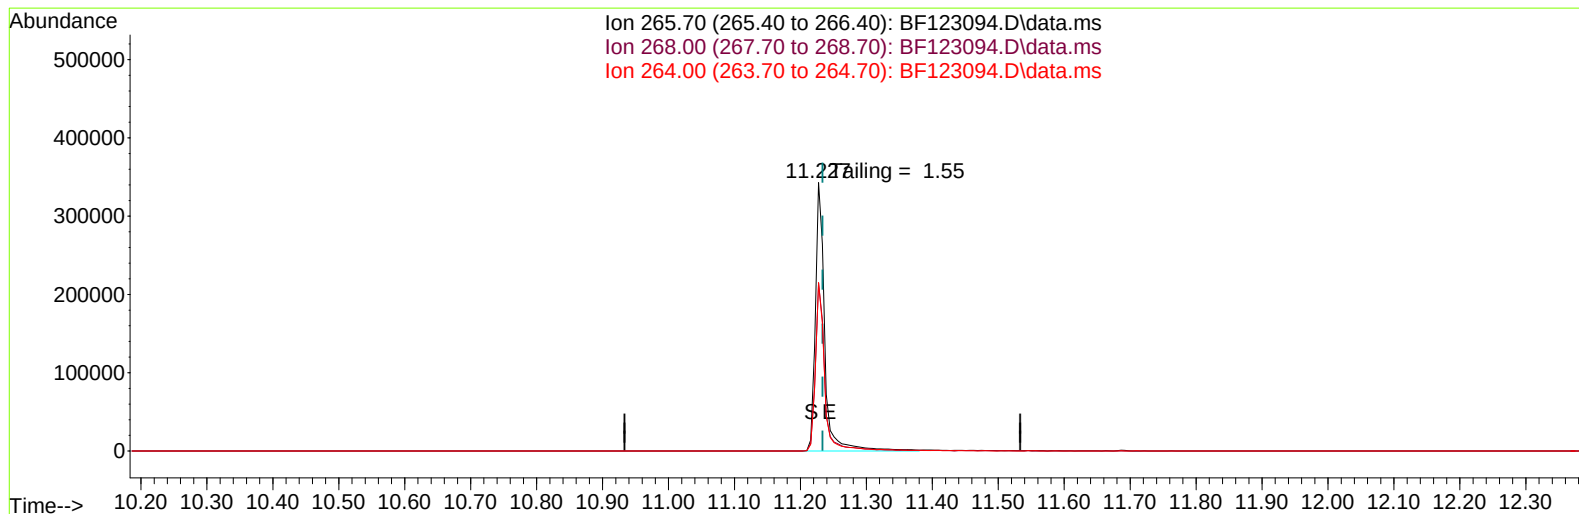

TIC: BF123094.D\data.ms

(70) Pentachlorophenol (C)

11.227min (-0.006) 33760.42 ng




response 338660

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.57
264.00	62.30	62.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020321\
Data File : BF123094.D
Acq On : 3 Feb 2021 9:33
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 04 02:00:41 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 29 12:29:00 2021
Response via : Initial Calibration

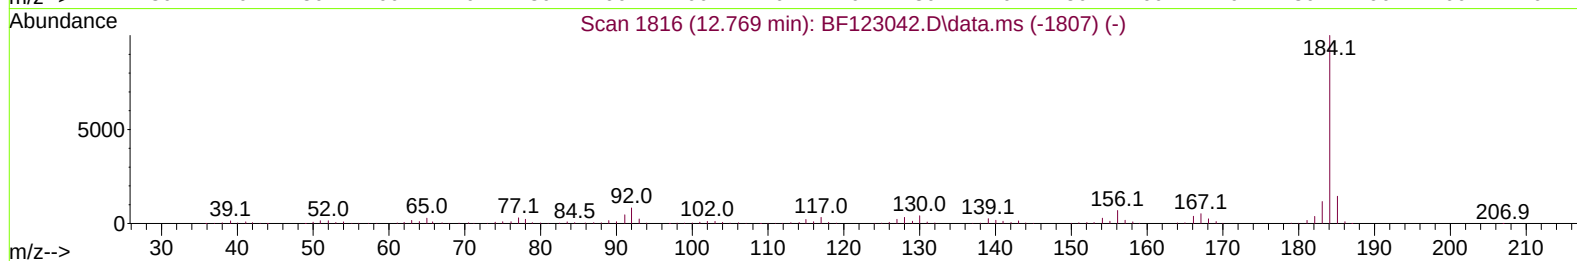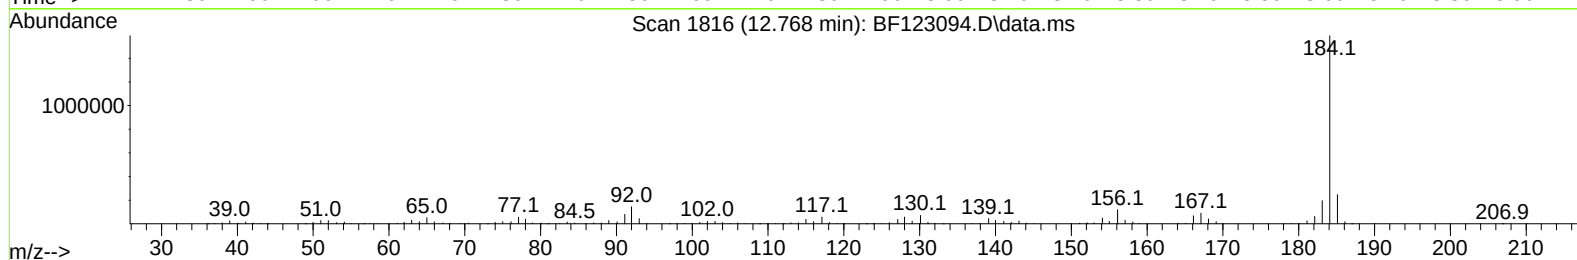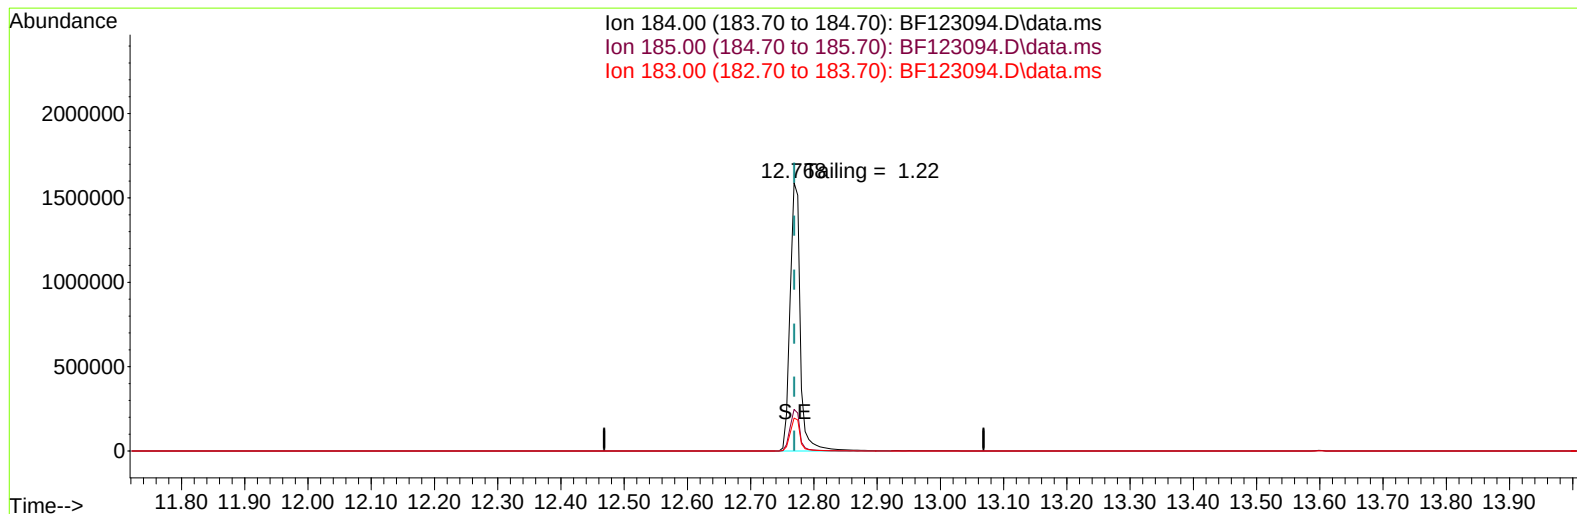

TIC: BF123094.D\data.ms

(77) Benzidine

12.768min (-0.000) 0.00 ng

response 1790154

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	15.53
183.00	12.10	12.29
0.00	0.00	0.00