
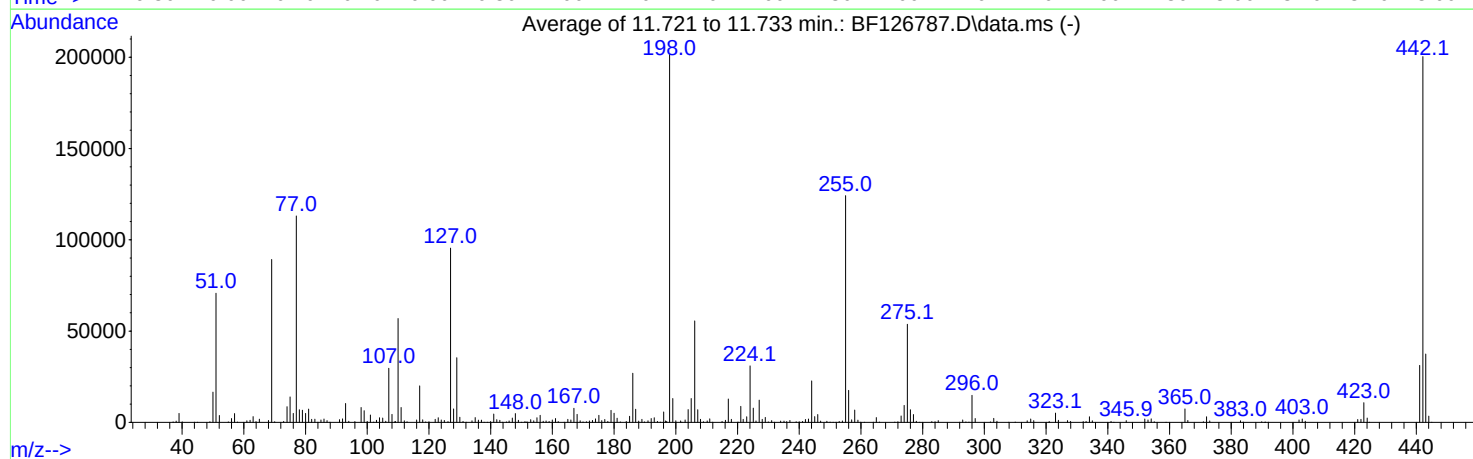


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020322\
 Data File : BF126787.D
 Acq On : 03 Feb 2022 09:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 02 15:08:47 2022

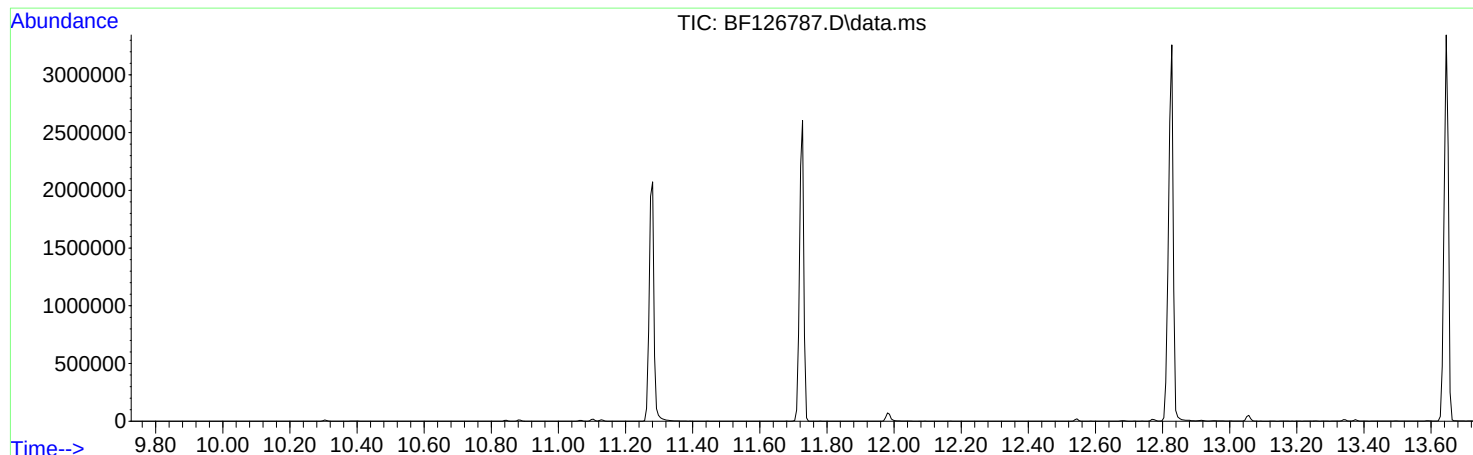

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	70765	PASS
68	69	0.00	2	1.2	1098	PASS
69	198	0.00	100	44.3	89205	PASS
70	69	0.00	2	0.4	345	PASS
127	198	10	80	47.3	95408	PASS
197	198	0.00	2	0.4	767	PASS
198	198	100	100	100.0	201496	PASS
199	198	5	9	6.5	13027	PASS
275	198	10	60	26.7	53763	PASS
365	198	1	100	3.6	7354	PASS
441	198	0.01	100	15.5	31165	PASS
442	442	50	100	100.0	200341	PASS
443	442	15	24	18.7	37429	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/3/2022	BNA_F	<u>BF126787.D</u>
Compound Name	Response	Retention Time
DDT	581362	13.64
DDD	3385	13.34
DDE	125	13.05
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3510	584872	0.60

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020322\
Data File : BF126787.D
Acq On : 03 Feb 2022 09:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 03 11:28:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 02 15:08:47 2022
Response via : Initial Calibration

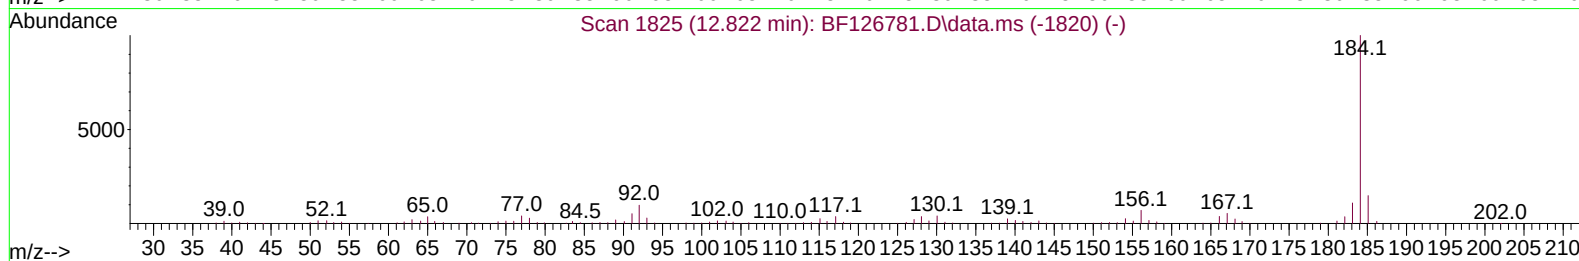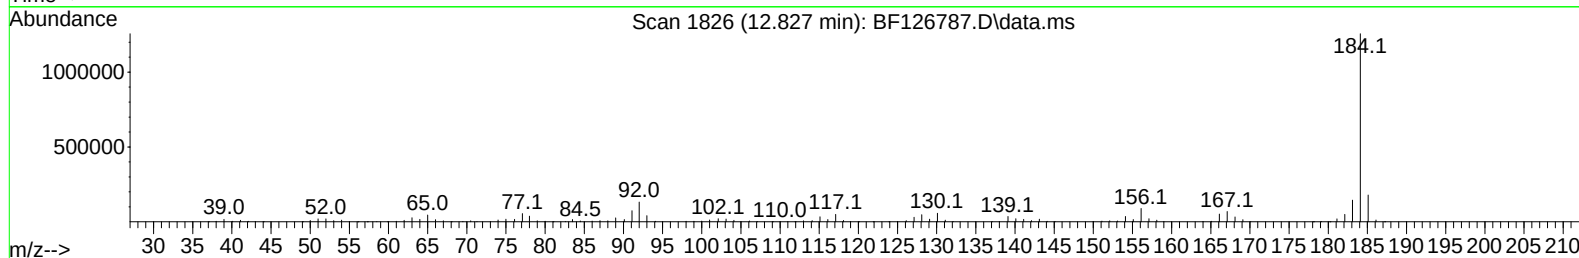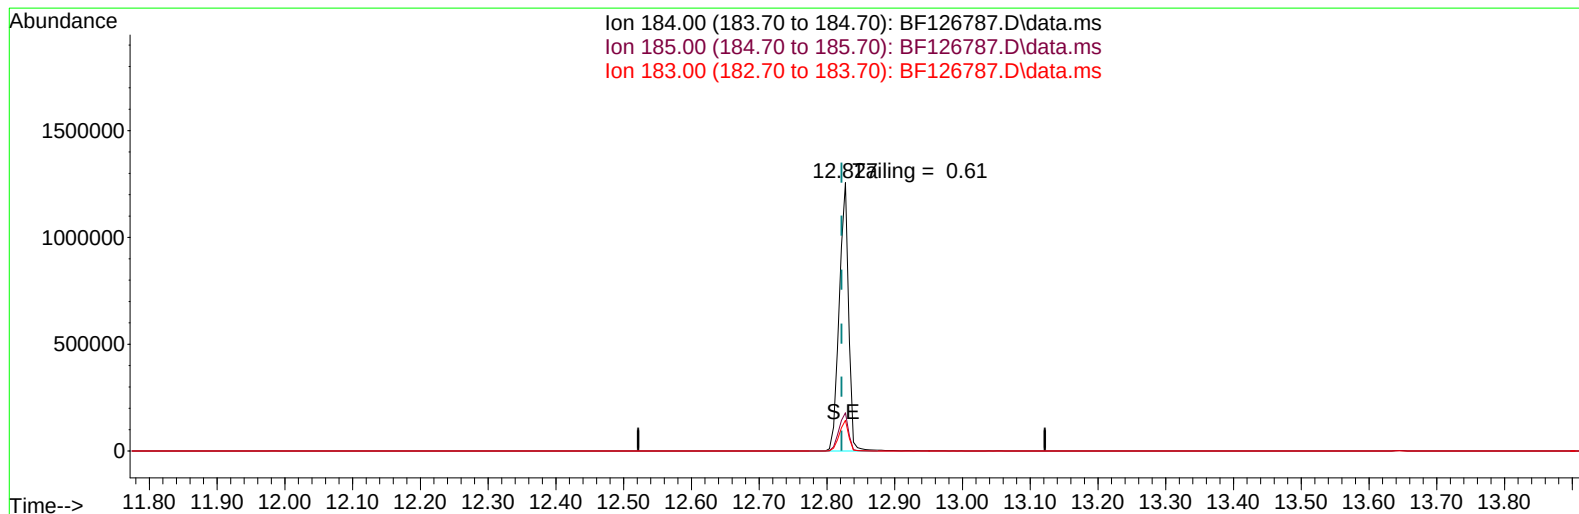

TIC: BF126787.D\data.ms

(77) Benzidine

12.827min (+ 0.006) 0.00 ng




response 1208717

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.27
183.00	10.20	11.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020322\
Data File : BF126787.D
Acq On : 03 Feb 2022 09:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 03 11:28:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 02 15:08:47 2022
Response via : Initial Calibration

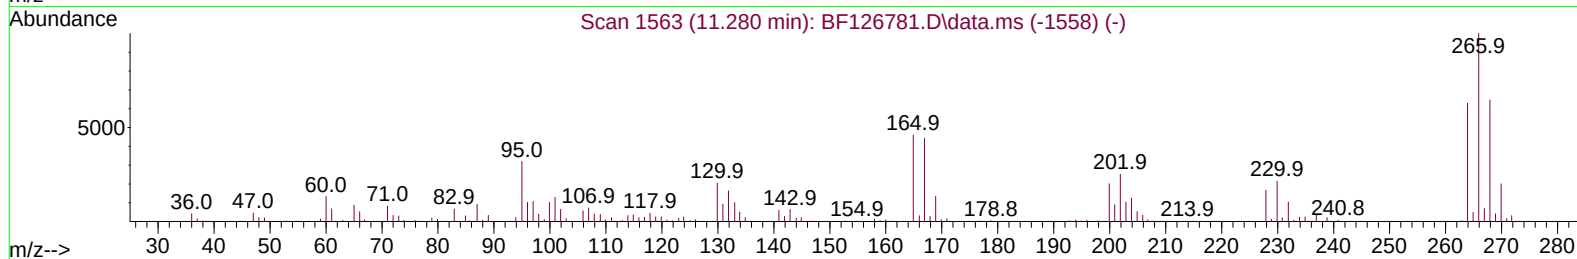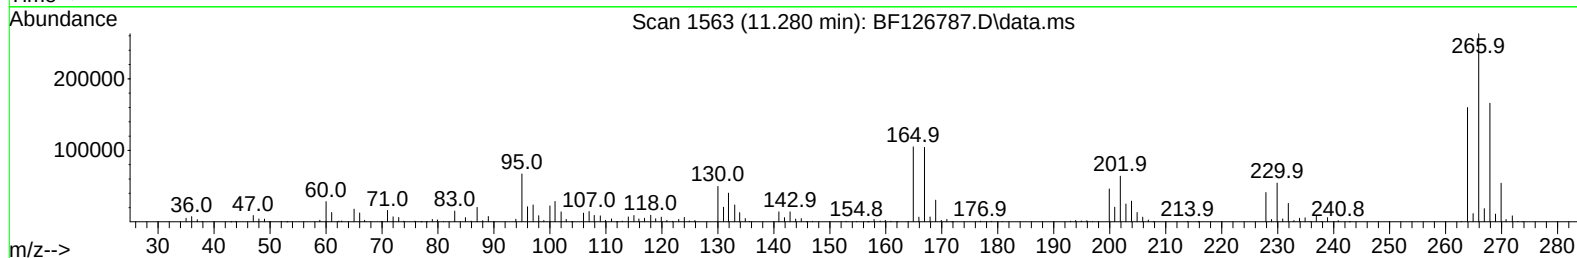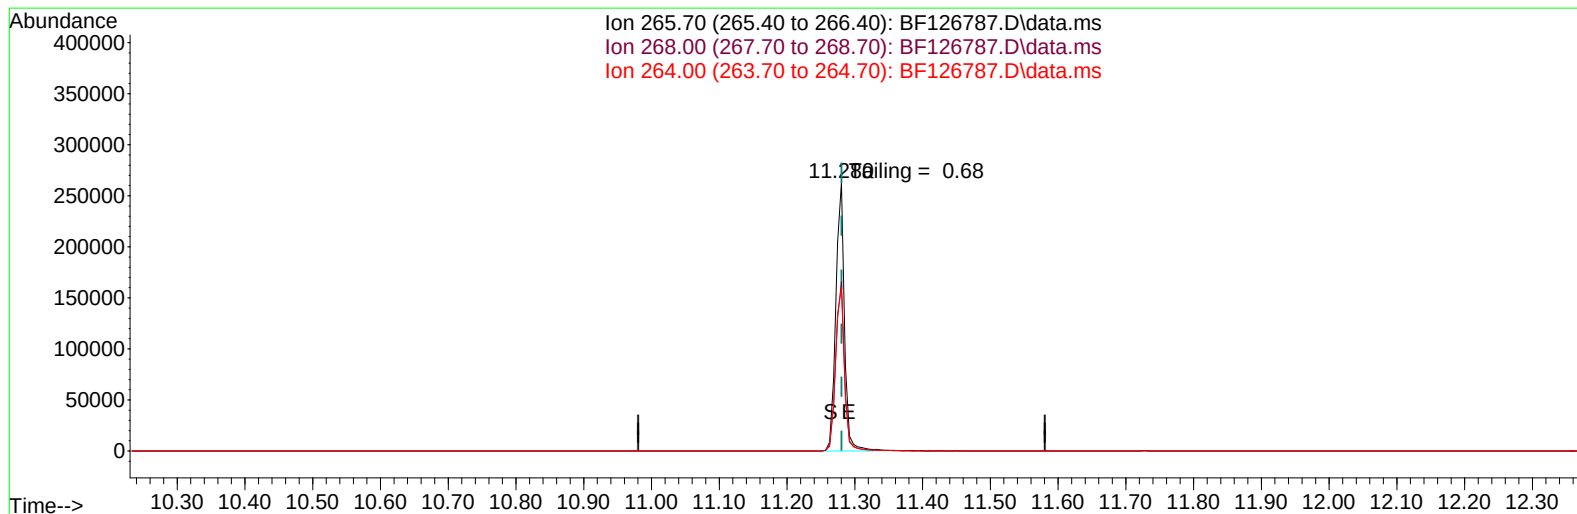

TIC: BF126787.D\data.ms

(70) Pentachlorophenol (C)

11.280min (-0.000) 36923.28 ng

response 236619

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	63.07
264.00	63.00	60.78
0.00	0.00	0.00