
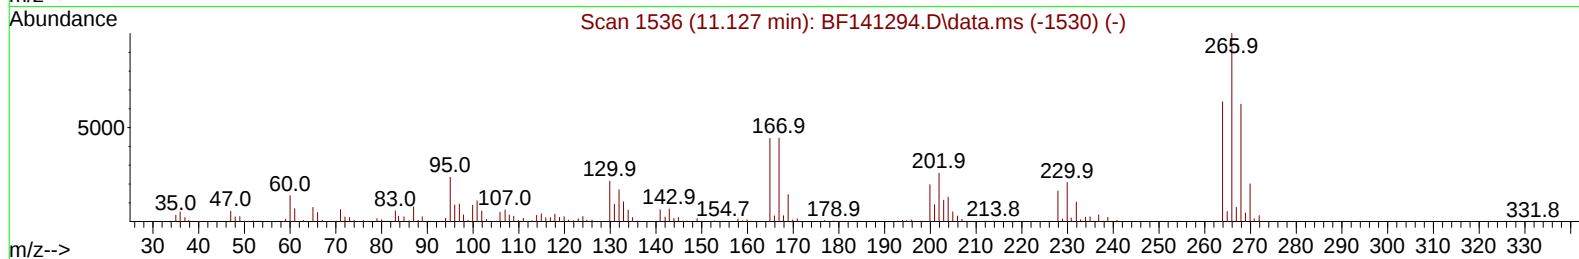
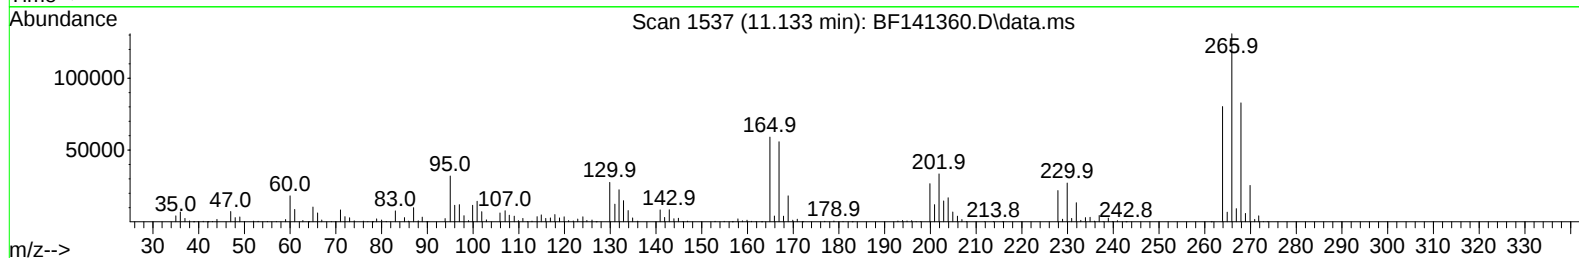


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020325\
Data File : BF141360.D
Acq On : 03 Feb 2025 09:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 03 12:16:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 29 17:41:25 2025
Response via : Initial Calibration

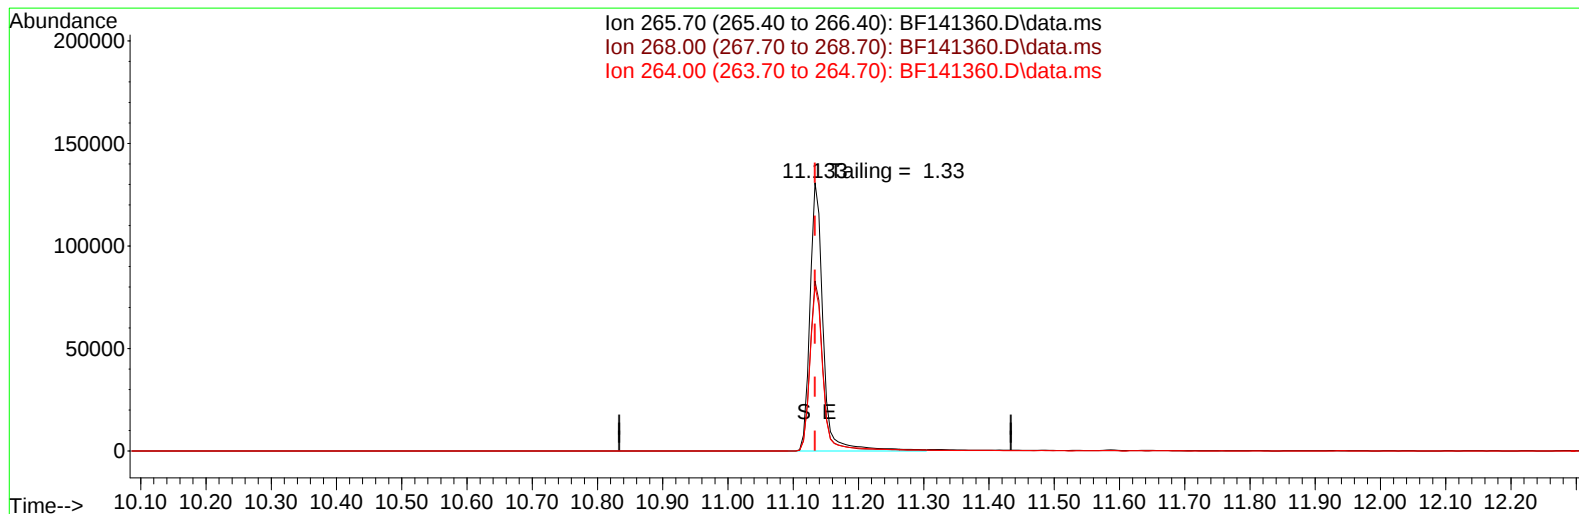

TIC: BF141360.D\data.ms

(70) Pentachlorophenol (C)




11.133min (-0.000) 6278.82 ng

response 185394

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	63.32
264.00	63.70	61.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020325\
Data File : BF141360.D
Acq On : 03 Feb 2025 09:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 03 12:16:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 29 17:41:25 2025
Response via : Initial Calibration

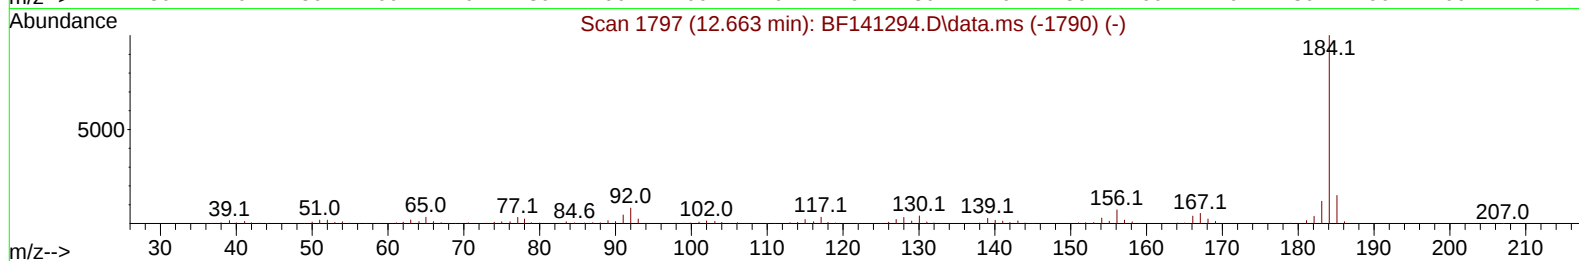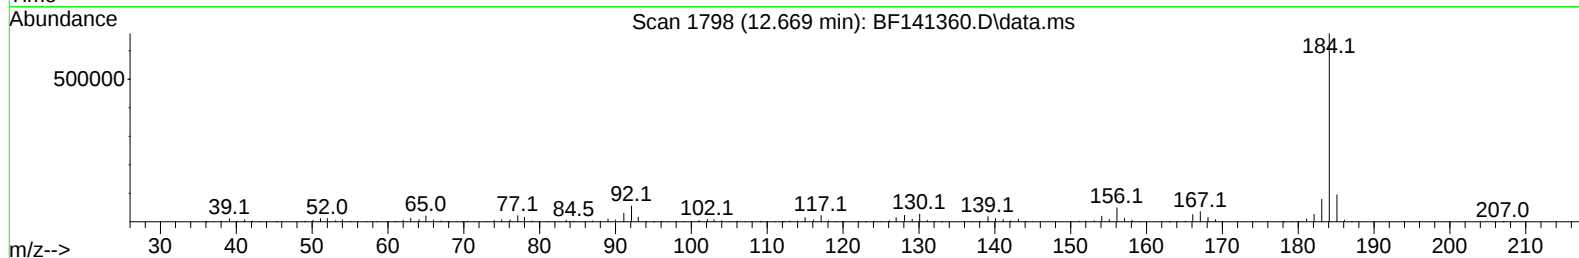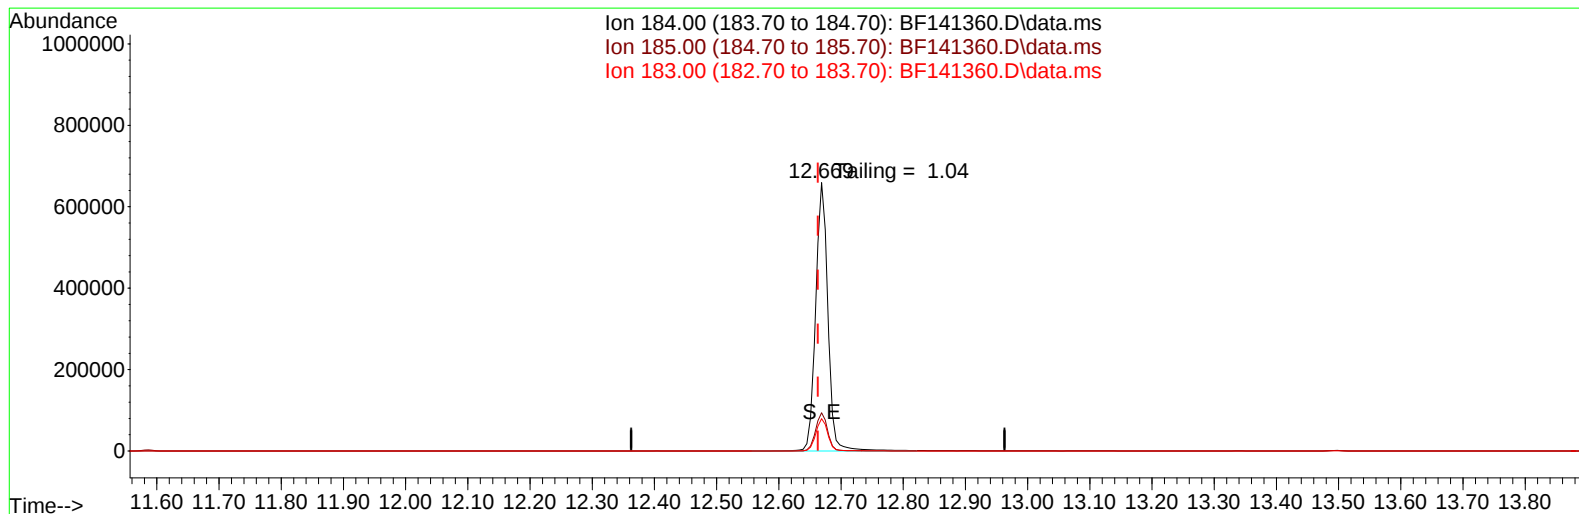

TIC: BF141360.D\data.ms

(77) Benzidine**12.669min (+ 0.006) 7483.96 ng****response 909791**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.28
183.00	11.90	12.04
0.00	0.00	0.00