
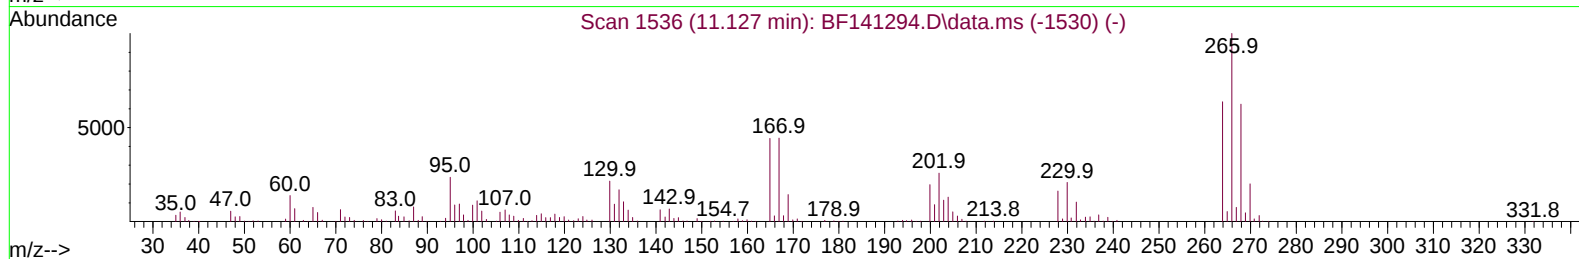
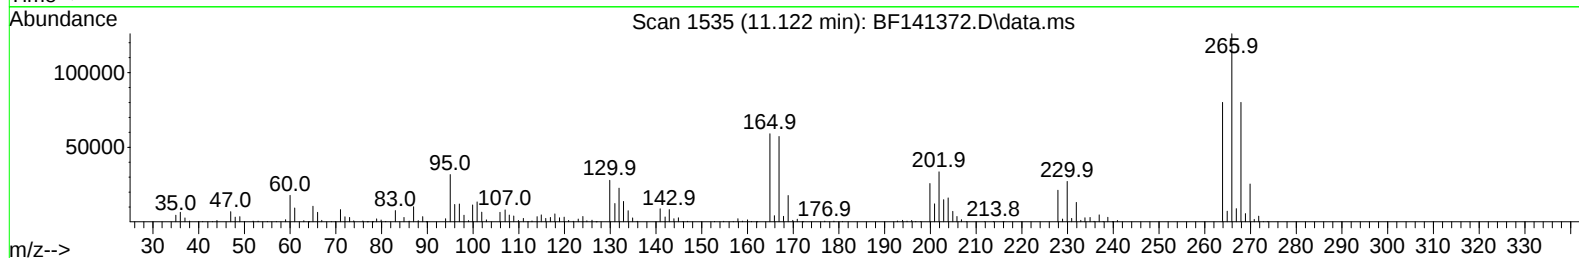


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020325\
Data File : BF141372.D
Acq On : 03 Feb 2025 16:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 04 05:08:05 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 29 17:41:25 2025
Response via : Initial Calibration

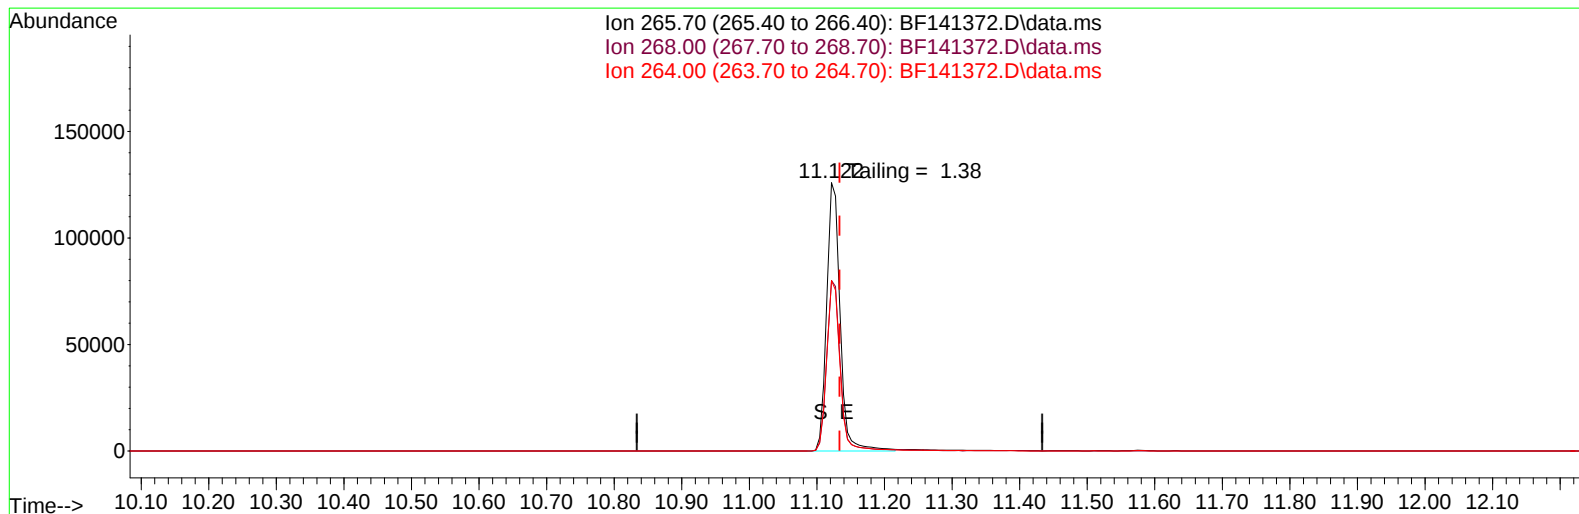

TIC: BF141372.D\data.ms

(70) Pentachlorophenol (C)




11.122min (-0.012) 6372.12 ng

response 175387

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	63.54
264.00	63.70	63.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020325\
Data File : BF141372.D
Acq On : 03 Feb 2025 16:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 04 05:08:05 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 29 17:41:25 2025
Response via : Initial Calibration

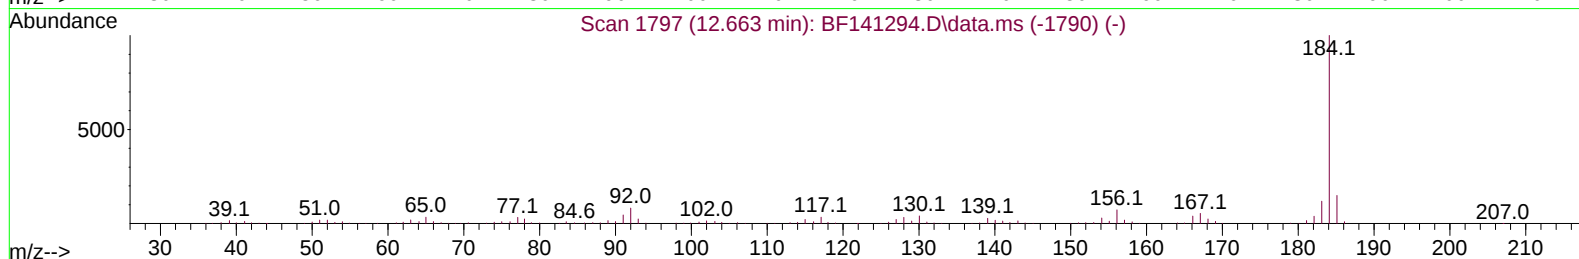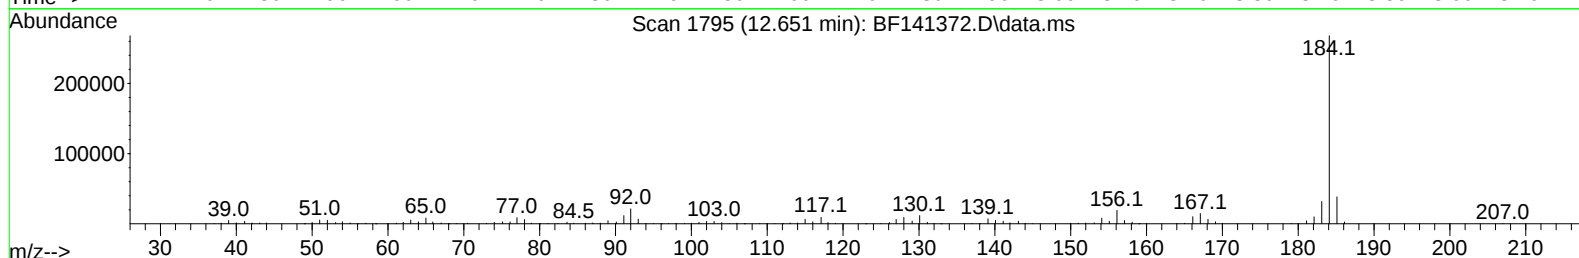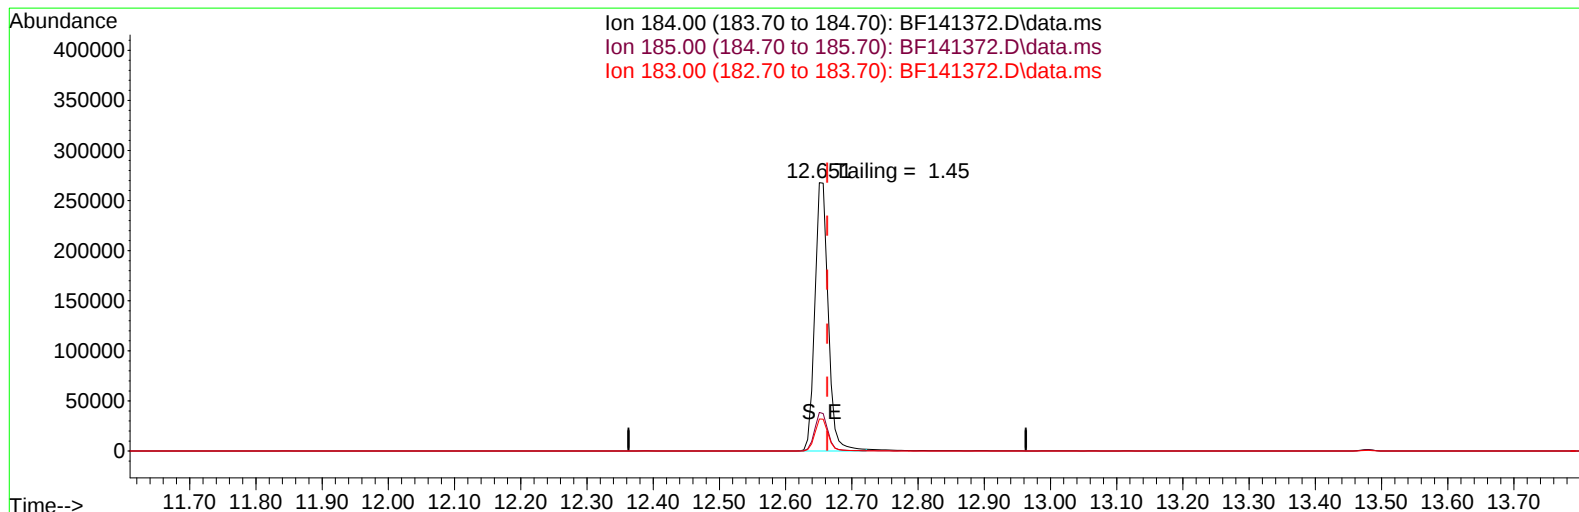

TIC: BF141372.D\data.ms

(77) Benzidine

12.651min (-0.012) 4251.31 ng

response 379432

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	14.90	14.36
--------	-------	-------

183.00	11.90	11.93
--------	-------	-------

0.00 0.00 0.00