

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020325\
 Data File : BF141365.D
 Acq On : 03 Feb 2025 13:10
 Operator : RC/JU
 Sample : PB166468BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB166468BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141365.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.857	293	300	311	rVB	53919	89300	1.99%	0.403%
2	5.422	561	566	586	rBV	1825193	2405070	53.62%	10.859%
3	6.434	732	738	761	rBV	1821513	2469762	55.06%	11.151%
4	6.792	794	799	805	rBV	521130	643391	14.34%	2.905%
5	7.357	888	895	900	rBV	1607478	2236607	49.86%	10.099%
6	8.075	1011	1017	1028	rBV	608376	783243	17.46%	3.536%
7	9.151	1193	1200	1205	rBV	2890924	3855767	85.96%	17.410%
8	9.827	1309	1315	1329	rVB	699268	892956	19.91%	4.032%
9	10.622	1444	1450	1470	rBV	1181659	1582714	35.28%	7.146%
10	11.316	1563	1568	1575	rBV	775755	962175	21.45%	4.344%
11	12.910	1832	1839	1844	rBV	3211143	4485571	100.00%	20.253%
12	13.957	2011	2017	2027	rBV	725435	937284	20.90%	4.232%
13	15.415	2259	2265	2279	rVB	505100	803625	17.92%	3.629%




Sum of corrected areas: 22147465

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020325\
Data File : BF141365.D
Acq On : 03 Feb 2025 13:10
Operator : RC/JU
Sample : PB166468BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166468BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

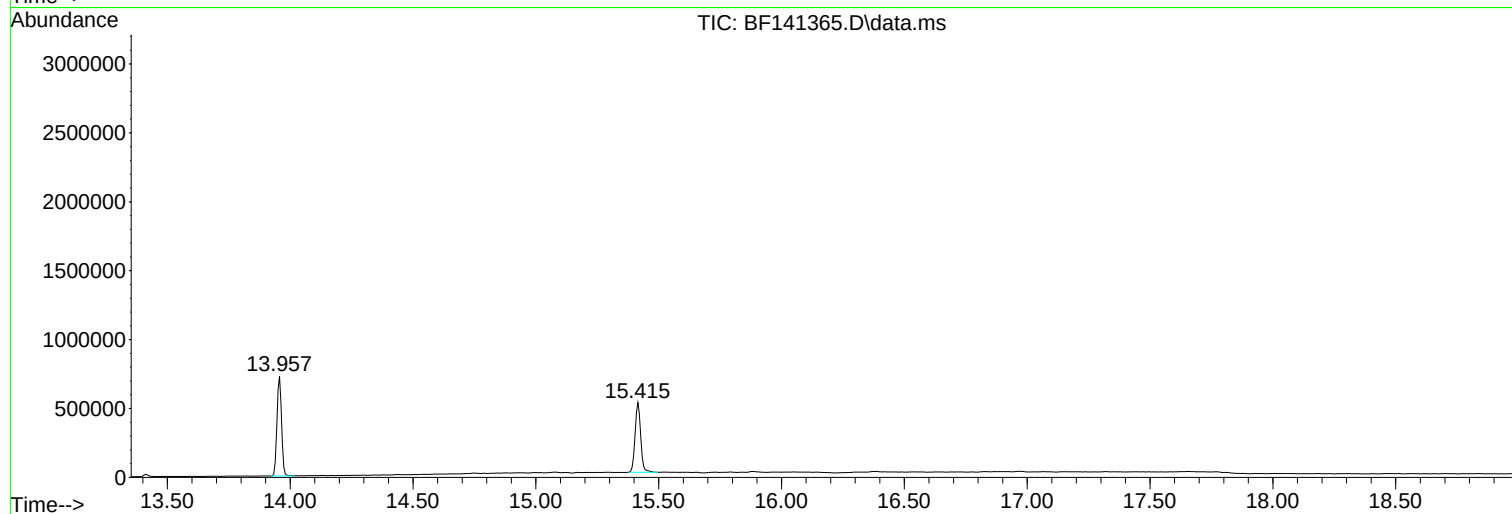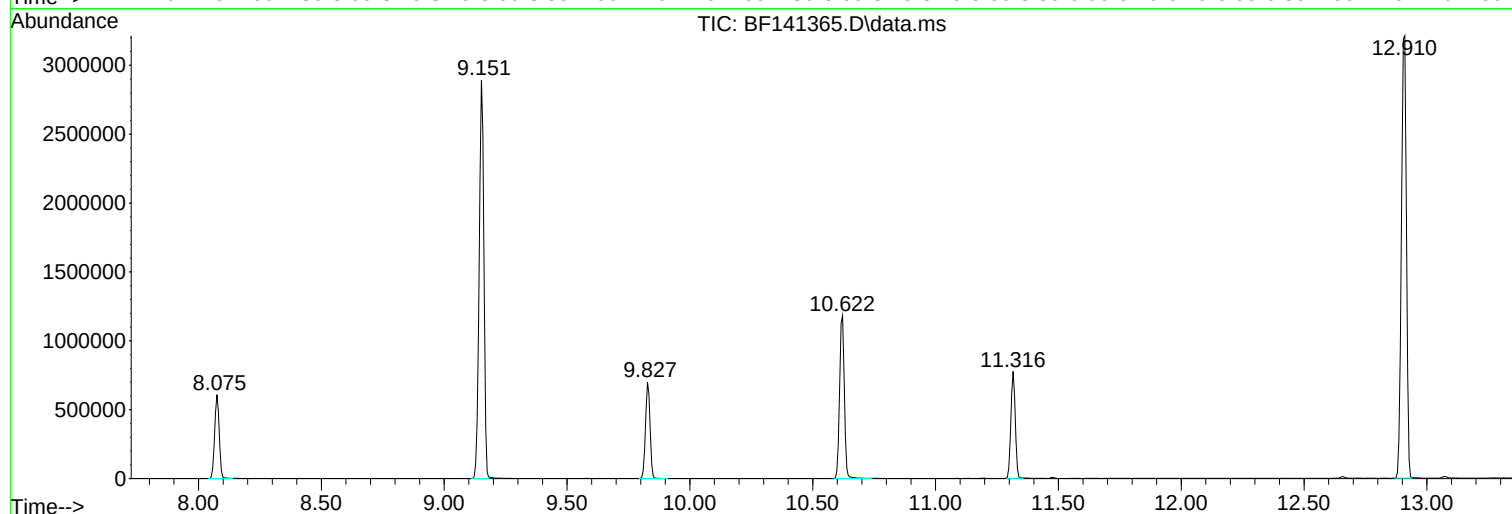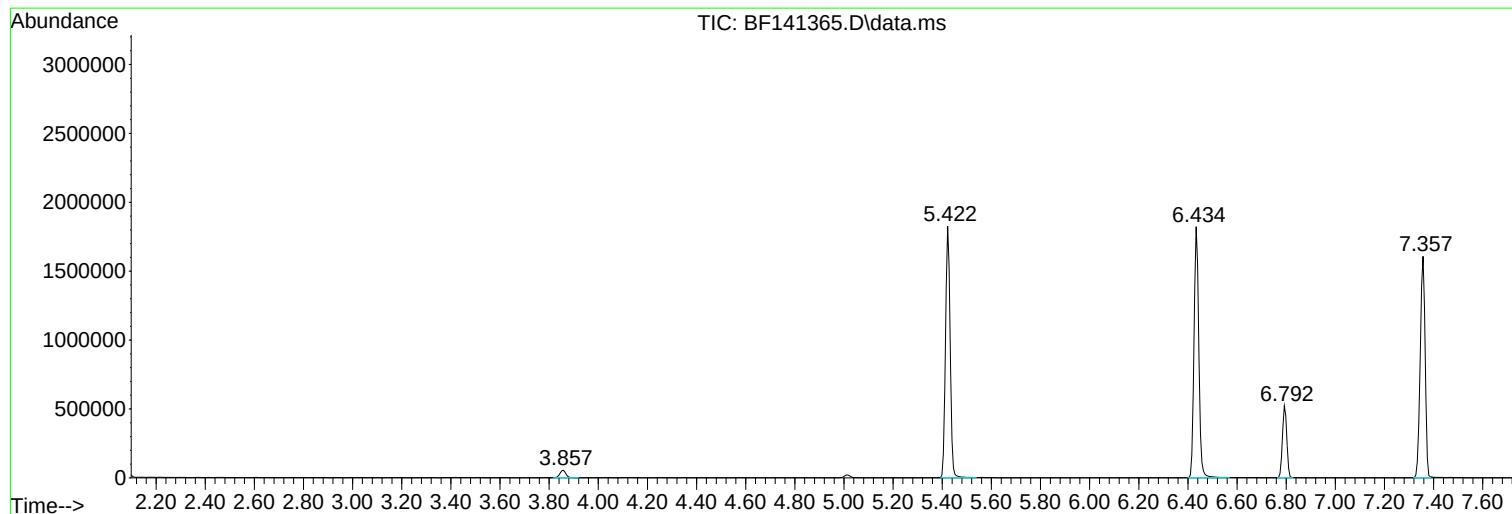

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020325\
Data File : BF141365.D
Acq On : 03 Feb 2025 13:10
Operator : RC/JU
Sample : PB166468BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166468BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020325\
Data File : BF141365.D
Acq On : 03 Feb 2025 13:10
Operator : RC/JU
Sample : PB166468BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166468BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------