


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020325\
Data File : BF141360.D
Acq On : 03 Feb 2025 09:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jan 29 17:41:25 2025

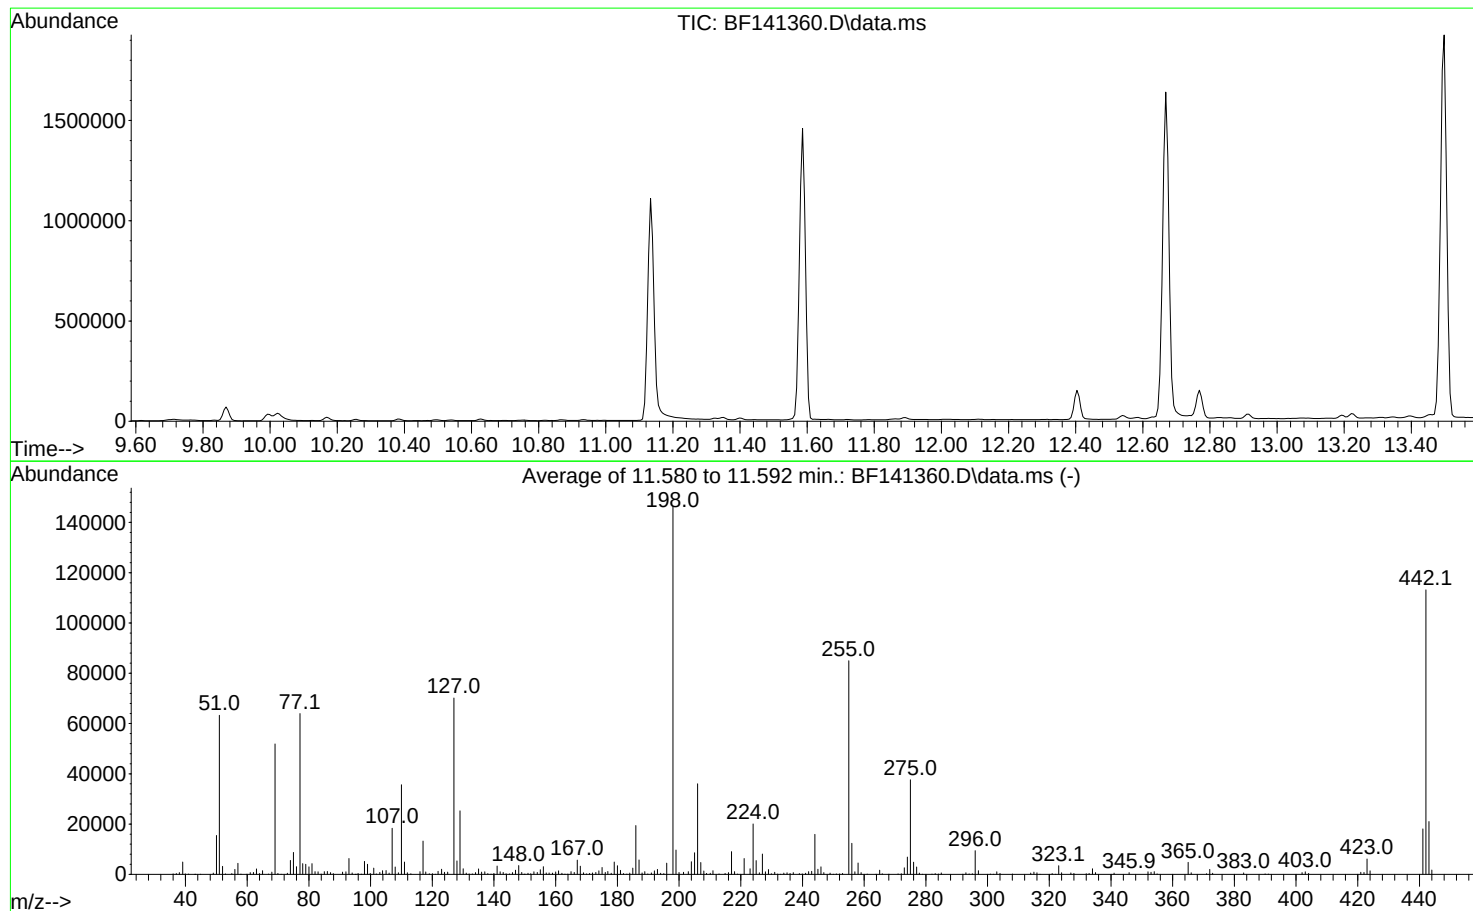

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.2	63285	PASS
68	69	0.00	2	1.7	900	PASS
69	198	0.00	100	35.5	51895	PASS
70	69	0.00	2	0.7	361	PASS
127	198	10	80	47.9	70147	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	146336	PASS
199	198	5	9	6.6	9686	PASS
275	198	10	60	25.7	37640	PASS
365	198	1	100	3.2	4754	PASS
441	198	0.01	100	12.3	18072	PASS
442	442	50	100	100.0	113157	PASS
443	442	15	24	18.6	21030	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/3/2025	BNA_F	<u>BF141360.D</u>
Compound Name	Response	Retention Time
DDT	493977	13.498
DDD	9683	13.221
DDE	491	12.857
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10174	504151	2.02

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020325\
Data File : BF141360.D
Acq On : 03 Feb 2025 09:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 03 12:16:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 29 17:41:25 2025
Response via : Initial Calibration

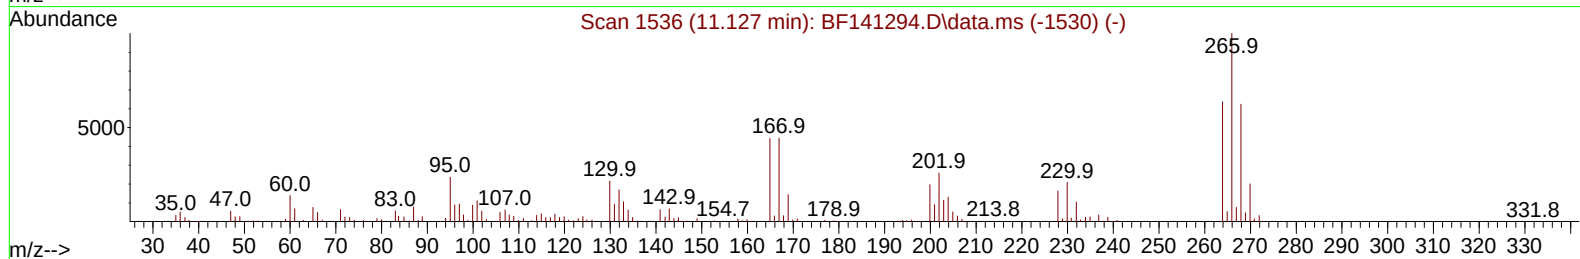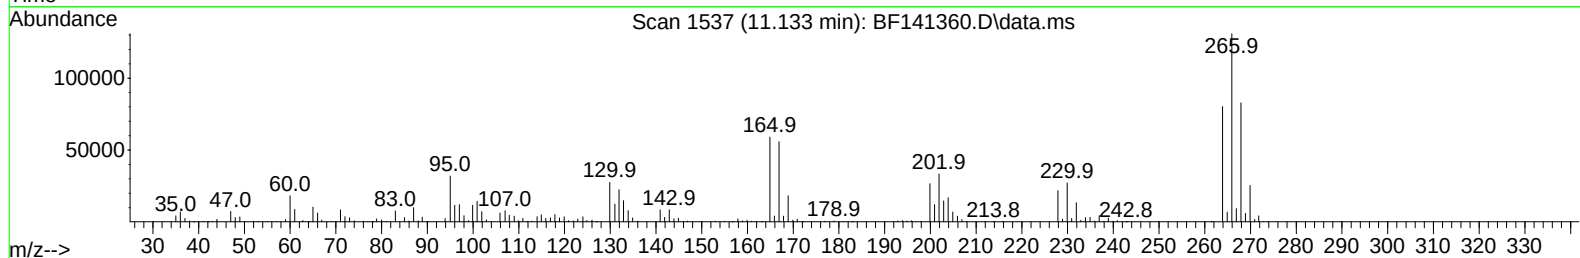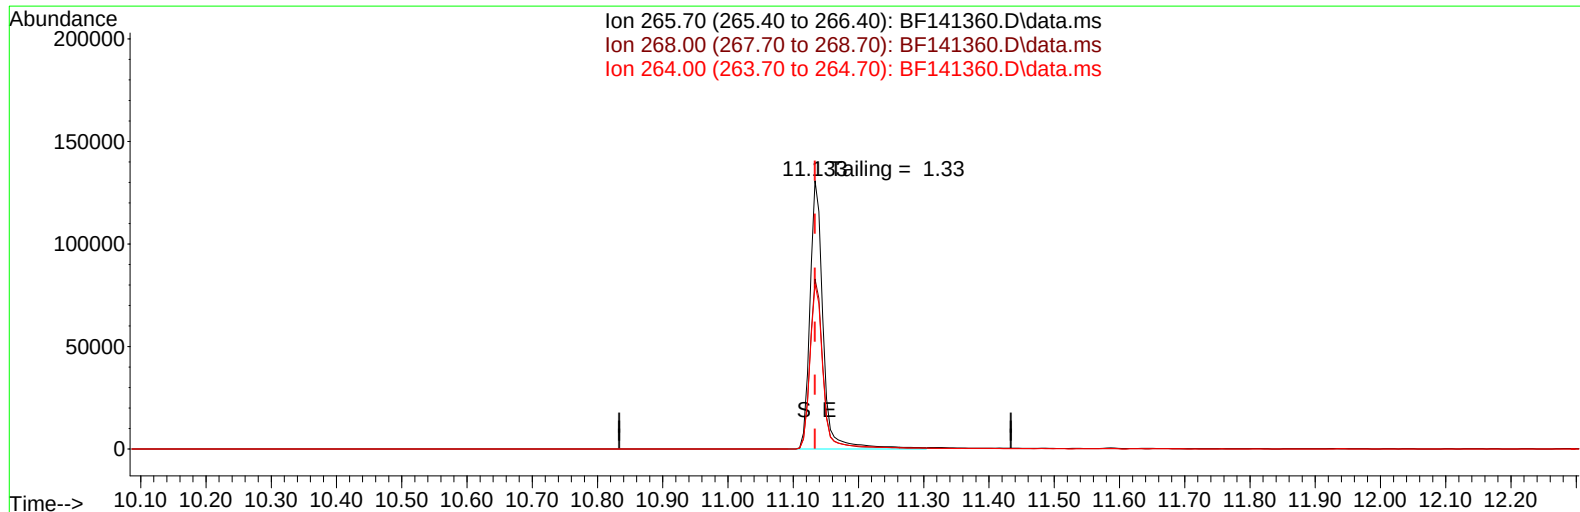

TIC: BF141360.D\data.ms

(70) Pentachlorophenol (C)

11.133min (-0.000) 6278.82 ng




response 185394

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	63.32
264.00	63.70	61.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020325\
Data File : BF141360.D
Acq On : 03 Feb 2025 09:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 03 12:16:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 29 17:41:25 2025
Response via : Initial Calibration

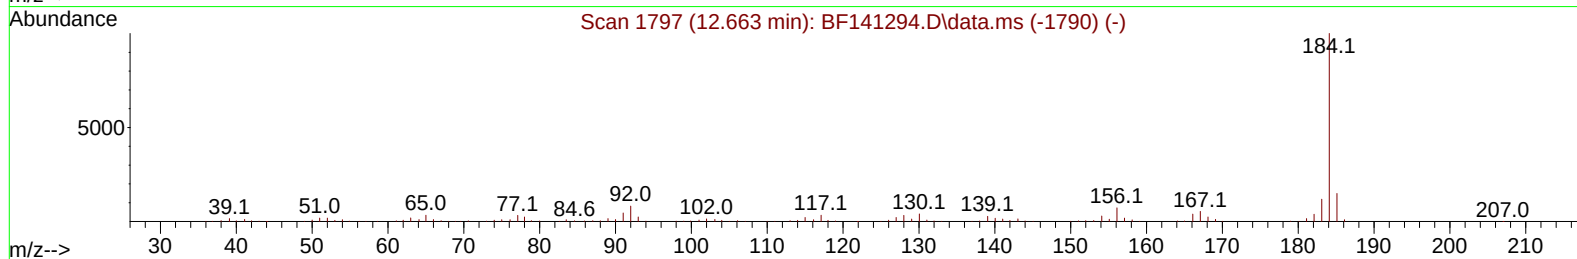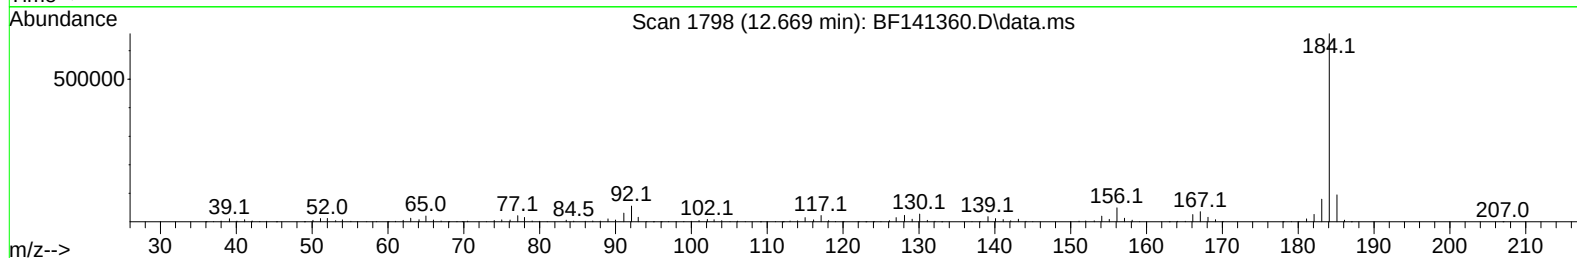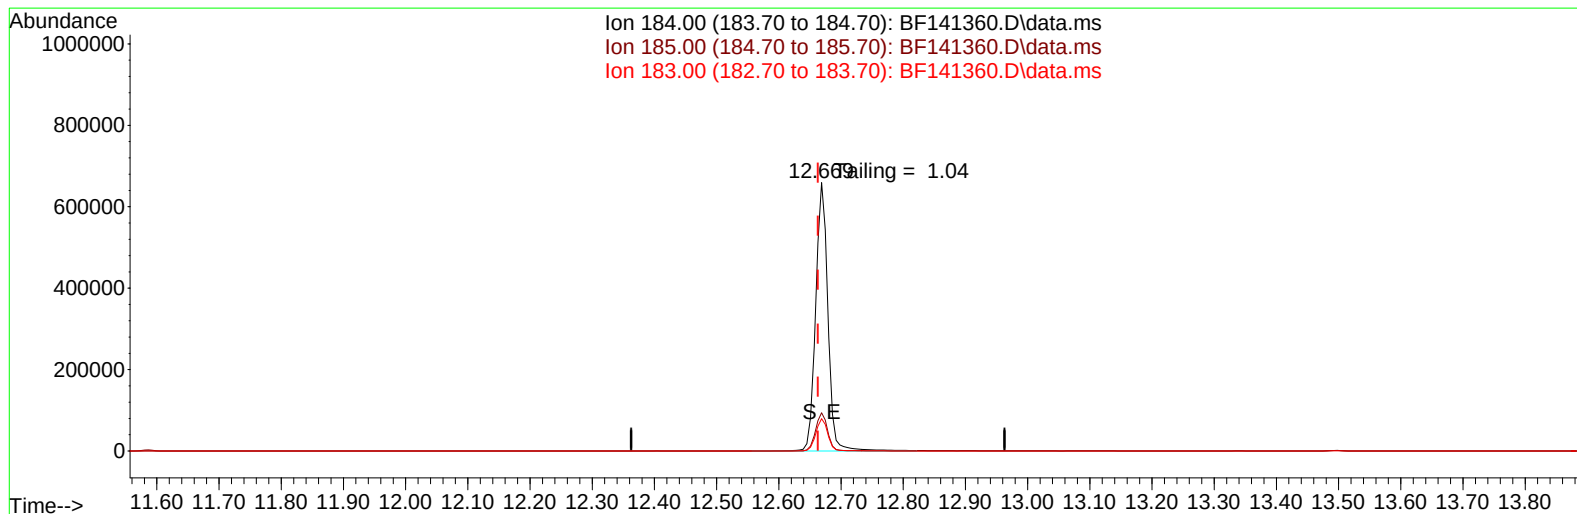

TIC: BF141360.D\data.ms

(77) Benzidine

12.669min (+ 0.006) 7483.96 ng

response 909791

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.28
183.00	11.90	12.04
0.00	0.00	0.00