
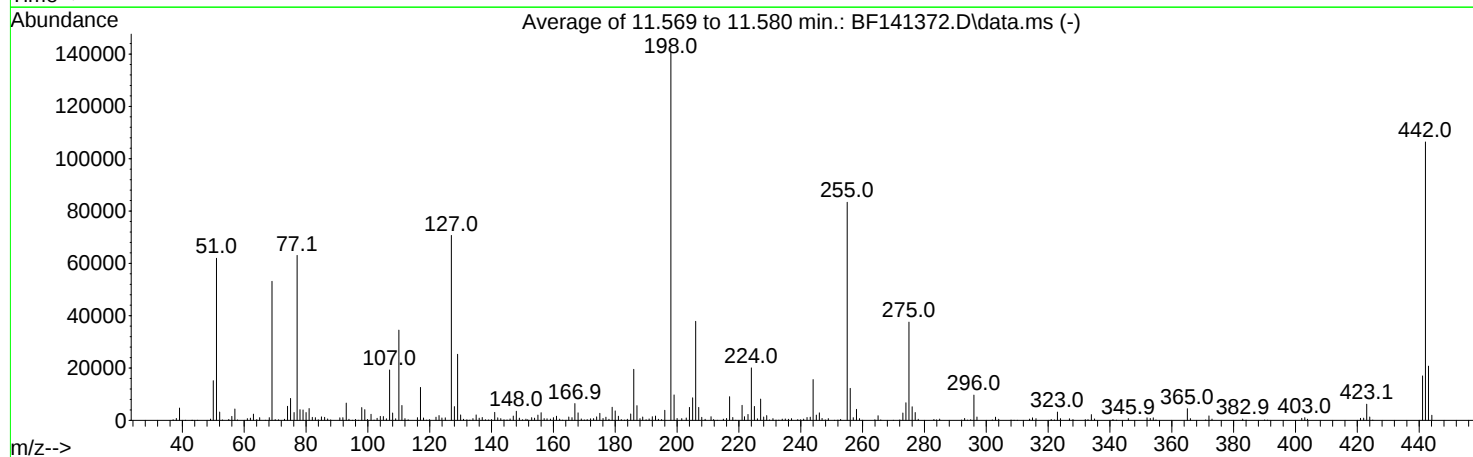


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020325\
Data File : BF141372.D
Acq On : 03 Feb 2025 16:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jan 29 17:41:25 2025

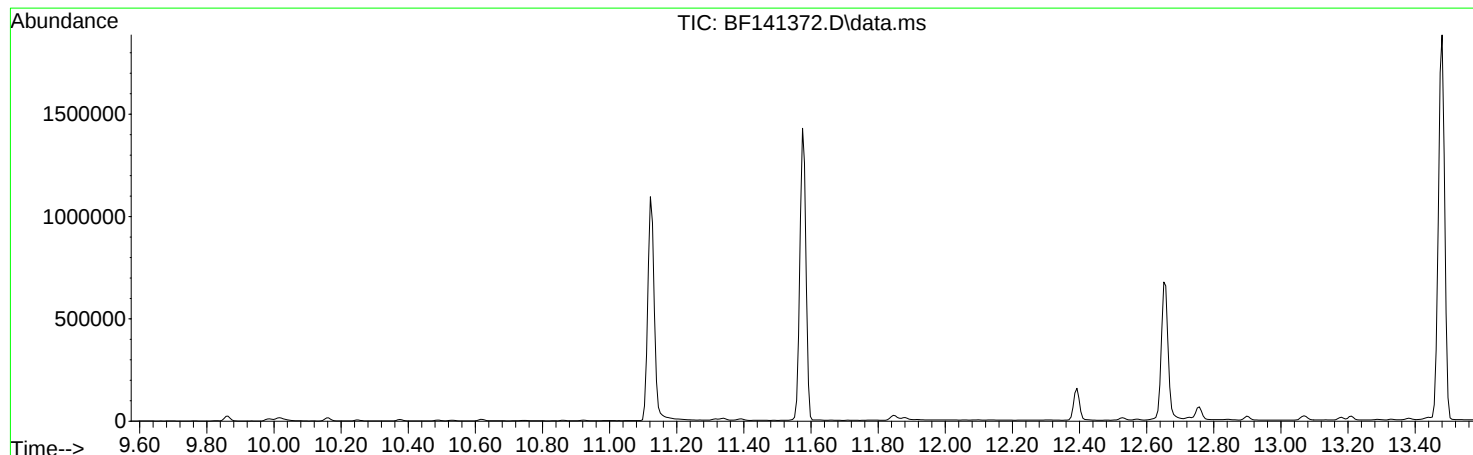

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.1	61981	PASS
68	69	0.00	2	2.0	1060	PASS
69	198	0.00	100	37.8	53141	PASS
70	69	0.00	2	0.6	326	PASS
127	198	10	80	50.3	70667	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	140589	PASS
199	198	5	9	6.9	9756	PASS
275	198	10	60	26.7	37523	PASS
365	198	1	100	3.2	4469	PASS
441	198	0.01	100	12.1	17032	PASS
442	442	50	100	100.0	106389	PASS
443	442	15	24	19.5	20710	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/3/2025	BNA_F	<u>BF141372.D</u>
Compound Name	Response	Retention Time
DDT	484680	13.48
DDD	8749	13.21
DDE	790	12.845
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9539	494219	1.93

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020325\
Data File : BF141372.D
Acq On : 03 Feb 2025 16:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 04 05:08:05 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 29 17:41:25 2025
Response via : Initial Calibration

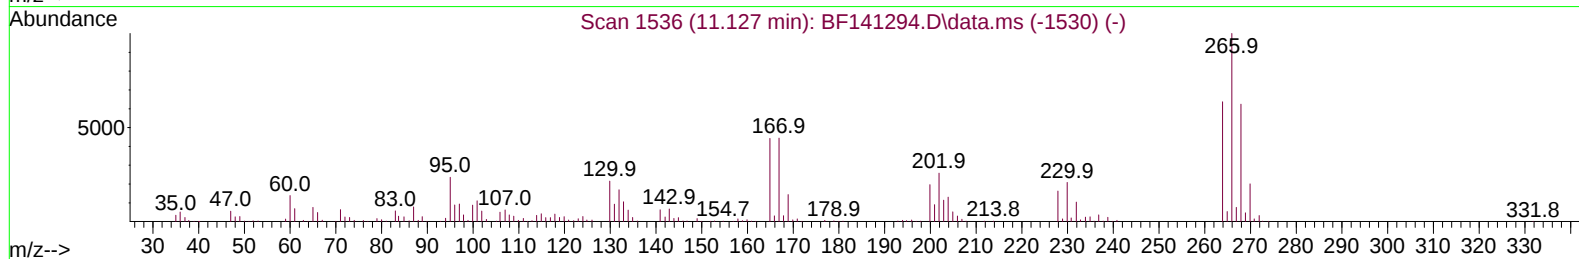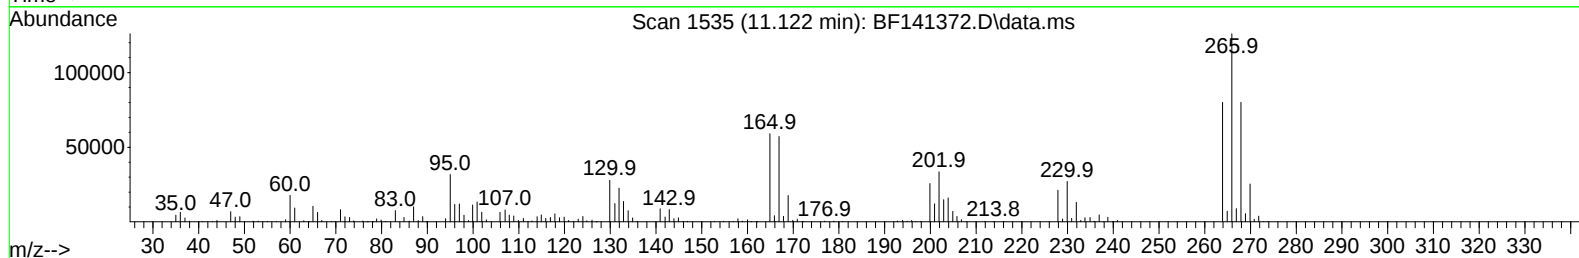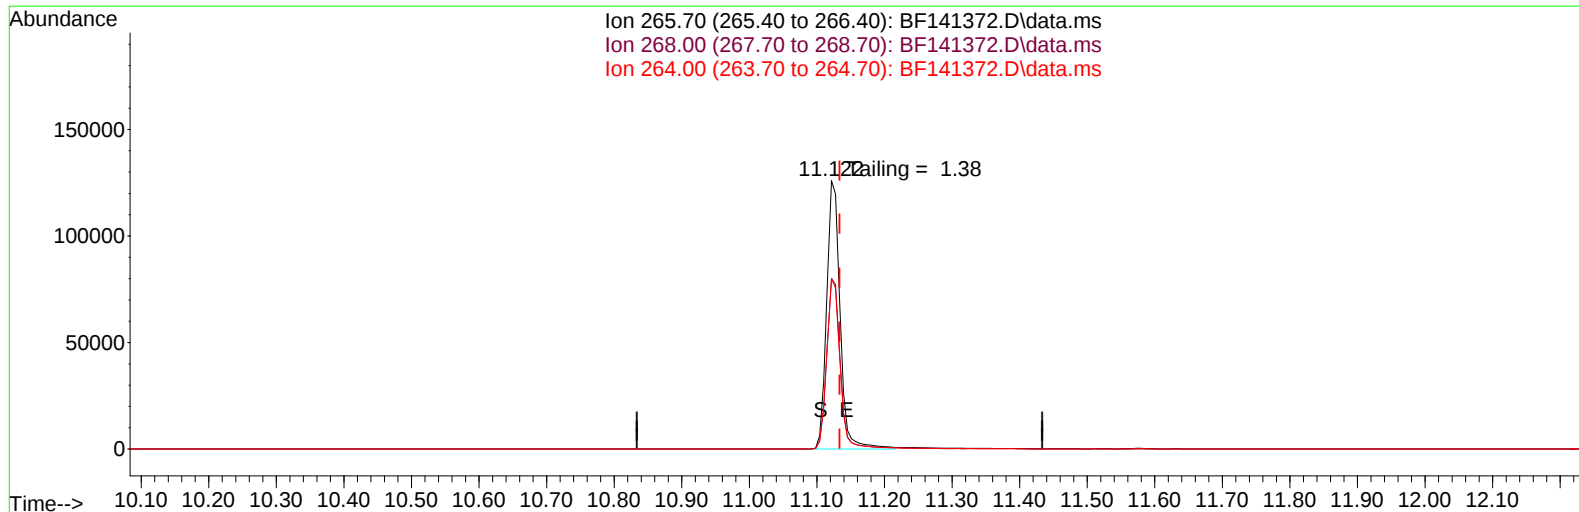

TIC: BF141372.D\data.ms

(70) Pentachlorophenol (C)

11.122min (-0.012) 6372.12 ng




response 175387

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	63.54
264.00	63.70	63.51
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020325\  
Data File : BF141372.D  
Acq On    : 03 Feb 2025  16:43  
Operator  : RC/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 04 05:08:05 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 29 17:41:25 2025
Response via : Initial Calibration

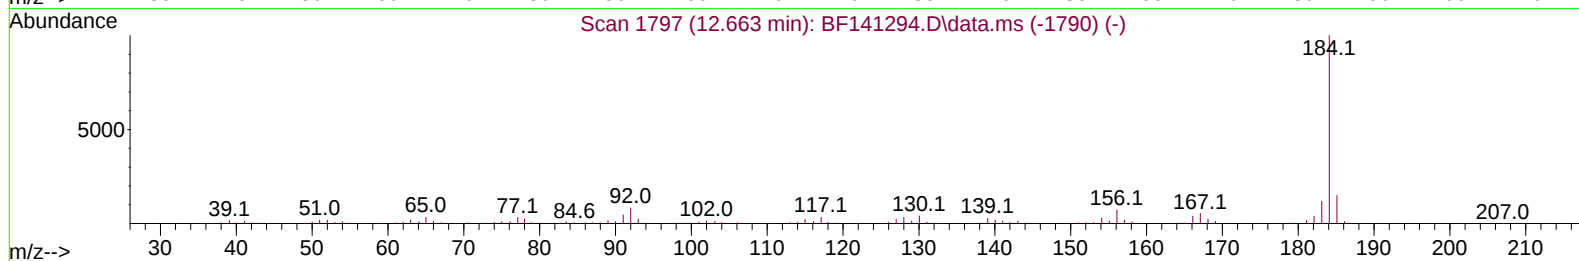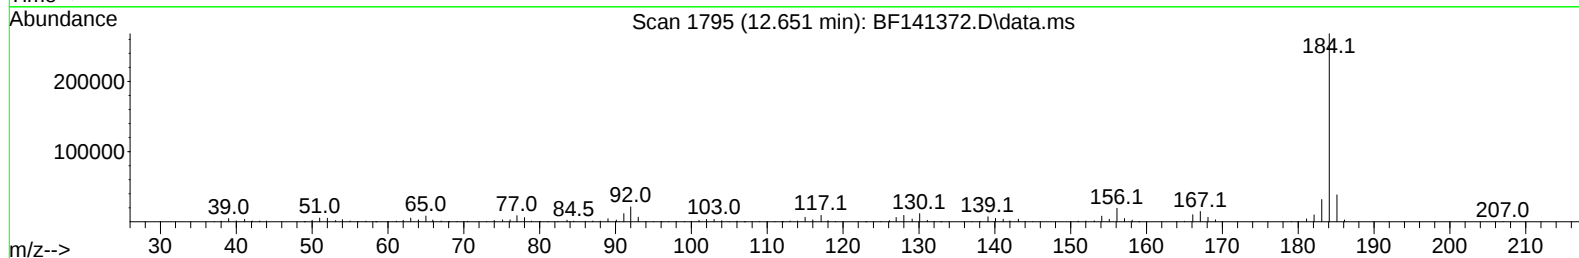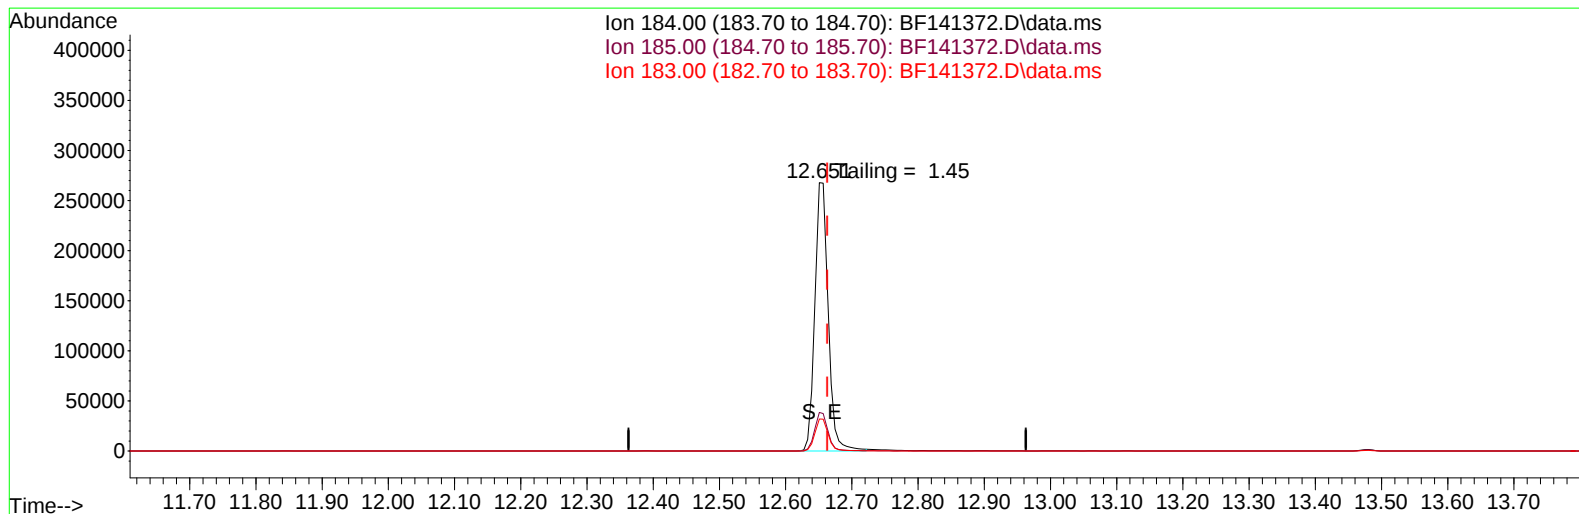

TIC: BF141372.D\data.ms

(77) Benzidine

12.651min (-0.012) 4251.31 ng

response **379432**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.36
183.00	11.90	11.93
0.00	0.00	0.00