


Data Path : Z:\HPCHEM1\BNA\_F\Data\BF020415\  
 Data File : BF077174.D  
 Acq On : 4 Feb 2015 9:42  
 Operator : TP/IZ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF011415.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Jan 30 22:48:24 2015

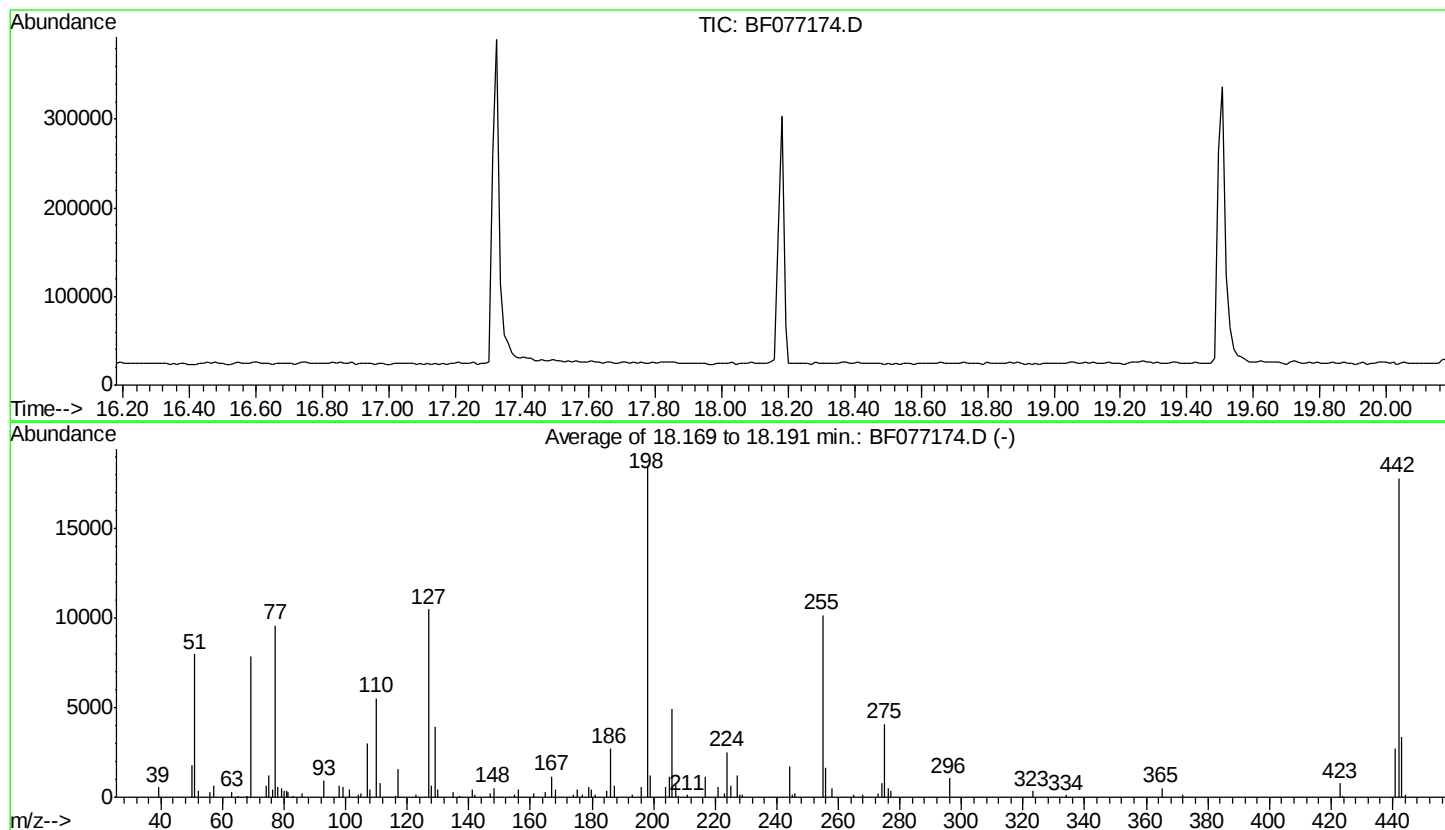

AutoFind: Scans 1512, 1513, 1514; Background Corrected with Scan 1508

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 43.2      | 7992    | PASS             |
| 68          | 69           | 0.00         | 2            | 1.4       | 108     | PASS             |
| 69          | 198          | 0.00         | 100          | 42.3      | 7826    | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 56.7      | 10482   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 18498   | PASS             |
| 199         | 198          | 5            | 9            | 6.5       | 1210    | PASS             |
| 275         | 198          | 10           | 60           | 22.2      | 4103    | PASS             |
| 365         | 198          | 1            | 100          | 2.9       | 530     | PASS             |
| 441         | 442          | 0.01         | 24           | 15.1      | 2688    | PASS             |
| 442         | 198          | 50           | 100          | 96.3      | 17816   | PASS             |
| 443         | 442          | 15           | 24           | 18.8      | 3355    | PASS             |