

Data Path : Z:\HPCHEM1\BNA F\DATA\BF020415\
 Data File : BF077177.D
 Acq On : 4 Feb 2015 13:18
 Operator : TP/IZ
 Sample : G1207-05
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.013	9	11	14	rVB2	1582	2665	1.21%	0.176%
2	1.138	19	22	23	rBV	1813	3407	1.55%	0.225%
3	1.276	33	34	38	rVB	1676	3168	1.44%	0.209%
4	1.356	38	41	42	rBV	1918	3462	1.57%	0.228%
5	1.378	42	43	54	rVB	49686	94812	43.02%	6.249%
6	1.961	92	94	98	rBV	1291	4042	1.83%	0.266%
7	2.087	102	105	107	rBV	1470	3032	1.38%	0.200%
8	3.253	206	207	211	rBV	1813	4932	2.24%	0.325%
9	4.144	284	285	287	rVB	2747	3102	1.41%	0.204%
10	4.202	287	290	293	rBV	2582	7112	3.23%	0.469%
11	4.282	293	297	299	rVV	1857	5256	2.38%	0.346%
12	4.316	299	300	302	rVV	2021	3138	1.42%	0.207%
13	4.384	304	306	310	rVV	1932	4164	1.89%	0.274%
14	4.464	310	313	314	rVV	1657	3005	1.36%	0.198%
15	4.522	314	318	321	rVV	1375	3634	1.65%	0.240%
16	4.739	335	337	340	rBV	1395	3370	1.53%	0.222%
17	4.944	350	355	357	rVB	1101	3091	1.40%	0.204%
18	5.653	415	417	422	rBV	1564	4632	2.10%	0.305%
19	6.293	471	473	476	rBV	1781	3531	1.60%	0.233%
20	6.510	486	492	493	rBV	1404	3842	1.74%	0.253%
21	6.807	517	518	522	rBV	2031	4106	1.86%	0.271%
22	6.899	524	526	530	rVV	2323	4236	1.92%	0.279%
23	7.093	541	543	548	rVB	1678	3944	1.79%	0.260%
24	7.619	588	589	592	rVB	1392	2694	1.22%	0.178%
25	7.688	592	595	603	rBV	56676	112356	50.98%	7.406%
26	7.813	603	606	607	rVB	1903	3117	1.41%	0.205%
27	8.636	675	678	680	rBV	1155	2867	1.30%	0.189%
28	9.139	720	722	727	rBV	1083	3178	1.44%	0.209%
29	9.516	753	755	759	rVB	1574	3727	1.69%	0.246%
30	9.916	787	790	793	rVB	1091	2686	1.22%	0.177%
31	9.996	795	797	800	rVB	1416	2896	1.31%	0.191%
32	10.145	807	810	812	rBV	1283	2883	1.31%	0.190%
33	10.339	824	827	831	rBV	1519	5106	2.32%	0.337%
34	10.522	840	843	844	rBV	1812	2802	1.27%	0.185%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020415\
 Data File : BF077177.D
 Acq On : 4 Feb 2015 13:18
 Operator : TP/IZ
 Sample : G1207-05
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	10.591	846	849	855	rVV	94207	163467	74.18%	10.775%
36	10.876	871	874	876	rVB	1407	3563	1.62%	0.235%
37	11.368	912	917	919	rVB	2215	4716	2.14%	0.311%
38	11.425	919	922	923	rBV	1787	2890	1.31%	0.190%
39	11.528	929	931	933	rVB	1755	2792	1.27%	0.184%
40	11.597	935	937	941	rVV	1831	5304	2.41%	0.350%
41	11.711	945	947	949	rVB	1401	2692	1.22%	0.177%
42	12.294	995	998	999	rBV	1474	2933	1.33%	0.193%
43	12.419	1006	1009	1011	rVB	1743	3164	1.44%	0.209%
44	12.499	1013	1016	1017	rVB	1779	2892	1.31%	0.191%
45	12.705	1030	1034	1037	rVB	1687	3879	1.76%	0.256%
46	13.162	1071	1074	1077	rVB	1711	4037	1.83%	0.266%
47	13.208	1077	1078	1080	rBV	1536	2750	1.25%	0.181%
48	13.288	1082	1085	1086	rBV	1501	3185	1.45%	0.210%
49	13.597	1104	1112	1115	rBV	1365	6794	3.08%	0.448%
50	14.054	1146	1152	1153	rBV	1849	4795	2.18%	0.316%
51	14.214	1163	1166	1167	rBV	1618	3343	1.52%	0.220%
52	14.271	1169	1171	1175	rBV	1176	2913	1.32%	0.192%
53	14.705	1206	1209	1215	rBV	99532	184445	83.69%	12.157%
54	14.957	1230	1231	1234	rBV	1649	2933	1.33%	0.193%
55	15.071	1237	1241	1245	rVB	1700	4513	2.05%	0.297%
56	15.254	1253	1257	1261	rVV	1594	4598	2.09%	0.303%
57	15.357	1263	1266	1269	rBV	1227	3206	1.45%	0.211%
58	15.906	1312	1314	1317	rVB	1564	2810	1.28%	0.185%
59	16.443	1357	1361	1363	rVB	1569	4348	1.97%	0.287%
60	16.500	1363	1366	1369	rBV	1945	6076	2.76%	0.400%
61	16.854	1395	1397	1399	rVB	2125	3384	1.54%	0.223%
62	16.968	1404	1407	1410	rVB	1059	2918	1.32%	0.192%
63	17.254	1427	1432	1435	rVB	1619	3361	1.53%	0.222%
64	17.346	1439	1440	1444	rBV	2193	4746	2.15%	0.313%
65	17.563	1457	1459	1466	rVB	133249	191289	86.80%	12.608%
66	17.940	1488	1492	1494	rVB	1653	3511	1.59%	0.231%
67	18.100	1505	1506	1509	rVB	2281	3634	1.65%	0.240%
68	18.146	1509	1510	1515	rBV	2212	7282	3.30%	0.480%
69	18.226	1515	1517	1522	rVV	1538	5425	2.46%	0.358%
70	19.060	1587	1590	1593	rVB	1803	5096	2.31%	0.336%
71	19.632	1638	1640	1643	rBV	1622	3594	1.63%	0.237%

Data Path : Z:\HPCHEM1\BNA F\DATA\BF020415\
 Data File : BF077177.D
 Acq On : 4 Feb 2015 13:18
 Operator : TP/IZ
 Sample : G1207-05
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	19.700	1643	1646	1647	rVV	1158	2770	1.26%	0.183%
73	19.746	1647	1650	1653	rVB	1153	2974	1.35%	0.196%
74	20.135	1681	1684	1685	rVB	1810	2731	1.24%	0.180%
75	20.169	1685	1687	1691	rBV	961	2731	1.24%	0.180%
76	20.329	1699	1701	1703	rBV	1406	3479	1.58%	0.229%
77	20.660	1728	1730	1732	rVV	1841	3449	1.57%	0.227%
78	20.752	1735	1738	1741	rVV	1501	4820	2.19%	0.318%
79	21.072	1763	1766	1776	rVB	186968	220379	100.00%	14.526%
80	21.735	1821	1824	1825	rBV	1932	3885	1.76%	0.256%
81	22.158	1860	1861	1864	rVB	1782	2647	1.20%	0.174%
82	22.478	1888	1889	1893	rBV	1275	3517	1.60%	0.232%
83	22.558	1893	1896	1897	rVV	1393	2888	1.31%	0.190%
84	22.752	1910	1913	1920	rVB	126301	201345	91.36%	13.271%
85	23.586	1984	1986	1990	rVB2	1635	3621	1.64%	0.239%
86	24.329	2050	2051	2054	rBV	1896	3721	1.69%	0.245%
87	25.095	2115	2118	2120	rVB	1775	3463	1.57%	0.228%
88	25.278	2132	2134	2137	rVB2	1642	4015	1.82%	0.265%
89	25.449	2147	2149	2156	rVB3	1274	5506	2.50%	0.363%
90	25.552	2156	2158	2161	rBV2	1365	3025	1.37%	0.199%
91	25.609	2161	2163	2167	rVB2	2053	3729	1.69%	0.246%
92	25.724	2170	2173	2175	rBV	1435	2753	1.25%	0.181%
93	26.135	2207	2209	2212	rVB2	2613	3562	1.62%	0.235%
94	26.409	2231	2233	2234	rVB	1965	2679	1.22%	0.177%
95	26.455	2234	2237	2238	rBV2	2417	5201	2.36%	0.343%
96	26.775	2263	2265	2266	rVB	2708	3138	1.42%	0.207%
97	26.821	2266	2269	2270	rBV	2524	4885	2.22%	0.322%
98	26.901	2273	2276	2277	rVV	1605	3479	1.58%	0.229%
99	27.004	2280	2285	2287	rVV3	1686	5227	2.37%	0.345%
100	27.175	2296	2300	2301	rBV2	2127	4265	1.94%	0.281%


Sum of corrected areas: 1517157

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020415\
Data File : BF077177.D
Acq On : 4 Feb 2015 13:18
Operator : TP/IZ
Sample : G1207-05
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

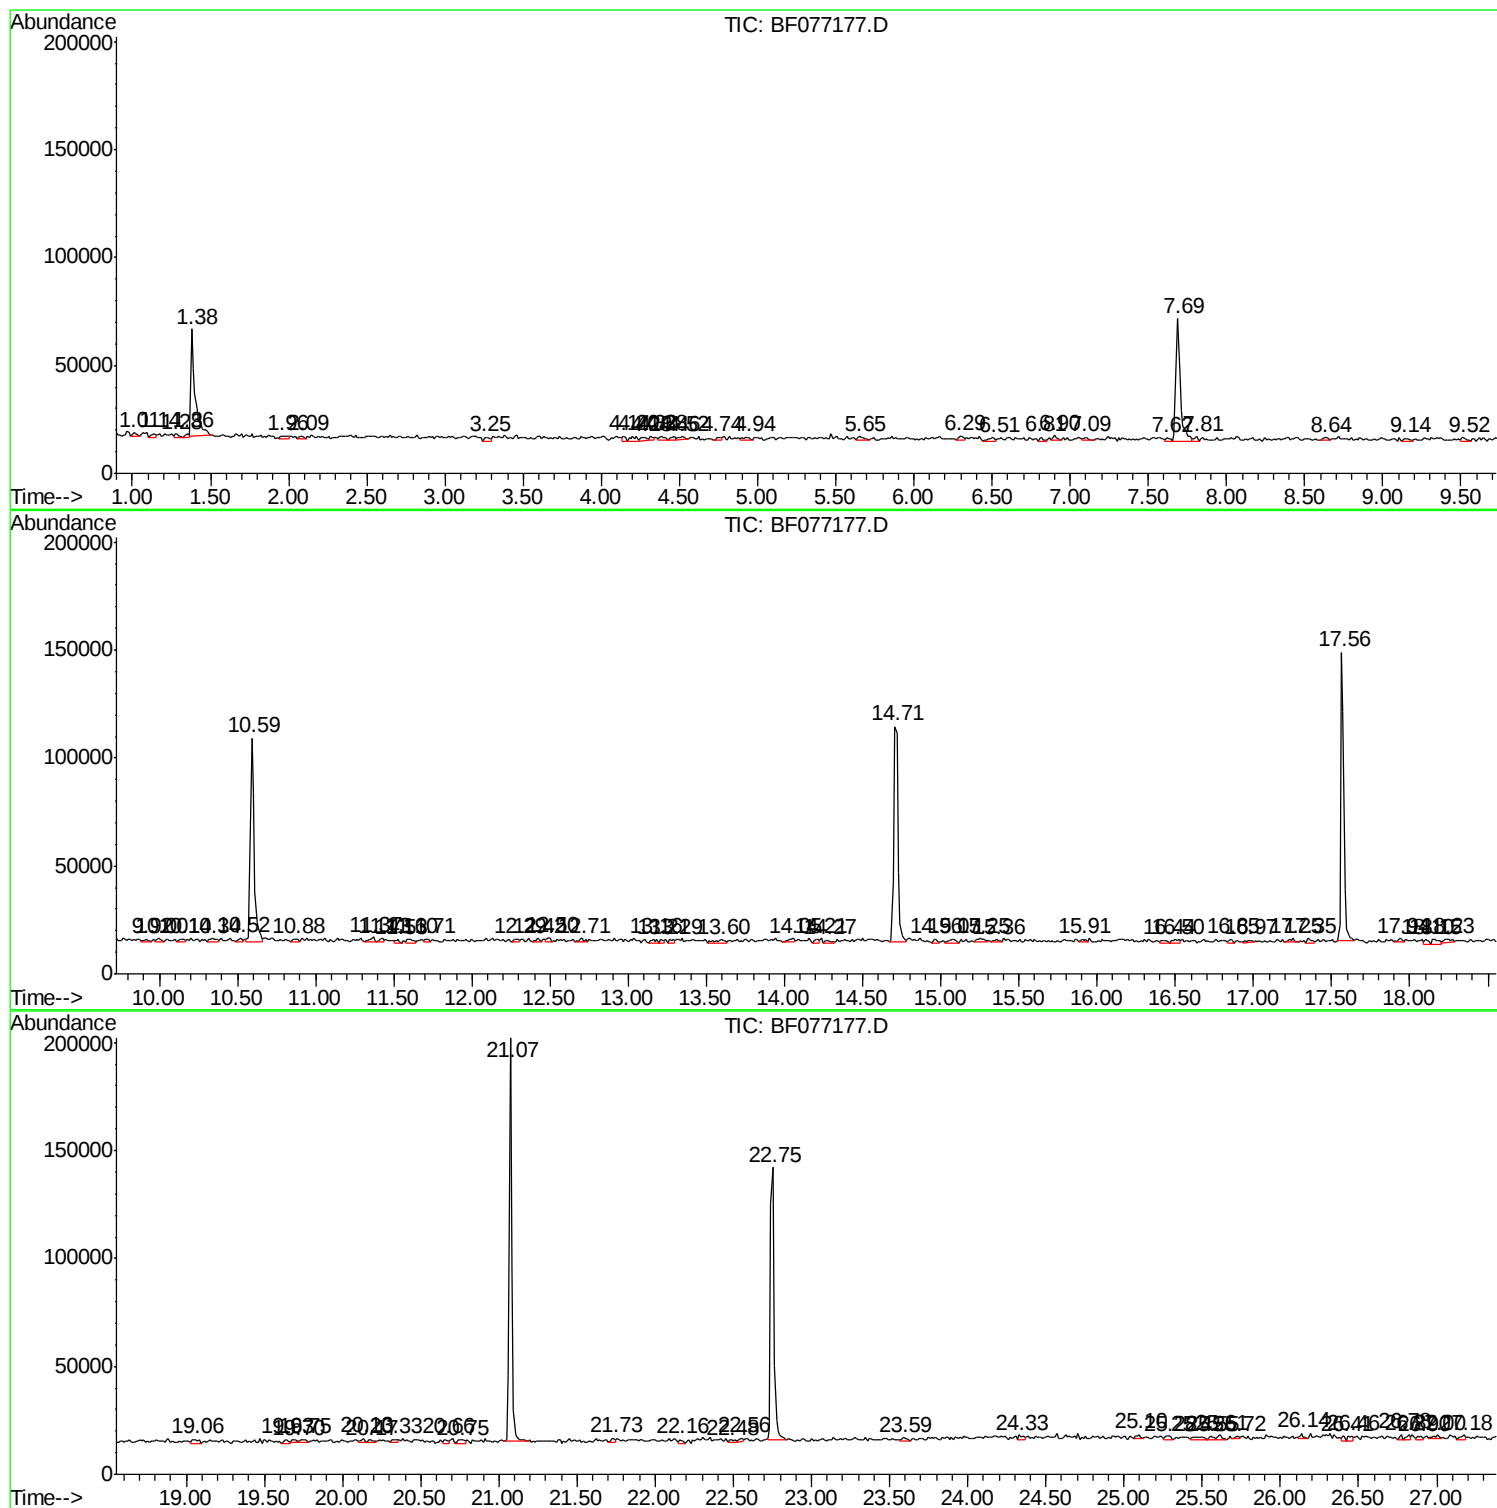

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF020415\
Data_File : BF077177.D
Acq_On : 4 Feb 2015 13:188
Operator : TP/IZZ
Sample : G1207-055
Misc :
ALS_Vial : 4 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
SVOC-GPC-BLANK

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION.NN

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
