


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020415\
 Data File : BF077174.D
 Acq On : 4 Feb 2015 9:42
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 30 22:48:24 2015

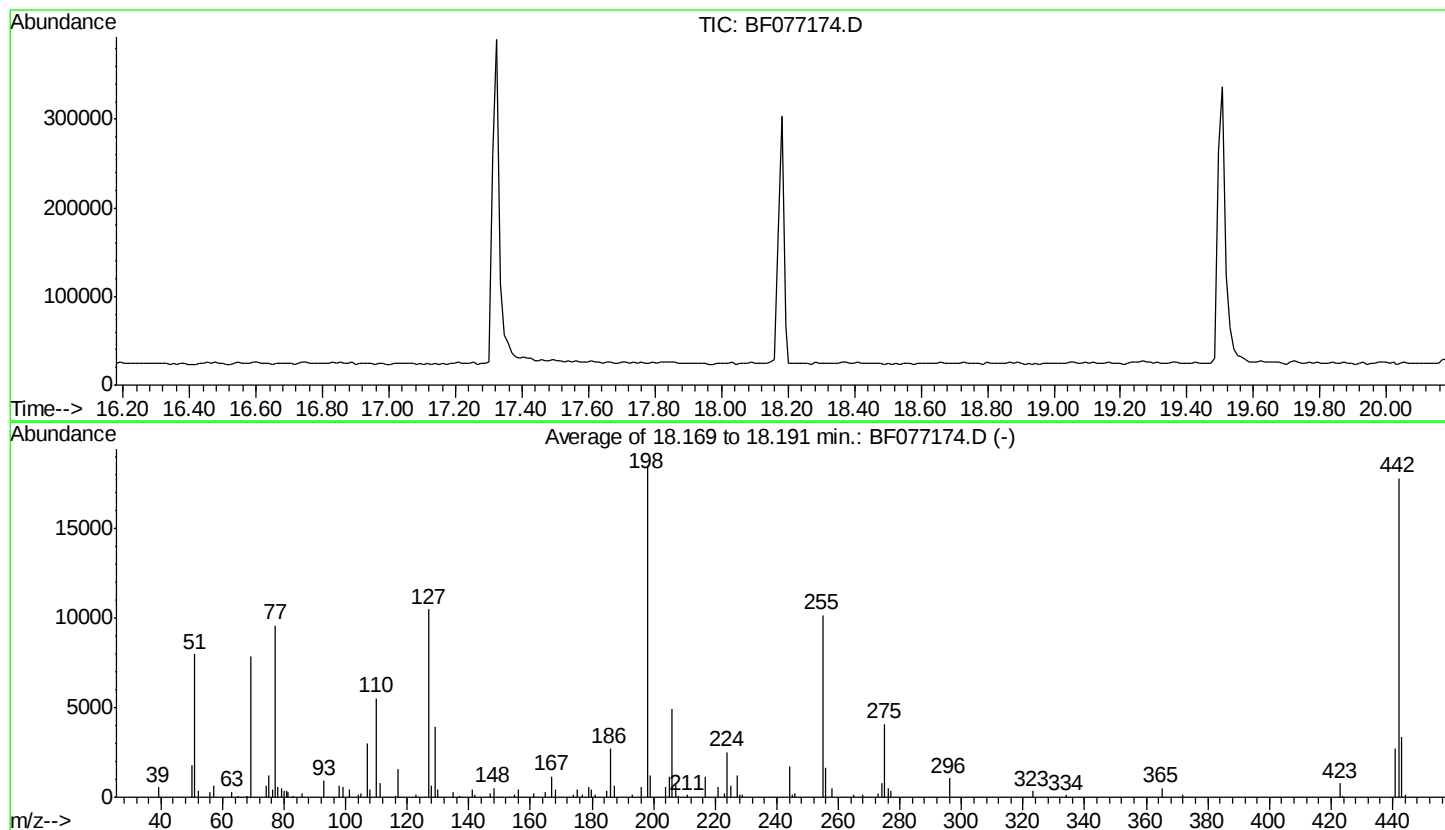

AutoFind: Scans 1512, 1513, 1514; Background Corrected with Scan 1508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.2	7992	PASS
68	69	0.00	2	1.4	108	PASS
69	198	0.00	100	42.3	7826	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	56.7	10482	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	18498	PASS
199	198	5	9	6.5	1210	PASS
275	198	10	60	22.2	4103	PASS
365	198	1	100	2.9	530	PASS
441	442	0.01	24	15.1	2688	PASS
442	198	50	100	96.3	17816	PASS
443	442	15	24	18.8	3355	PASS