
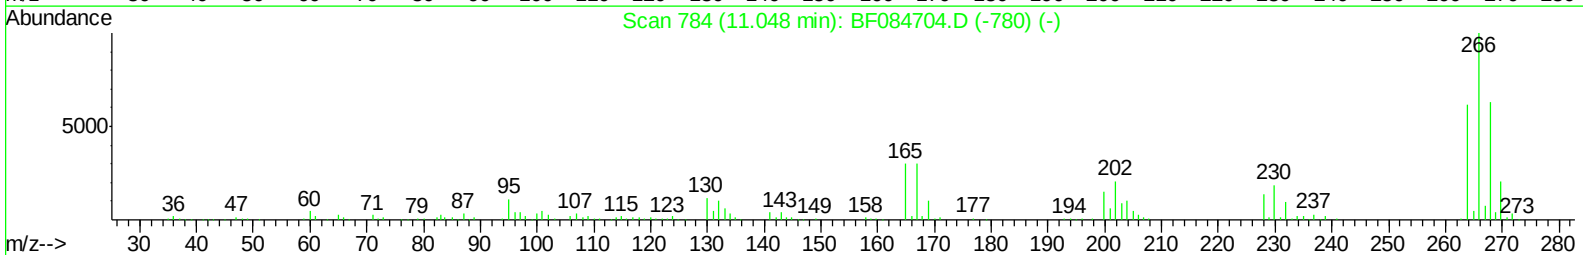
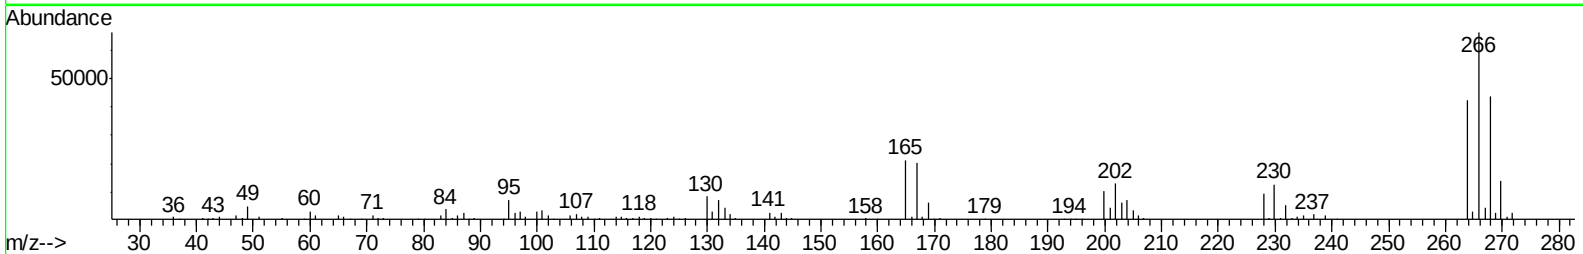


Data Path : Z:\HPCHEM1\BNA_F\Data\BF020416\
Data File : BF084829.D
Acq On : 4 Feb 2016 14:51
Operator : SJ/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 05 06:07:45 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 03 14:16:01 2016
Response via : Initial Calibration

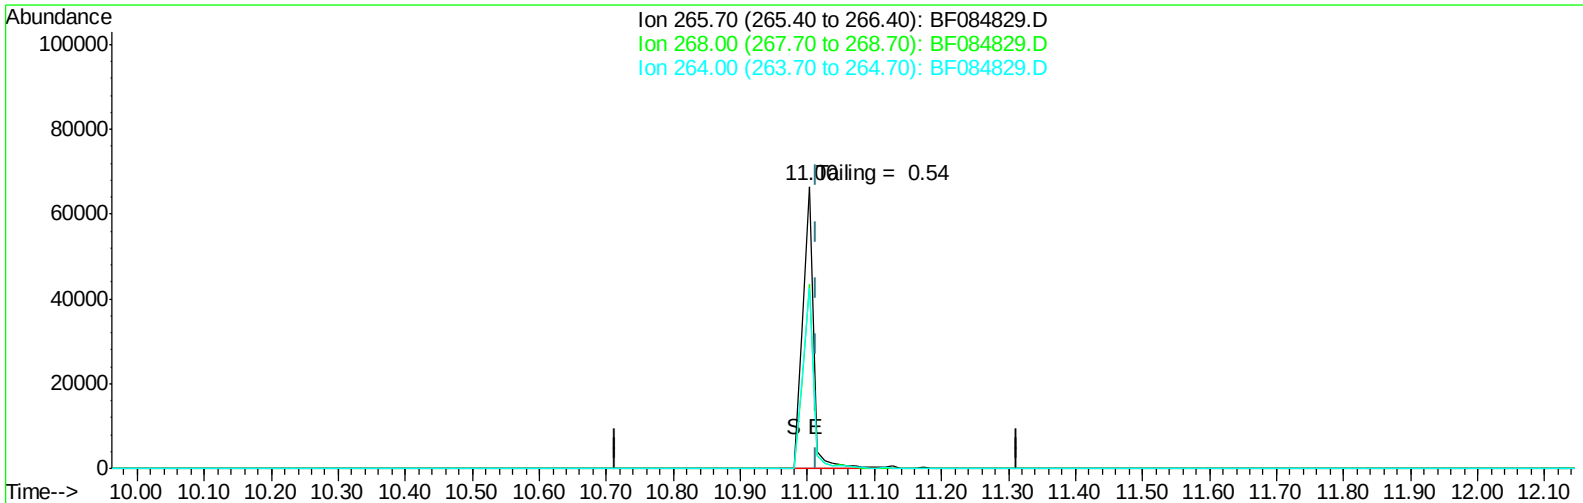

TIC: BF084829.D

(69) Pentachlorophenol (C)




11.002min (-0.011) 49914.06ng

response 75095

Ion	Exp%	Act%
265.70	100	100
268.00	65.50	65.62
264.00	62.70	64.05
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF020416\
Data File : BF084829.D
Acq On : 4 Feb 2016 14:51
Operator : SJ/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 05 06:07:45 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 03 14:16:01 2016
Response via : Initial Calibration

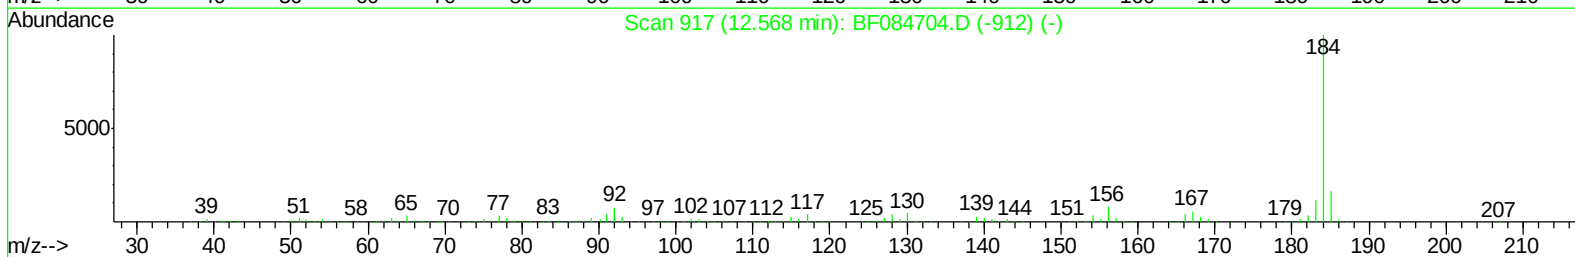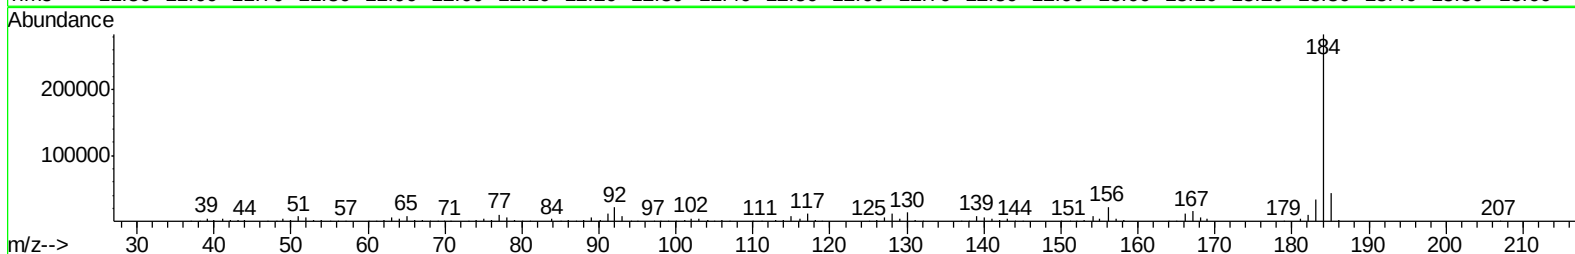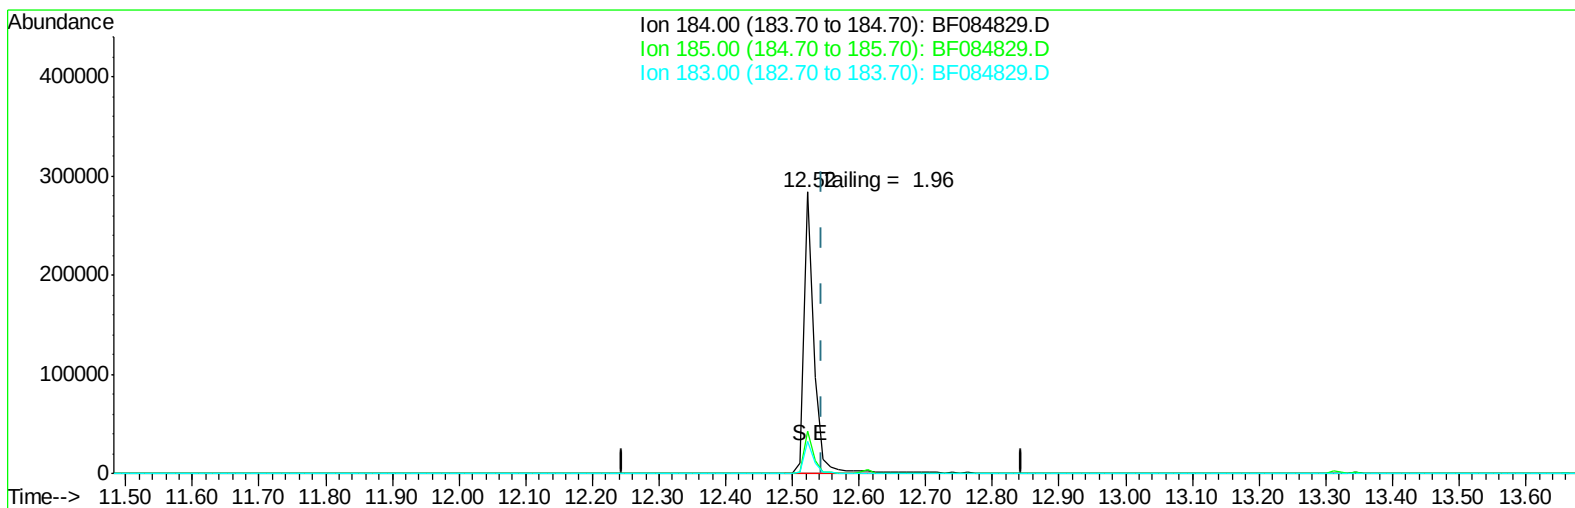

TIC: BF084829.D

(76) Benzidine

12.522min (-0.023) -20.00ng

response 296984

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.94
183.00	12.30	11.43
0.00	0.00	0.00