


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020416\
 Data File : BF084829.D
 Acq On : 4 Feb 2016 14:51
 Operator : SJ/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 03 14:16:01 2016

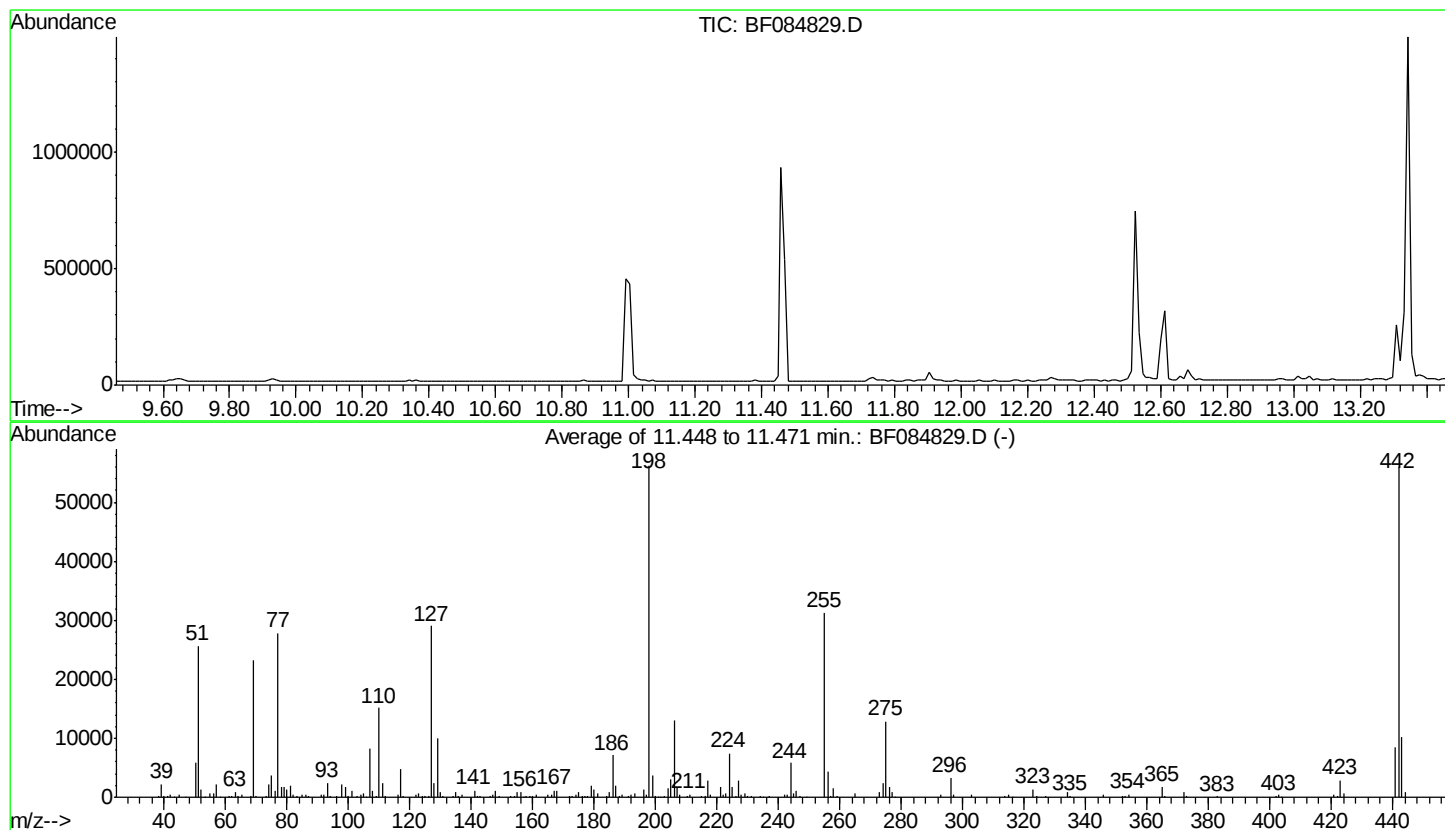

AutoFind: Scans 819, 820, 821; Background Corrected with Scan 816

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.7	25675	PASS
68	69	0.00	2	1.3	291	PASS
69	198	0.00	100	41.3	23198	PASS
70	69	0.00	2	0.8	177	PASS
127	198	10	80	51.7	29048	PASS
197	198	0.00	2	0.6	354	PASS
198	198	100	100	100.0	56208	PASS
199	198	5	9	6.5	3673	PASS
275	198	10	60	22.8	12829	PASS
365	198	1	100	3.3	1831	PASS
441	442	0.01	24	15.1	8441	PASS
442	198	50	100	99.7	56040	PASS
443	442	15	24	18.4	10308	PASS