
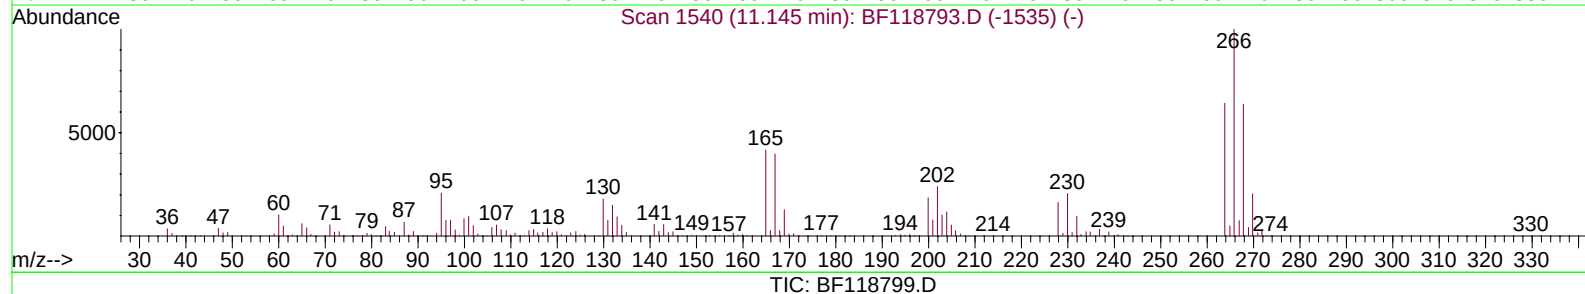
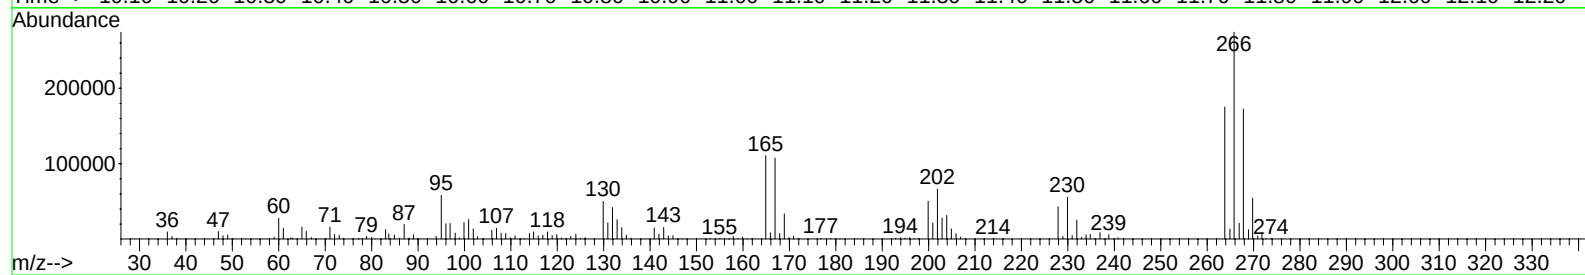


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF020420\
Data File : BF118799.D
Acq On : 4 Feb 2020 13:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 04 18:09:22 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF020320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 03 16:26:03 2020
Response via : Initial Calibration

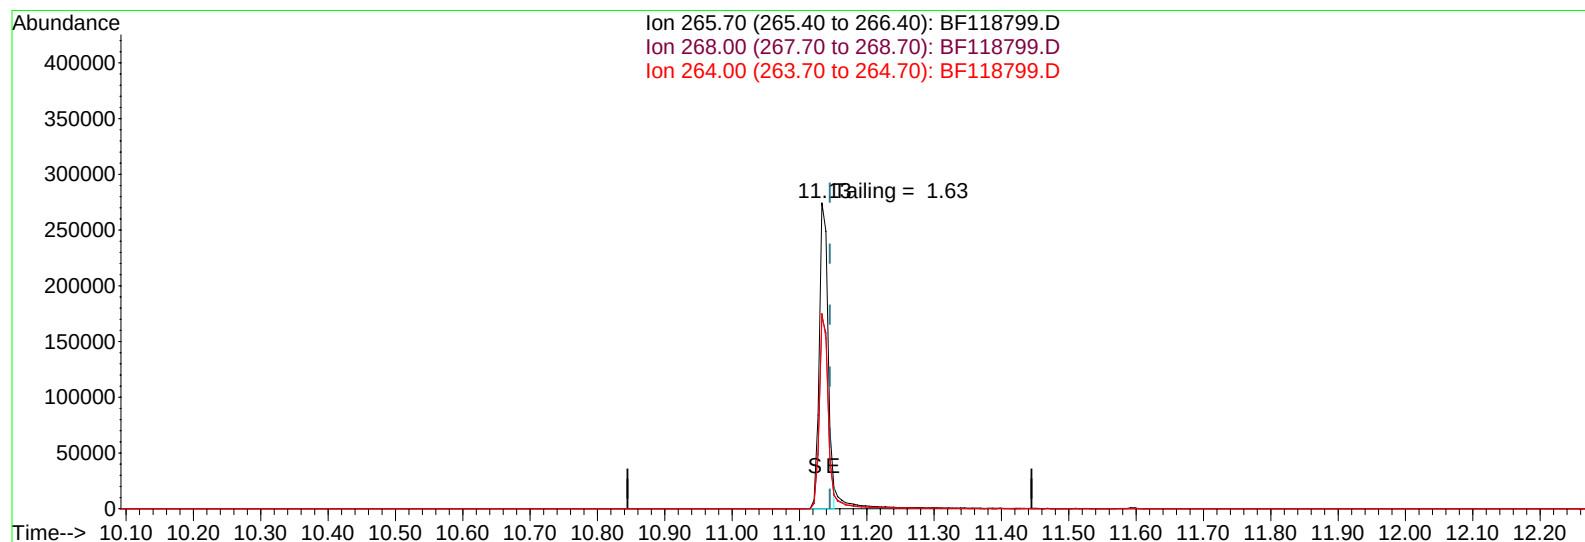

(70) Pentachlorophenol (C)




11.133min (-0.012) 33311.17ng

response 269679

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	62.93
264.00	64.30	63.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF020420\
 Data File : BF118799.D
 Acq On : 4 Feb 2020 13:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 04 18:09:22 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF020320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 03 16:26:03 2020
 Response via : Initial Calibration

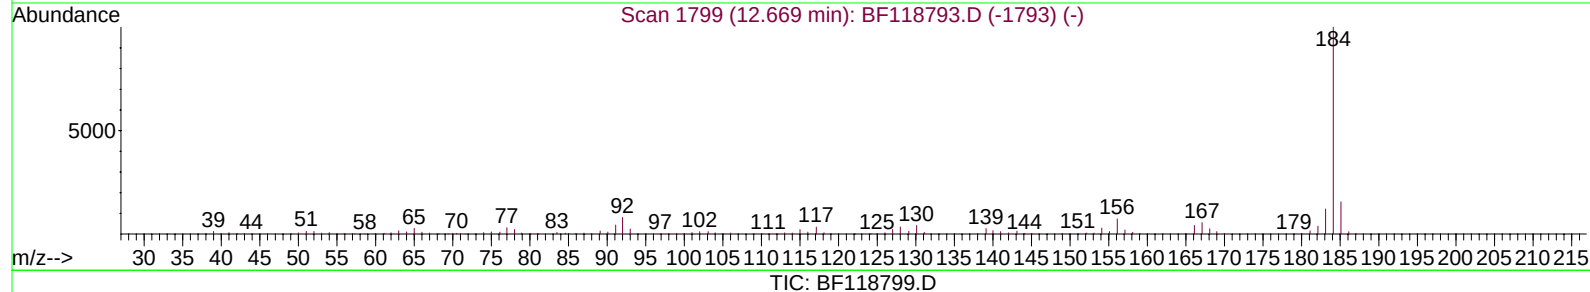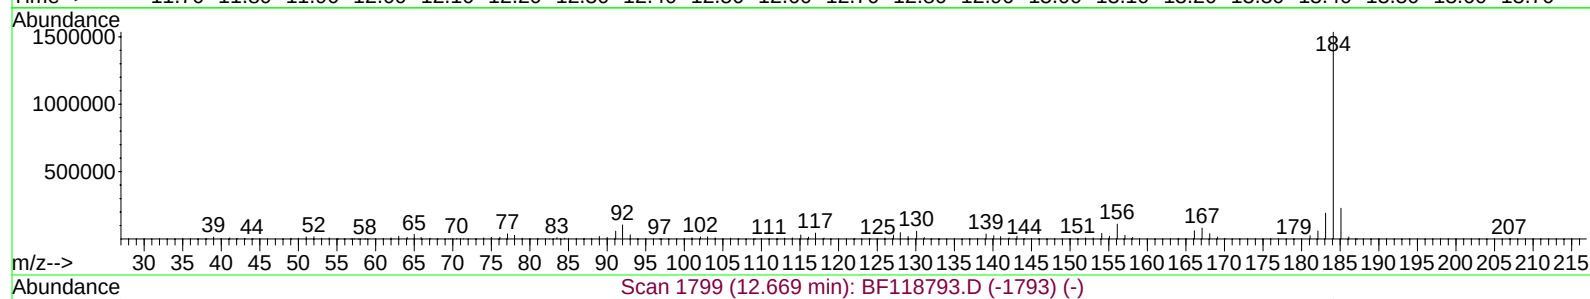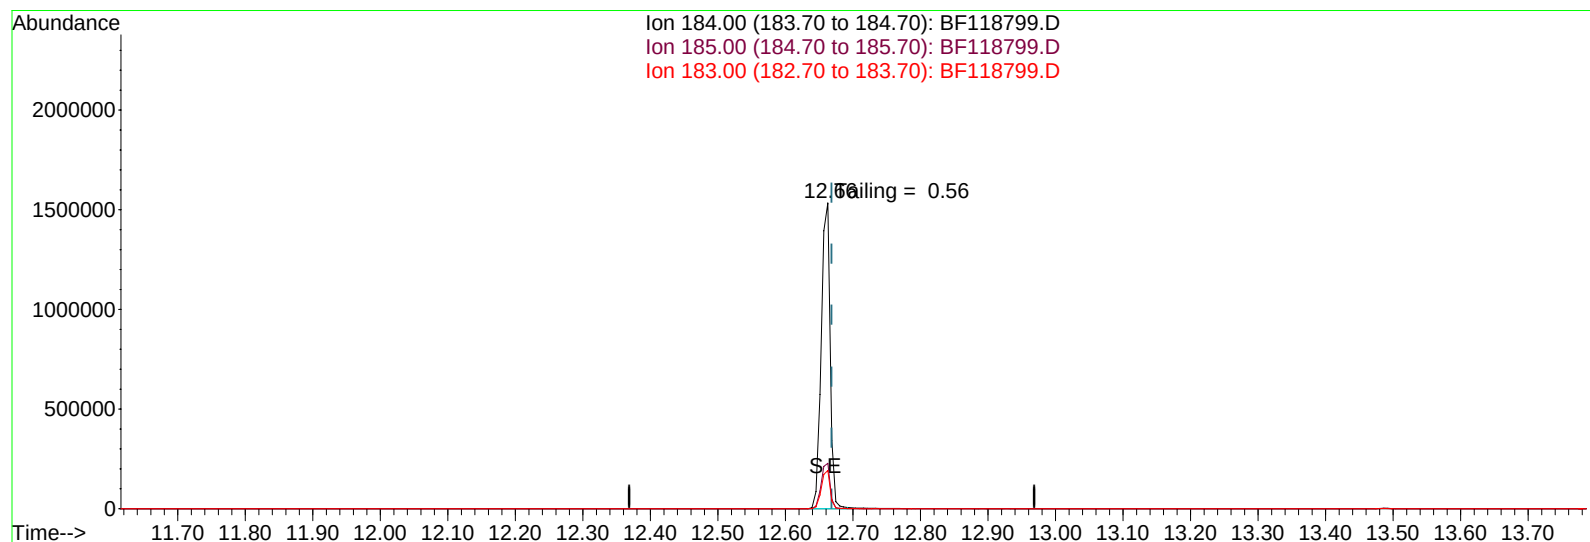

(77) Benzidine

12.663min (-0.006) 0.00ng

response 1423638

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	14.85
183.00	12.10	12.49
0.00	0.00	0.00