

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF020420\
 Data File : BF118812.D
 Acq On : 4 Feb 2020 20:17
 Operator : CG/JU
 Sample : PB126588BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB126588BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF020320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.228	19	24	31	rVB	106962	142520	1.26%	0.218%
2	5.051	500	504	512	rVB	98068	132798	1.18%	0.203%
3	5.440	564	570	573	rBV	6147831	6581242	58.33%	10.060%
4	6.445	735	741	744	rBV	5704903	6468048	57.33%	9.887%
5	6.810	799	803	807	rBV	1933274	1536480	13.62%	2.349%
6	6.969	825	830	833	rBV	6074850	5820858	51.59%	8.897%
7	7.369	893	898	902	rBV	3910266	4500806	39.89%	6.880%
8	8.092	1016	1021	1024	rBV	2292043	2014502	17.86%	3.079%
9	9.169	1198	1204	1207	rBV	8467199	9126700	80.90%	13.951%
10	9.845	1314	1319	1322	rBV	2935458	2571052	22.79%	3.930%
11	10.633	1447	1453	1456	rBV	6429430	6603855	58.53%	10.094%
12	11.327	1566	1571	1574	rBV	3277886	2784307	24.68%	4.256%
13	12.916	1836	1841	1845	rBV	9866430	11282105	100.00%	17.245%
14	13.963	2014	2019	2022	rBV	2982436	2680013	23.75%	4.097%
15	15.068	2203	2207	2218	rVB	143536	192552	1.71%	0.294%
16	15.404	2258	2264	2268	rBV	1953138	2343236	20.77%	3.582%
17	15.439	2268	2270	2276	rVB2	145885	169924	1.51%	0.260%
18	15.862	2337	2342	2348	rBV	98733	152540	1.35%	0.233%
19	16.215	2392	2402	2415	rVB6	49083	192588	1.71%	0.294%
20	16.357	2419	2426	2434	rBV2	58868	125550	1.11%	0.192%


Sum of corrected areas: 65421676

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF020420\
Data File : BF118812.D
Acq On : 4 Feb 2020 20:17
Operator : CG/JU
Sample : PB126588BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB126588BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF020320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

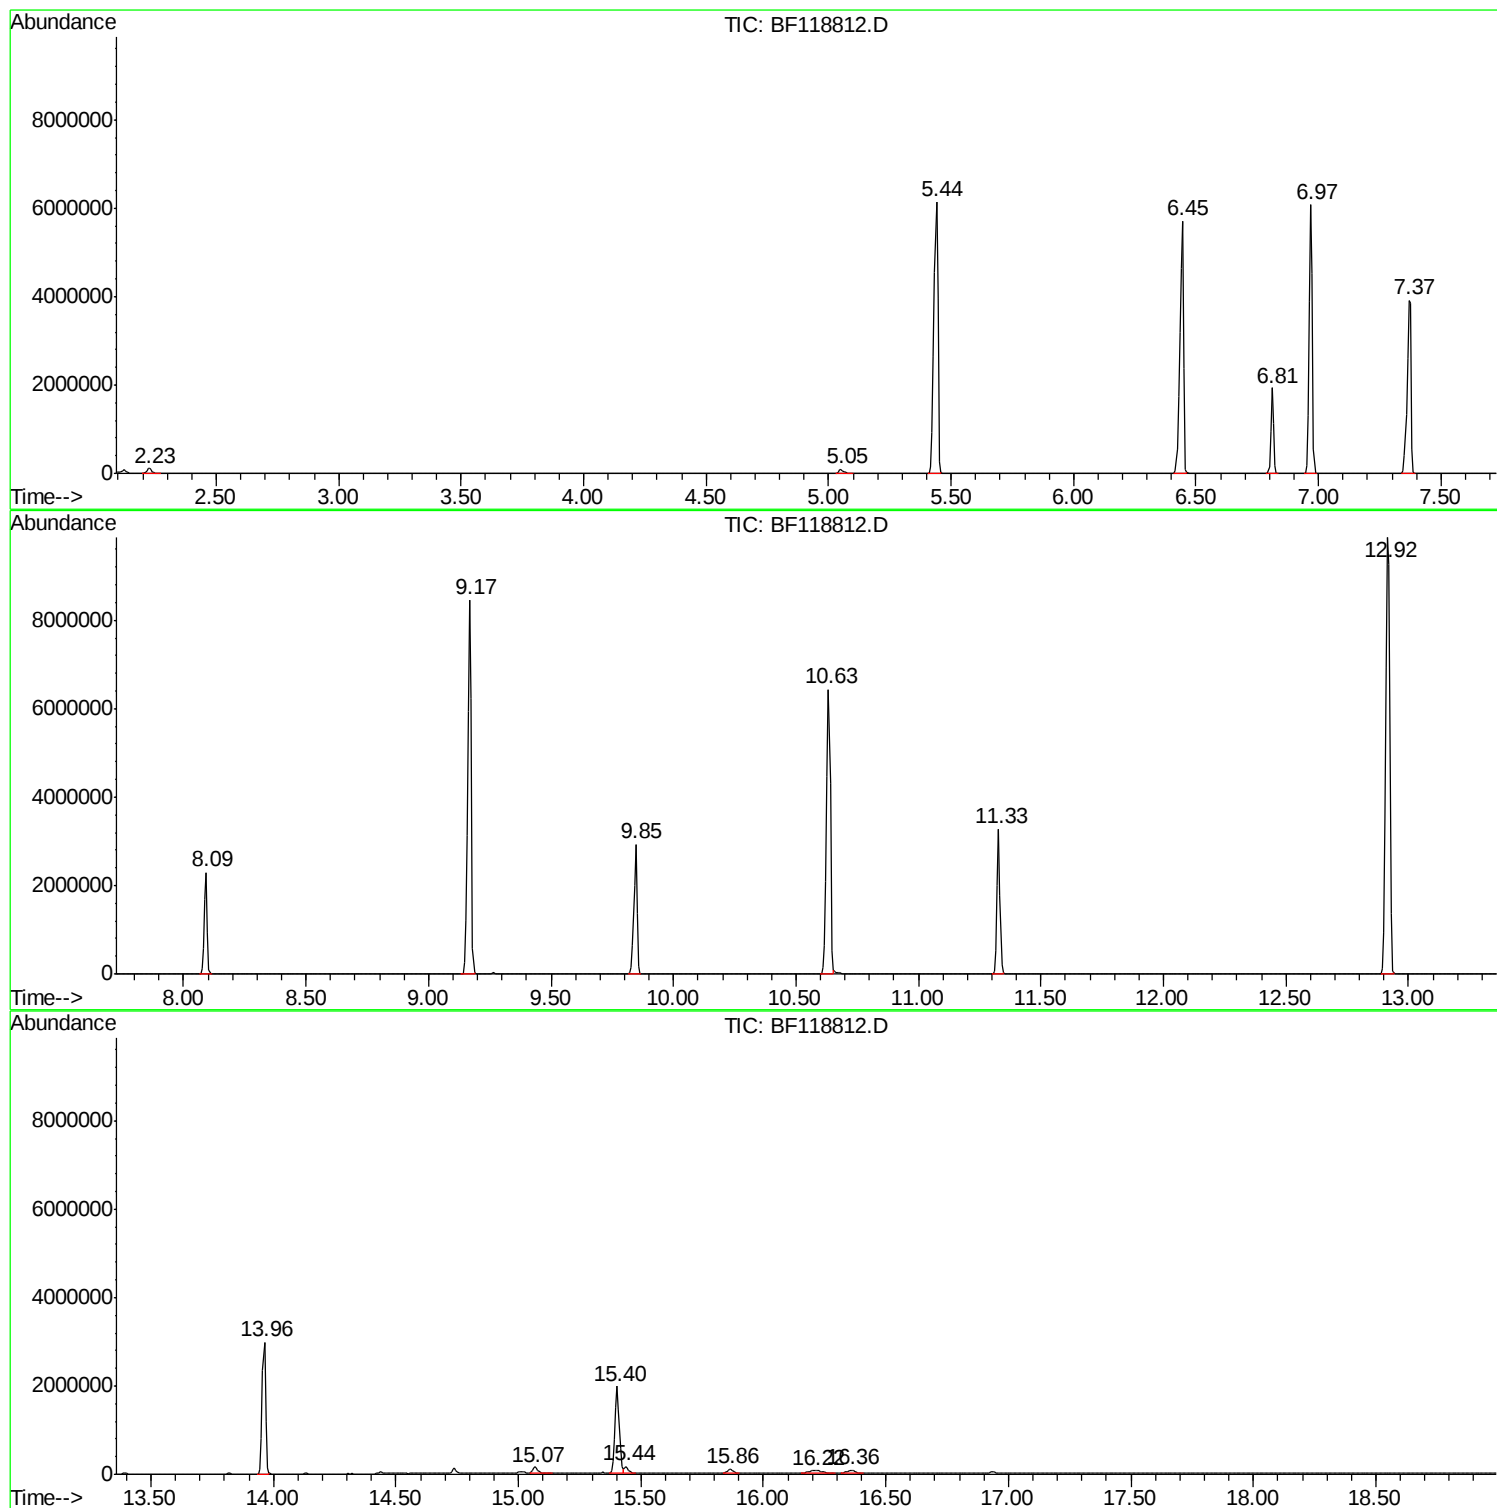

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF020420\
Data_File : BF118812.D
Acq_On : 4 Feb 2020 20:177
Operator : CG/JUU
Sample : PB126588BLL
Misc :
ALS_Vial : 14 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
PB126588BL

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF020320.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
