


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF020420\
 Data File : BF118799.D
 Acq On : 4 Feb 2020 13:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF020320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 03 16:26:03 2020

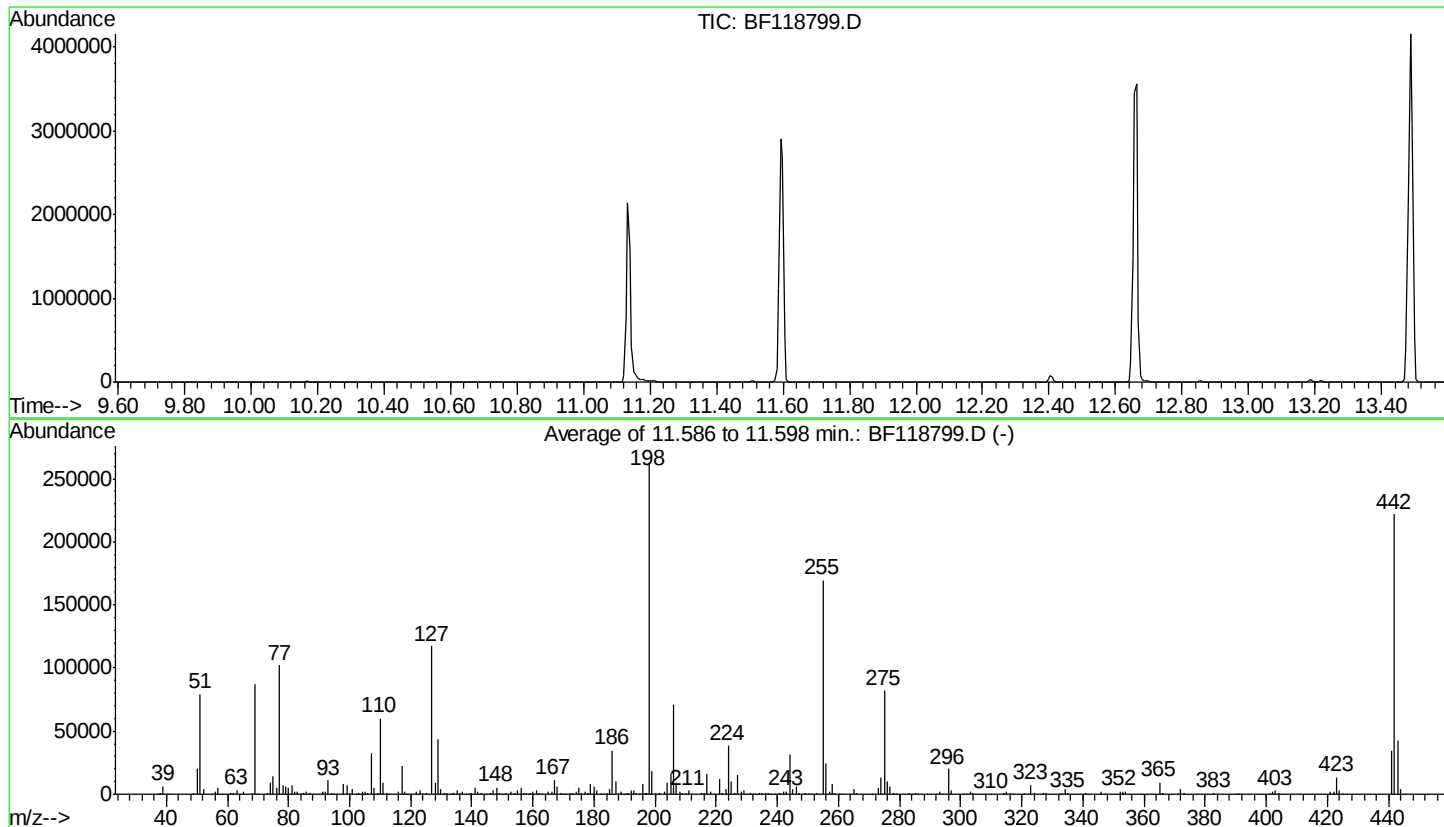

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.2	79368	PASS
68	69	0.00	2	1.0	871	PASS
69	198	0.00	100	33.1	87008	PASS
70	69	0.00	2	0.4	381	PASS
127	198	10	80	44.7	117453	PASS
197	198	0.00	2	0.5	1189	PASS
198	198	100	100	100.0	262805	PASS
199	198	5	9	7.0	18358	PASS
275	198	10	60	31.1	81733	PASS
365	198	1	100	3.6	9471	PASS
441	198	0.01	100	13.1	34340	PASS
442	198	50	100	84.4	221770	PASS
443	442	15	24	19.2	42615	PASS