
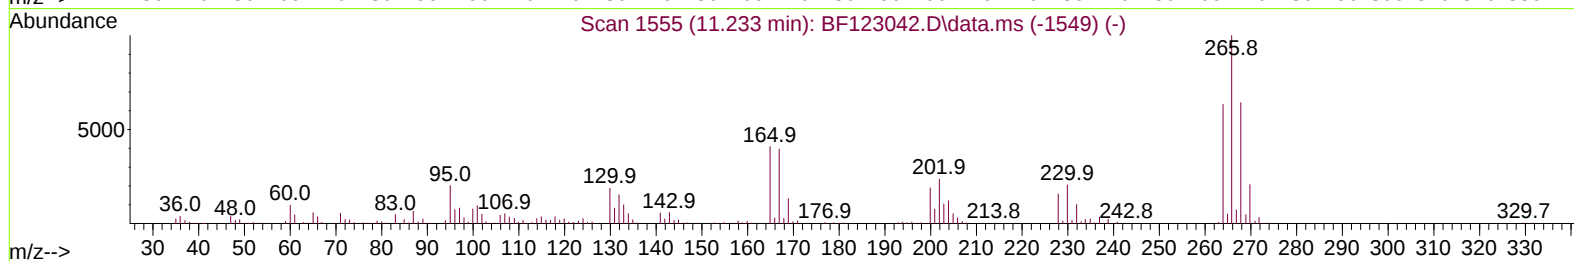
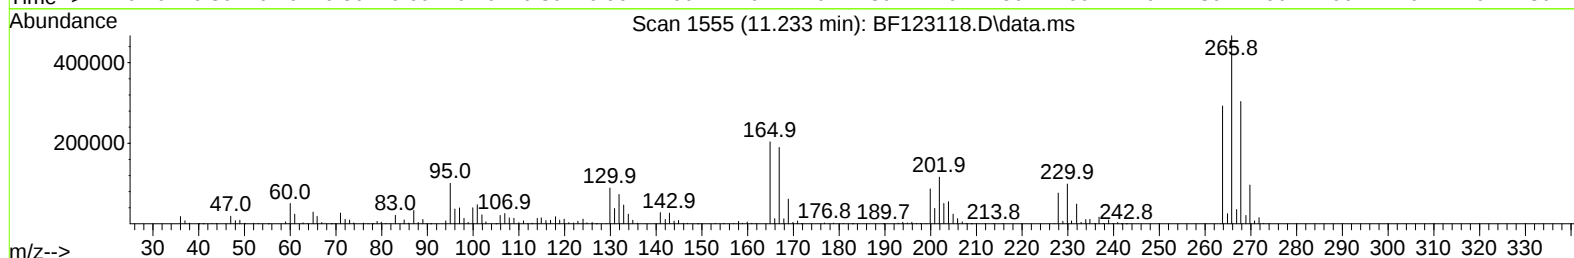


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020421\
 Data File : BF123118.D
 Acq On : 4 Feb 2021 17:37
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 05 01:35:30 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 29 12:29:00 2021
 Response via : Initial Calibration

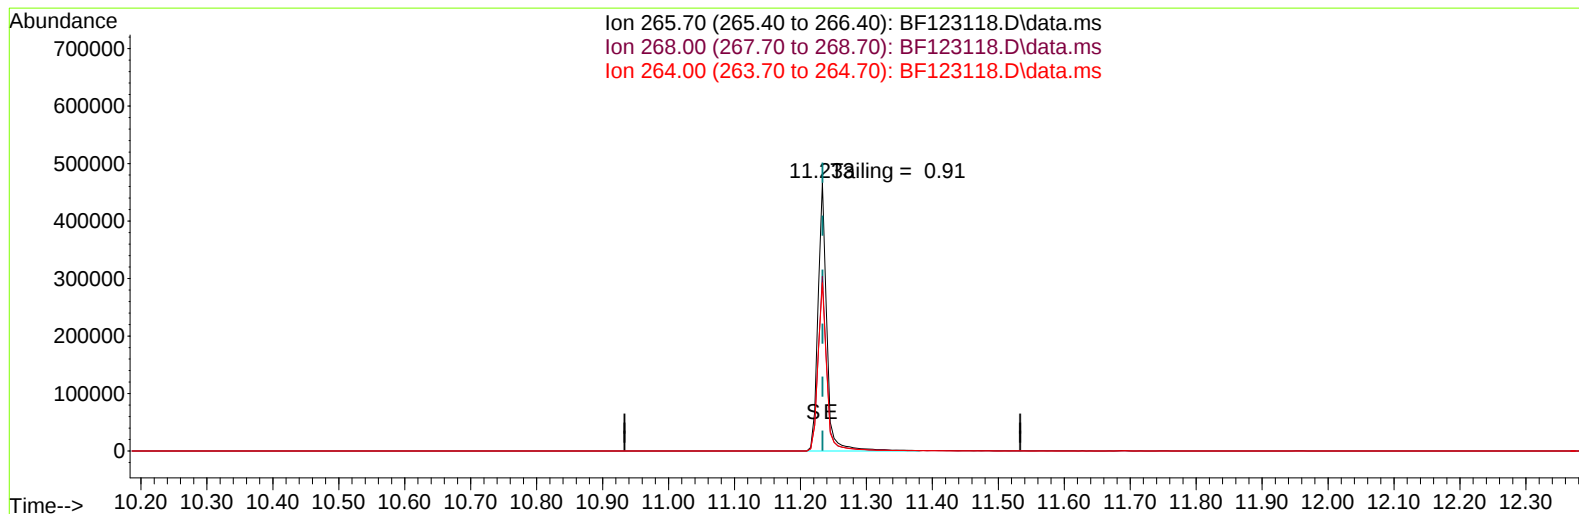

TIC: BF123118.D\data.ms

(70) Pentachlorophenol (C)




11.233min (-0.000) 34048.25 ng

response 434559

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	65.05
264.00	62.30	62.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020421\
 Data File : BF123118.D
 Acq On : 4 Feb 2021 17:37
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 05 01:35:30 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 29 12:29:00 2021
 Response via : Initial Calibration

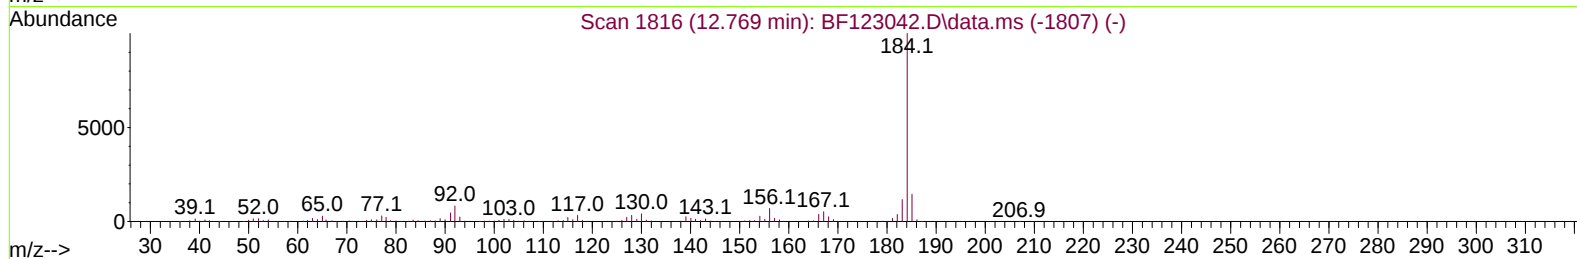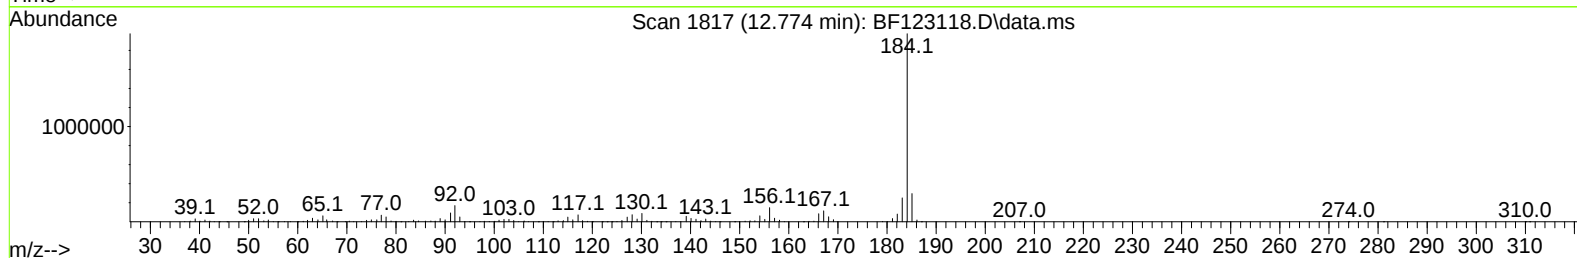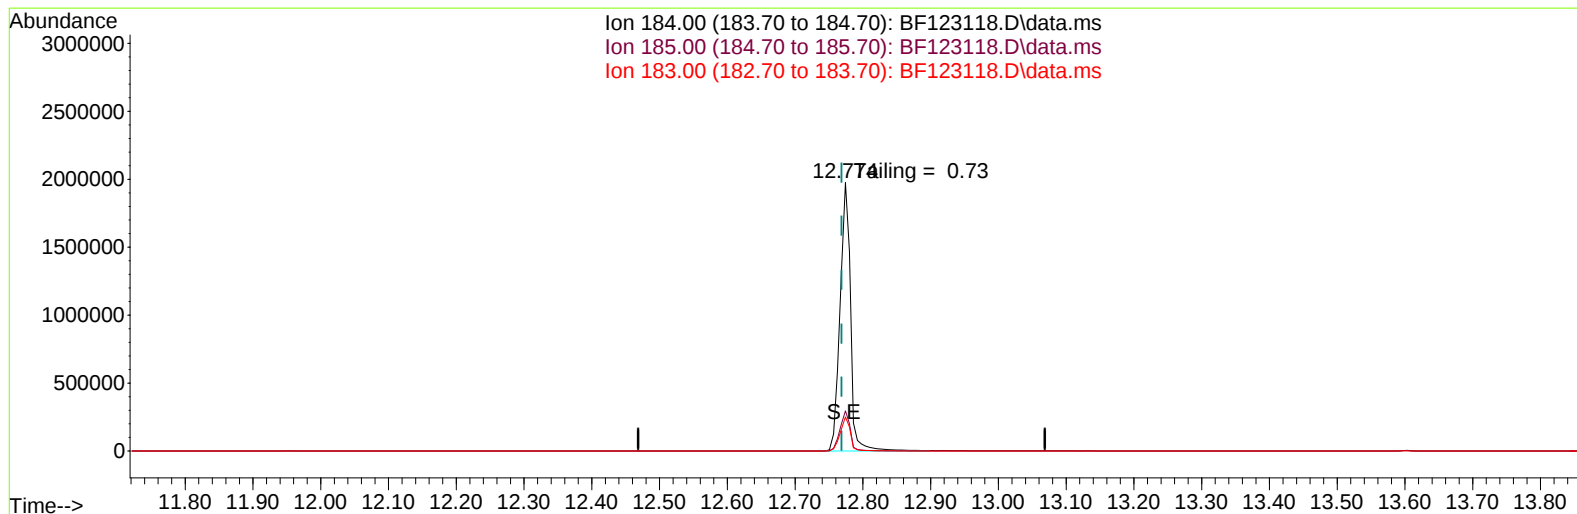

TIC: BF123118.D\data.ms

(77) Benzidine

12.774min (+ 0.006) 613669.23 ng m

response 2110790

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.97
183.00	12.10	12.70
0.00	0.00	0.00