

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020421\
 Data File : BF123108.D
 Acq On : 4 Feb 2021 11:19
 Operator : JU/CG
 Sample : PB134405BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB134405BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF123108.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.522	578	584	587	rBV	6324199	6571507	67.09%	11.920%
2	6.516	747	753	756	rBV	5648097	6581646	67.19%	11.938%
3	6.893	813	817	820	rBV	1951312	1618701	16.53%	2.936%
4	7.451	906	912	915	rBV	3980181	4506356	46.01%	8.174%
5	8.175	1030	1035	1038	rBV	2308478	2150050	21.95%	3.900%
6	9.257	1212	1219	1222	rBV	7144946	8110411	82.80%	14.711%
7	9.934	1328	1334	1338	rBV	2561758	2530282	25.83%	4.590%
8	10.728	1462	1469	1497	rBV	4945879	5597970	57.15%	10.154%
9	11.428	1581	1588	1591	rBV	2697875	2667065	27.23%	4.838%
10	13.027	1852	1860	1863	rBV	8771554	9795337	100.00%	17.767%
11	14.074	2034	2038	2050	rBV	2701346	2685321	27.41%	4.871%
12	15.563	2285	2291	2307	rVB	1621610	2317122	23.66%	4.203%




Sum of corrected areas: 55131768

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020421\
Data File : BF123108.D
Acq On : 4 Feb 2021 11:19
Operator : JU/CG
Sample : PB134405BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB134405BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

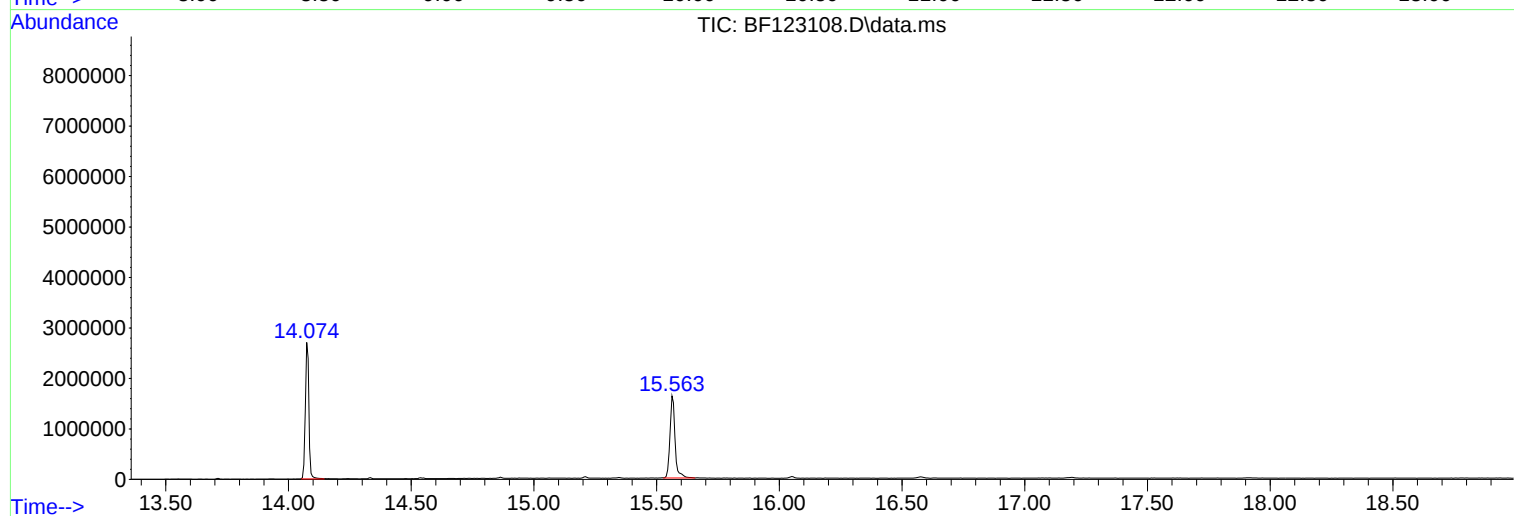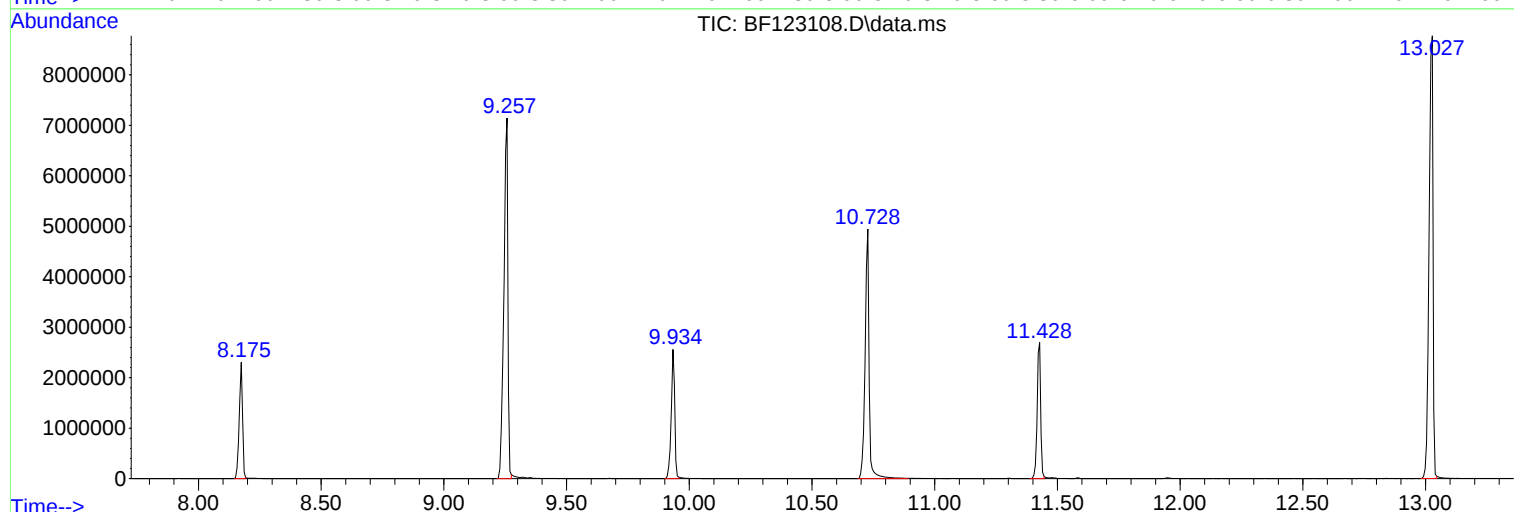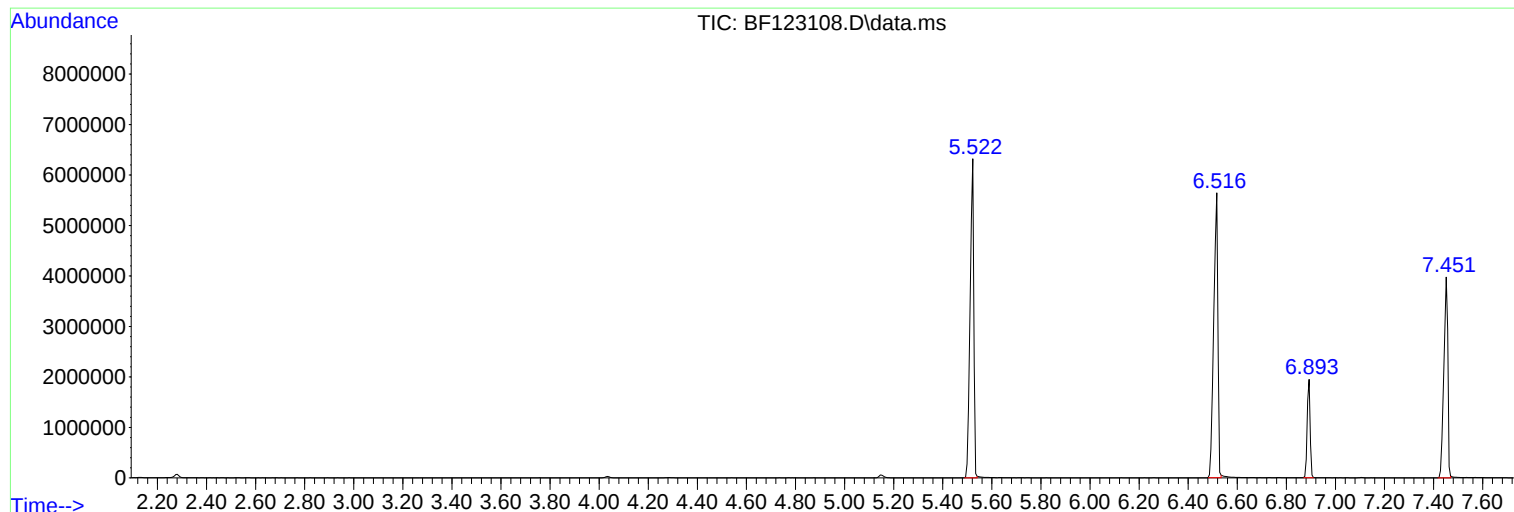

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020421\
Data File : BF123108.D
Acq On : 4 Feb 2021 11:19
Operator : JU/CG
Sample : PB134405BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB134405BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020421\
Data File : BF123108.D
Acq On : 4 Feb 2021 11:19
Operator : JU/CG
Sample : PB134405BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB134405BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------