

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020421\
 Data File : BF123111.D
 Acq On : 4 Feb 2021 12:59
 Operator : JU/CG
 Sample : M1291-07
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU421-006-0510

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF123111.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.181	7	16	23	rBV	559730	715076	11.61%	1.546%
2	5.116	510	515	520	rVB	68681	87836	1.43%	0.190%
3	5.510	577	582	585	rBV	4765308	4630641	75.21%	10.013%
4	6.516	747	753	766	rBV	4496316	4800366	77.97%	10.380%
5	6.892	813	817	820	rBV	1620744	1274293	20.70%	2.755%
6	7.451	907	912	915	rBV	3340984	3085557	50.12%	6.672%
7	8.175	1031	1035	1038	rBV	2036727	1683566	27.34%	3.640%
8	9.251	1213	1218	1222	rBV	5442451	5539228	89.97%	11.977%
9	9.527	1261	1265	1270	rBV	147412	124557	2.02%	0.269%
10	9.645	1281	1285	1289	rBV	237943	197361	3.21%	0.427%
11	9.933	1330	1334	1338	rBV	2278057	1969815	31.99%	4.259%
12	10.722	1463	1468	1480	rBV	3610585	3869082	62.84%	8.366%
13	11.080	1524	1529	1534	rBV6	42072	64606	1.05%	0.140%
14	11.427	1583	1588	1591	rBV	2295017	2054323	33.37%	4.442%
15	11.951	1672	1677	1693	rBV	1243790	1651235	26.82%	3.570%
16	12.663	1792	1798	1806	rBV6	66646	150540	2.45%	0.326%
17	12.745	1806	1812	1820	rVV	828650	999469	16.23%	2.161%
18	12.833	1824	1827	1831	rVB2	58230	73634	1.20%	0.159%
19	12.915	1839	1841	1848	rVB3	67245	87488	1.42%	0.189%
20	13.021	1854	1859	1862	rBV	6679519	6156824	100.00%	13.313%
21	13.115	1864	1875	1885	rVB3	183538	709543	11.52%	1.534%
22	13.251	1895	1898	1902	rVB	81592	72237	1.17%	0.156%
23	13.598	1954	1957	1959	rVB	113491	94883	1.54%	0.205%
24	13.927	2010	2013	2018	rVB2	168000	165475	2.69%	0.358%
25	13.992	2018	2024	2034	rBV2	166331	582716	9.46%	1.260%
26	14.074	2034	2038	2042	rVV	2076839	1860150	30.21%	4.022%
27	14.127	2042	2047	2060	rVV	249515	555436	9.02%	1.201%
28	14.245	2064	2067	2070	rVB	187015	154447	2.51%	0.334%
29	14.551	2116	2119	2123	rVB	176458	154509	2.51%	0.334%
30	14.845	2164	2169	2170	rBV2	204673	259088	4.21%	0.560%
31	14.862	2170	2172	2176	rVB	234583	248586	4.04%	0.538%
32	14.939	2182	2185	2189	rVB	79280	85187	1.38%	0.184%
33	15.209	2228	2231	2238	rVB	132258	155757	2.53%	0.337%
34	15.562	2286	2291	2295	rBV	1135852	1446444	23.49%	3.128%
35	15.598	2295	2297	2305	rVB	150577	221846	3.60%	0.480%
36	16.051	2370	2374	2380	rVB2	89709	135519	2.20%	0.293%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020421\
Data File : BF123111.D
Acq On : 4 Feb 2021 12:59
Operator : JU/CG
Sample : M1291-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU421-006-0510

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	16.574	2460	2463	2475	rVB4	61482	130651	2.12%	0.283%
----	--------	------	------	------	------	-------	--------	-------	--------




Sum of corrected areas: 46247971

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020421\
Data File : BF123111.D
Acq On : 4 Feb 2021 12:59
Operator : JU/CG
Sample : M1291-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU421-006-0510

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

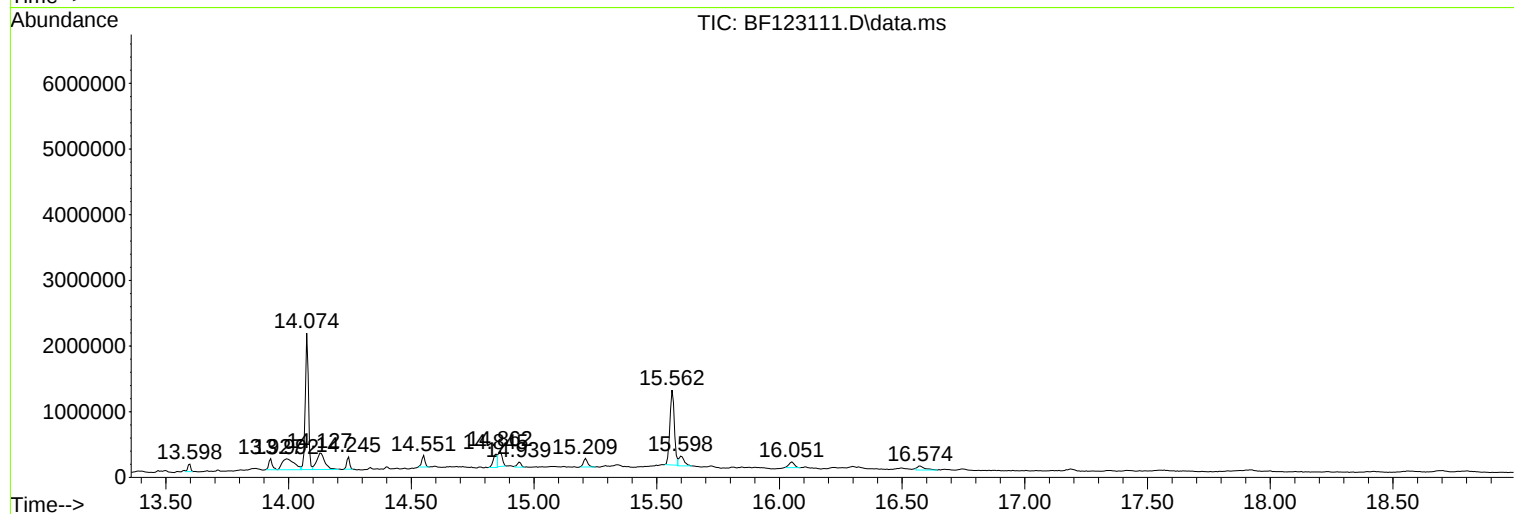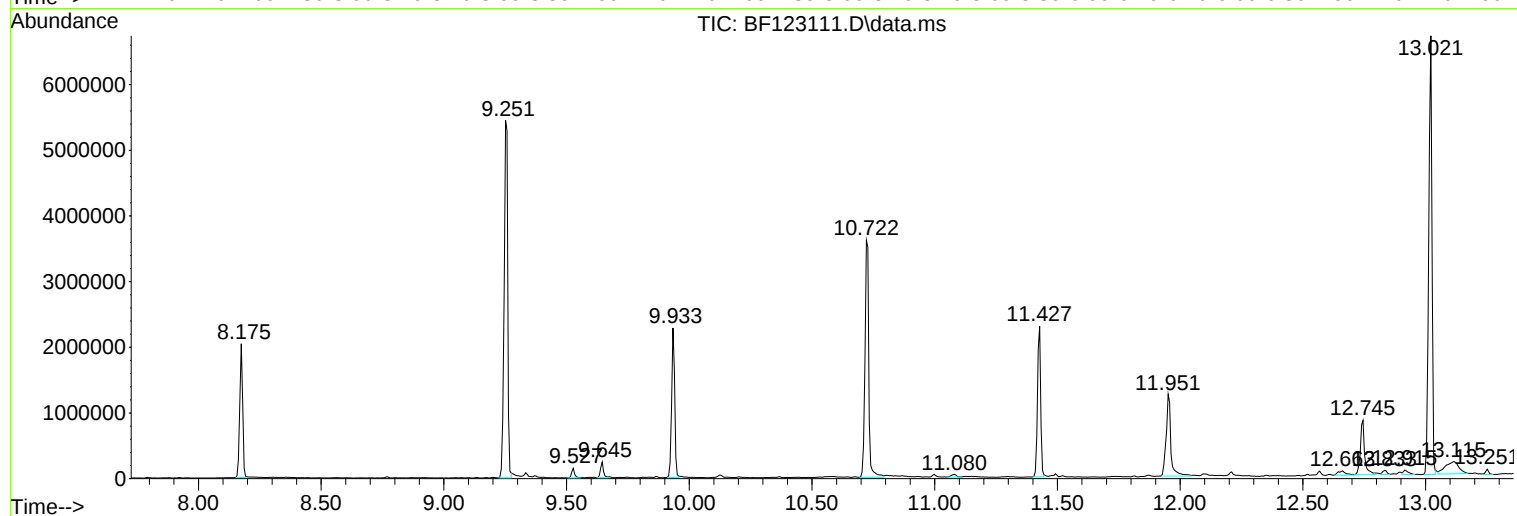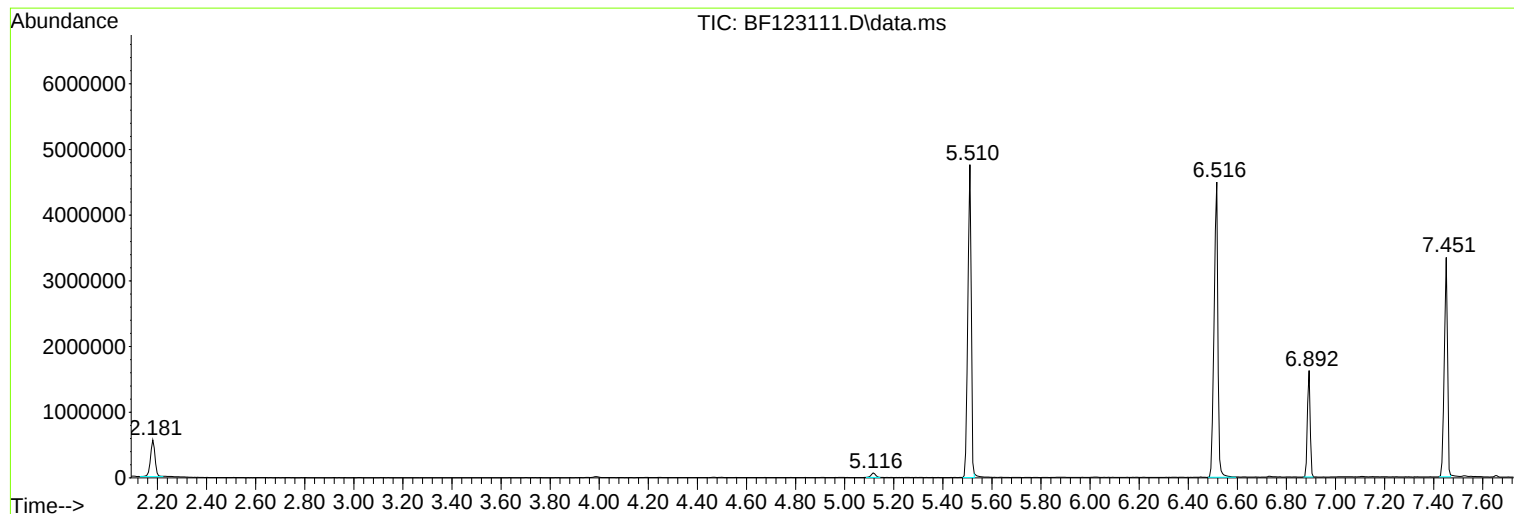

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020421\
Data File : BF123111.D
Acq On : 4 Feb 2021 12:59
Operator : JU/CG
Sample : M1291-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU421-006-0510

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020421\
Data File : BF123111.D
Acq On : 4 Feb 2021 12:59
Operator : JU/CG
Sample : M1291-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU421-006-0510

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------