

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020421\
 Data File : BF123112.D
 Acq On : 4 Feb 2021 13:32
 Operator : JU/CG
 Sample : M1291-06
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU421-006-0205

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF123112.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.193	10	18	24	rBV	629104	808687	13.57%	1.904%
2	5.122	508	516	521	rBV	61723	79825	1.34%	0.188%
3	5.510	577	582	585	rBV	4816230	4640534	77.90%	10.926%
4	6.516	747	753	769	rBV	4467425	4817830	80.87%	11.344%
5	6.892	813	817	820	rBV	1633626	1305313	21.91%	3.073%
6	7.451	907	912	915	rBV	3287300	3074838	51.62%	7.240%
7	8.175	1031	1035	1039	rBV	2053897	1728201	29.01%	4.069%
8	9.251	1213	1218	1222	rBV	5384387	5473243	91.88%	12.887%
9	9.645	1281	1285	1289	rBV	170299	144095	2.42%	0.339%
10	9.933	1330	1334	1338	rBV	2268476	1986785	33.35%	4.678%
11	10.727	1463	1469	1481	rBV	3464406	3790462	63.63%	8.925%
12	11.427	1583	1588	1591	rBV	2396843	2059749	34.58%	4.850%
13	11.951	1671	1677	1690	rBV	856030	997370	16.74%	2.348%
14	12.739	1808	1811	1820	rBV	356384	390141	6.55%	0.919%
15	13.021	1854	1859	1862	rBV	6433580	5957215	100.00%	14.027%
16	13.716	1973	1977	1980	rBV	124270	105620	1.77%	0.249%
17	13.980	2015	2022	2034	rBV5	210914	878596	14.75%	2.069%
18	14.074	2034	2038	2042	rVV	1943838	1783161	29.93%	4.199%
19	14.110	2042	2044	2051	rVB2	105886	102339	1.72%	0.241%
20	14.245	2064	2067	2072	rVB	72739	69759	1.17%	0.164%
21	14.374	2086	2089	2092	rVB	161442	145640	2.44%	0.343%
22	14.421	2094	2097	2100	rVB2	144490	132492	2.22%	0.312%
23	14.551	2114	2119	2123	rVB2	78867	92402	1.55%	0.218%
24	14.792	2157	2160	2166	rVB4	81138	76378	1.28%	0.180%
25	14.862	2170	2172	2175	rVB	74271	64681	1.09%	0.152%
26	15.086	2207	2210	2213	rBV3	117158	123214	2.07%	0.290%
27	15.210	2228	2231	2240	rVB	80495	122927	2.06%	0.289%
28	15.562	2286	2291	2295	rBV	1133657	1419902	23.83%	3.343%
29	16.051	2370	2374	2379	rBV2	58098	99624	1.67%	0.235%




Sum of corrected areas: 42471023

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020421\
Data File : BF123112.D
Acq On : 4 Feb 2021 13:32
Operator : JU/CG
Sample : M1291-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU421-006-0205

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

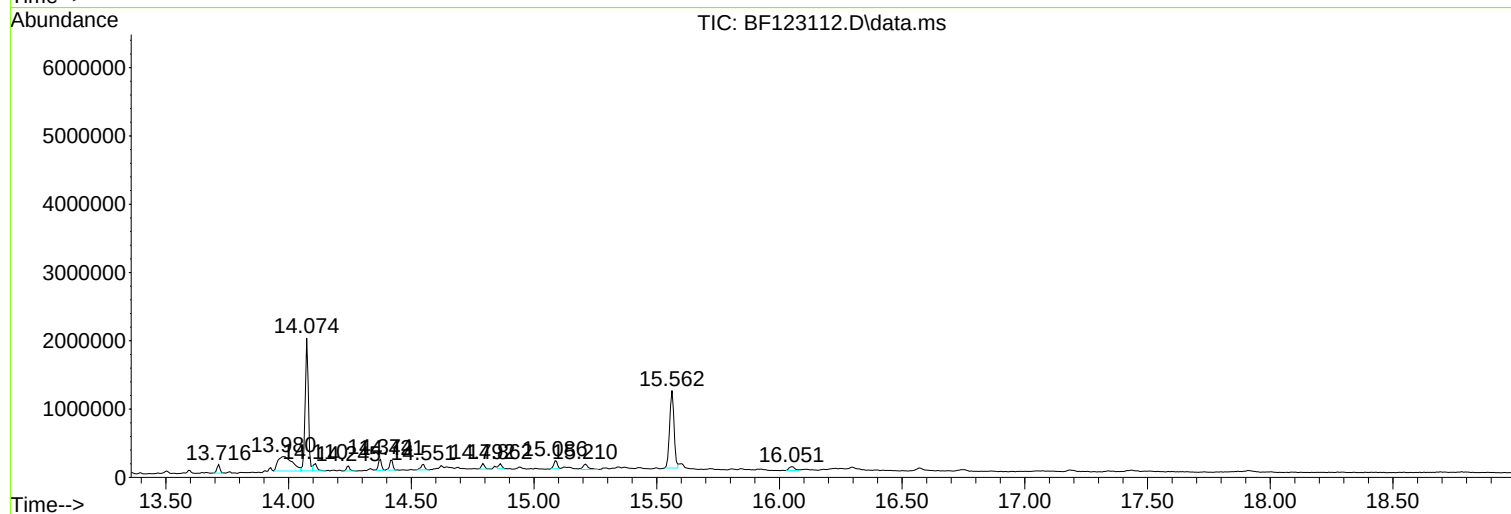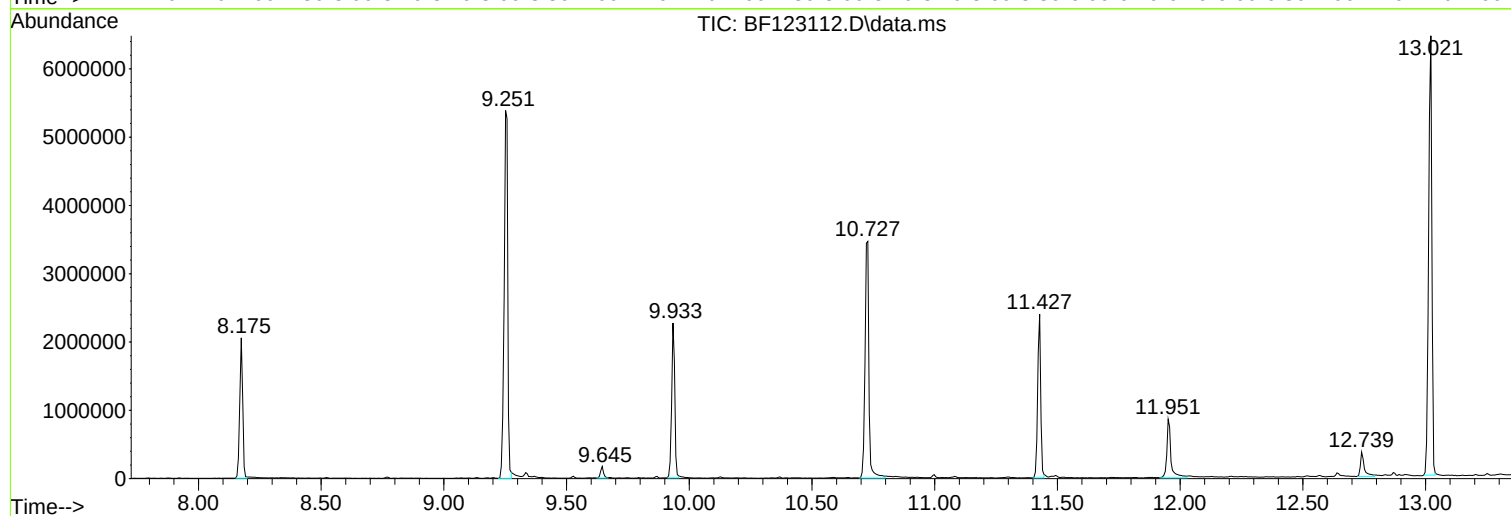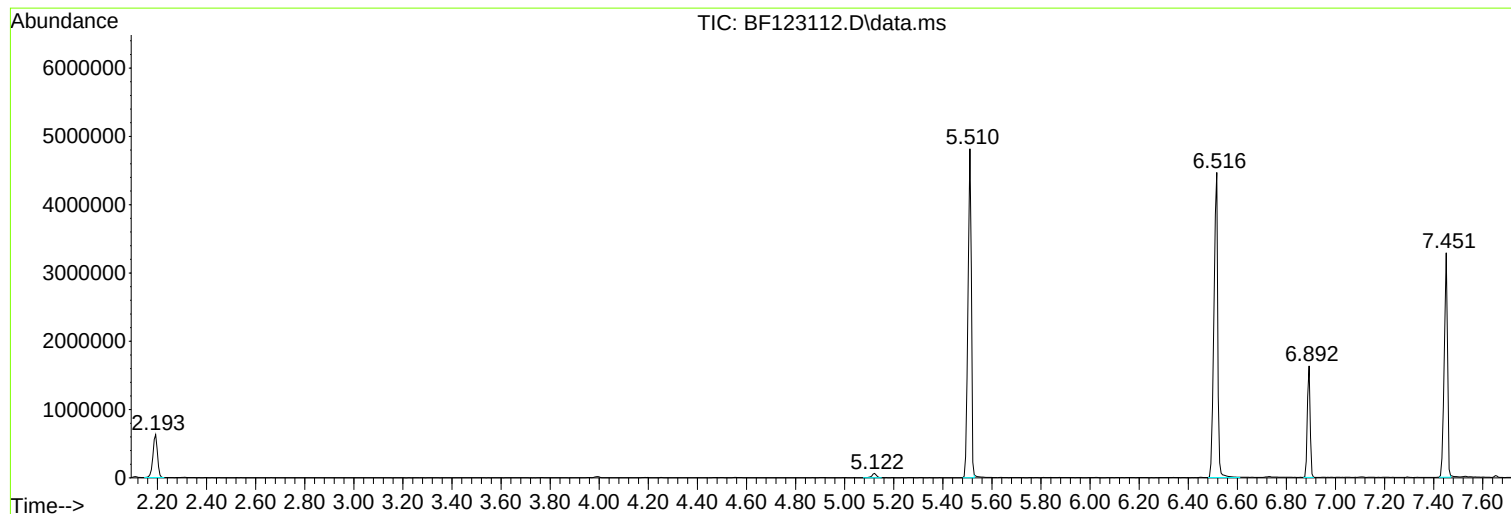

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020421\
Data File : BF123112.D
Acq On : 4 Feb 2021 13:32
Operator : JU/CG
Sample : M1291-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU421-006-0205

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020421\
Data File : BF123112.D
Acq On : 4 Feb 2021 13:32
Operator : JU/CG
Sample : M1291-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU421-006-0205

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
