

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020421\
 Data File : BF123113.D
 Acq On : 4 Feb 2021 14:04
 Operator : JU/CG
 Sample : M1291-22
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU421-005-0205

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF123113.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.157	6	12	18	rVB	504907	627614	8.19%	0.423%
2	5.510	574	582	585	rBV	4037658	4375324	57.11%	2.948%
3	6.516	745	753	757	rBV	4028821	4409561	57.55%	2.971%
4	6.722	784	788	792	rBV2	322280	472927	6.17%	0.319%
5	6.892	813	817	824	rVB	1638766	1371318	17.90%	0.924%
6	7.139	854	859	862	rBV	217144	207562	2.71%	0.140%
7	7.287	880	884	887	rBV2	141576	167437	2.19%	0.113%
8	7.451	903	912	915	rBV	3004310	2958596	38.62%	1.994%
9	7.492	916	919	923	rVV	479057	395338	5.16%	0.266%
10	7.822	969	975	979	rBV6	185093	290489	3.79%	0.196%
11	7.922	989	992	995	rBV4	130142	159672	2.08%	0.108%
12	7.957	995	998	1002	rVV	299816	292943	3.82%	0.197%
13	8.175	1029	1035	1038	rBV	1978956	1950765	25.46%	1.315%
14	8.234	1042	1045	1049	rVB2	620515	515873	6.73%	0.348%
15	8.528	1091	1095	1098	rVB	1290698	1112655	14.52%	0.750%
16	8.604	1103	1108	1110	rVV3	206509	224314	2.93%	0.151%
17	8.769	1131	1136	1141	rBV3	373700	390668	5.10%	0.263%
18	8.892	1154	1157	1165	rVB2	275122	281655	3.68%	0.190%
19	8.986	1171	1173	1177	rVB2	168374	166811	2.18%	0.112%
20	9.198	1203	1209	1213	rVB3	225473	349497	4.56%	0.236%
21	9.257	1214	1219	1222	rBV	5130191	4916543	64.17%	3.313%
22	9.333	1229	1232	1234	rBV	275787	243074	3.17%	0.164%
23	9.592	1272	1276	1278	rBV2	179675	208212	2.72%	0.140%
24	9.616	1278	1280	1283	rVB2	251311	203997	2.66%	0.137%
25	9.645	1283	1285	1290	rBV2	215671	306858	4.01%	0.207%
26	9.869	1320	1323	1325	rVB	245246	179677	2.35%	0.121%
27	9.933	1328	1334	1338	rBV	2060579	1908470	24.91%	1.286%
28	10.133	1364	1368	1373	rVB3	219890	269869	3.52%	0.182%
29	10.233	1381	1385	1387	rBV	179244	209595	2.74%	0.141%
30	10.369	1405	1408	1411	rVB	261641	206580	2.70%	0.139%
31	10.580	1439	1444	1450	rBV2	677417	780678	10.19%	0.526%
32	10.639	1451	1454	1458	rVB2	290180	264398	3.45%	0.178%
33	10.727	1464	1469	1472	rBV	3087564	3043368	39.72%	2.051%
34	10.775	1472	1477	1480	rVV	646212	593753	7.75%	0.400%
35	10.845	1486	1489	1493	rBV3	401018	481897	6.29%	0.325%
36	11.022	1516	1519	1523	rVV3	143788	154978	2.02%	0.104%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020421\
 Data File : BF123113.D
 Acq On : 4 Feb 2021 14:04
 Operator : JU/CG
 Sample : M1291-22
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU421-005-0205

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	11.427	1584	1588	1590	rBV	2077485	1713282	22.36%	1.155%
38	11.722	1635	1638	1639	rBV2	241351	184144	2.40%	0.124%
39	11.739	1639	1641	1644	rVV2	241274	225672	2.95%	0.152%
40	11.774	1644	1647	1650	rVB	870471	678607	8.86%	0.457%
41	11.822	1652	1655	1658	rVB2	202293	156480	2.04%	0.105%
42	11.980	1675	1682	1687	rVV2	4947345	7437283	97.07%	5.012%
43	12.098	1700	1702	1703	rBV	368913	261219	3.41%	0.176%
44	12.122	1703	1706	1716	rVV2	1200538	1983797	25.89%	1.337%
45	12.216	1719	1722	1724	rVV3	428738	466519	6.09%	0.314%
46	12.251	1724	1728	1736	rVB	3682119	4101880	53.54%	2.764%
47	12.380	1748	1750	1757	rVB2	546846	737428	9.62%	0.497%
48	12.480	1763	1767	1769	rBV	1109479	1364676	17.81%	0.920%
49	12.504	1769	1771	1776	rVV2	1906805	2243501	29.28%	1.512%
50	12.545	1776	1778	1780	rVV2	295562	227980	2.98%	0.154%
51	12.592	1784	1786	1788	rVB2	215060	158360	2.07%	0.107%
52	12.651	1794	1796	1797	rBV	231875	188682	2.46%	0.127%
53	12.692	1797	1803	1807	rVV2	2279180	3618109	47.22%	2.438%
54	12.769	1810	1816	1820	rVV2	5773752	7661697	100.00%	5.163%
55	12.810	1821	1823	1829	rVV5	698731	849040	11.08%	0.572%
56	12.857	1829	1831	1833	rVV	540612	374136	4.88%	0.252%
57	12.939	1842	1845	1847	rBV	318381	298080	3.89%	0.201%
58	13.021	1856	1859	1866	rVB	4493079	4645478	60.63%	3.130%
59	13.116	1873	1875	1879	rVB3	414113	468961	6.12%	0.316%
60	13.163	1880	1883	1886	rVB	1592850	1288221	16.81%	0.868%
61	13.210	1888	1891	1895	rVB2	705359	613617	8.01%	0.413%
62	13.257	1896	1899	1901	rVV2	339807	297982	3.89%	0.201%
63	13.368	1915	1918	1921	rBV	2635059	2001803	26.13%	1.349%
64	13.398	1921	1923	1927	rVB2	1057113	967546	12.63%	0.652%
65	13.474	1934	1936	1938	rBV	414040	379497	4.95%	0.256%
66	13.510	1939	1942	1944	rVV	1427552	1419753	18.53%	0.957%
67	13.533	1944	1946	1949	rVB	702007	559645	7.30%	0.377%
68	13.568	1950	1952	1953	rBV2	216907	158785	2.07%	0.107%
69	13.592	1953	1956	1963	rVB2	604134	895376	11.69%	0.603%
70	13.651	1964	1966	1969	rVB	447534	374241	4.88%	0.252%
71	13.698	1972	1974	1975	rVV	255514	196207	2.56%	0.132%
72	13.727	1975	1979	1982	rVB	5118399	4769730	62.25%	3.214%
73	13.768	1983	1986	1988	rVV	1125518	954226	12.45%	0.643%
74	13.857	1998	2001	2004	rBV	1458952	1724163	22.50%	1.162%
75	13.910	2007	2010	2015	rVV4	1944304	2896620	37.81%	1.952%
76	13.963	2015	2019	2026	rVB3	3246576	3881179	50.66%	2.615%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020421\
 Data File : BF123113.D
 Acq On : 4 Feb 2021 14:04
 Operator : JU/CG
 Sample : M1291-22
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU421-005-0205

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	14.021	2026	2029	2033	rVB	1140388	1075554	14.04%	0.725%
78	14.086	2036	2040	2042	rVB	1360214	1276886	16.67%	0.860%
79	14.121	2042	2046	2048	rBV	4614188	3966937	51.78%	2.673%
80	14.145	2048	2050	2055	rVB	386141	332616	4.34%	0.224%
81	14.215	2059	2062	2065	rBV3	778429	723756	9.45%	0.488%
82	14.339	2080	2083	2085	rBV2	351279	404501	5.28%	0.273%
83	14.386	2086	2091	2094	rVV	7185282	7483039	97.67%	5.043%
84	14.433	2094	2099	2102	rVB	7111716	6824280	89.07%	4.599%
85	14.557	2117	2120	2122	rBV	249389	255199	3.33%	0.172%
86	14.598	2124	2127	2130	rVV2	488613	839963	10.96%	0.566%
87	14.633	2130	2133	2135	rVV	2041579	2132615	27.83%	1.437%
88	14.651	2135	2136	2141	rVV2	894197	700060	9.14%	0.472%
89	14.698	2141	2144	2147	rVB	963134	869036	11.34%	0.586%
90	14.774	2155	2157	2159	rBV	327516	381418	4.98%	0.257%
91	14.804	2159	2162	2167	rVB	4266014	4397531	57.40%	2.963%
92	15.110	2208	2214	2217	rBV	5888223	6968811	90.96%	4.696%
93	15.374	2256	2259	2266	rVB2	579433	654891	8.55%	0.441%
94	15.574	2289	2293	2297	rVB	1038861	1214493	15.85%	0.818%
95	15.780	2324	2328	2332	rBV2	258901	549190	7.17%	0.370%
96	15.851	2337	2340	2345	rVB	628402	860465	11.23%	0.580%
97	16.051	2367	2374	2379	rBV	1621664	3444293	44.95%	2.321%
98	16.198	2395	2399	2405	rVB2	443892	803895	10.49%	0.542%
99	16.457	2437	2443	2458	rBV	1043119	2849232	37.19%	1.920%
100	17.751	2657	2663	2677	rBV5	385233	1271576	16.60%	0.857%


Sum of corrected areas: 148396805

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020421\
Data File : BF123113.D
Acq On : 4 Feb 2021 14:04
Operator : JU/CG
Sample : M1291-22
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU421-005-0205

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

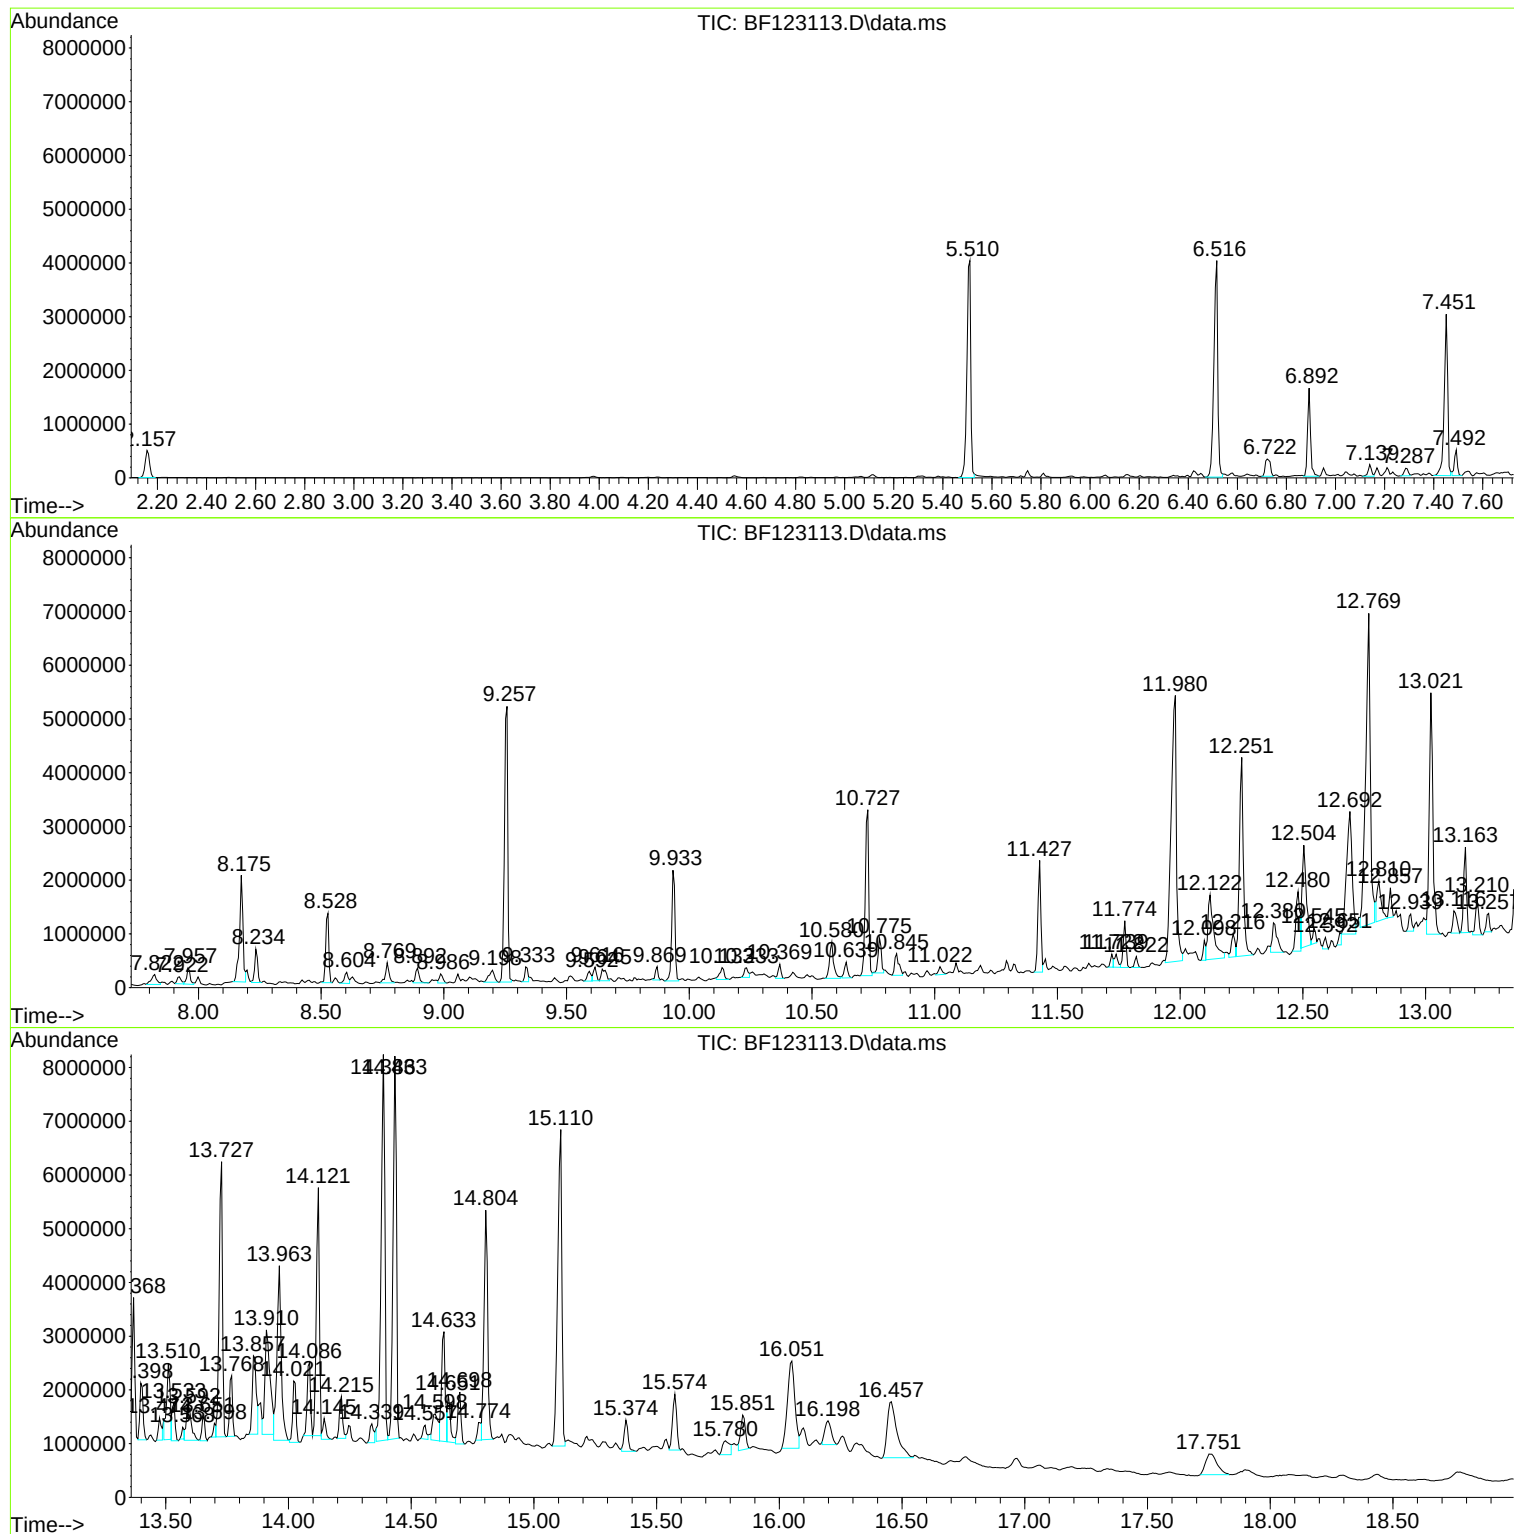

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020421\
Data File : BF123113.D
Acq On : 4 Feb 2021 14:04
Operator : JU/CG
Sample : M1291-22
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU421-005-0205

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020421\
Data File : BF123113.D
Acq On : 4 Feb 2021 14:04
Operator : JU/CG
Sample : M1291-22
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU421-005-0205

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------