

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020421\
 Data File : BF123115.D
 Acq On : 4 Feb 2021 15:10
 Operator : JU/CG
 Sample : M1291-10
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU421-008-0002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF123115.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.204	11	20	25	rBV	402440	533164	10.39%	1.352%
2	5.128	509	517	523	rBV	64849	91727	1.79%	0.233%
3	5.516	577	583	586	rBV	4400078	4349986	84.78%	11.034%
4	6.516	747	753	756	rBV	4267874	4439847	86.53%	11.261%
5	6.892	813	817	820	rBV	1741237	1344576	26.20%	3.410%
6	7.451	907	912	915	rBV	2958269	2902937	56.58%	7.363%
7	8.175	1031	1035	1039	rBV	1979113	1759453	34.29%	4.463%
8	9.257	1213	1219	1222	rBV	5562865	5131046	100.00%	13.015%
9	9.333	1228	1232	1235	rBV2	55236	55757	1.09%	0.141%
10	9.645	1282	1285	1289	rBV	157385	129946	2.53%	0.330%
11	9.939	1330	1335	1338	rBV	2123550	2019179	39.35%	5.122%
12	10.727	1463	1469	1472	rBV	3522210	3240595	63.16%	8.220%
13	11.427	1584	1588	1591	rBV	2330947	1931714	37.65%	4.900%
14	11.957	1671	1678	1689	rBV	1456865	1576886	30.73%	4.000%
15	12.104	1699	1703	1710	rBV	65579	133148	2.59%	0.338%
16	12.233	1718	1725	1733	rBV3	134341	308345	6.01%	0.782%
17	12.645	1792	1795	1797	rBV	156618	150705	2.94%	0.382%
18	12.745	1807	1812	1820	rBV	830201	854072	16.65%	2.166%
19	12.874	1831	1834	1835	rBV	88618	80609	1.57%	0.204%
20	13.021	1854	1859	1862	rBV	5209134	4684481	91.30%	11.882%
21	13.251	1896	1898	1904	rVB	79201	85422	1.66%	0.217%
22	13.598	1955	1957	1959	rVB	90580	67602	1.32%	0.171%
23	13.939	2011	2015	2024	rVB3	341056	584279	11.39%	1.482%
24	14.080	2034	2039	2042	rBV	1594788	1591058	31.01%	4.036%
25	14.245	2065	2067	2071	rBV	101181	92801	1.81%	0.235%
26	15.568	2288	2292	2296	rVB	1116092	1285798	25.06%	3.261%




Sum of corrected areas: 39425133

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020421\
Data File : BF123115.D
Acq On : 4 Feb 2021 15:10
Operator : JU/CG
Sample : M1291-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU421-008-0002

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

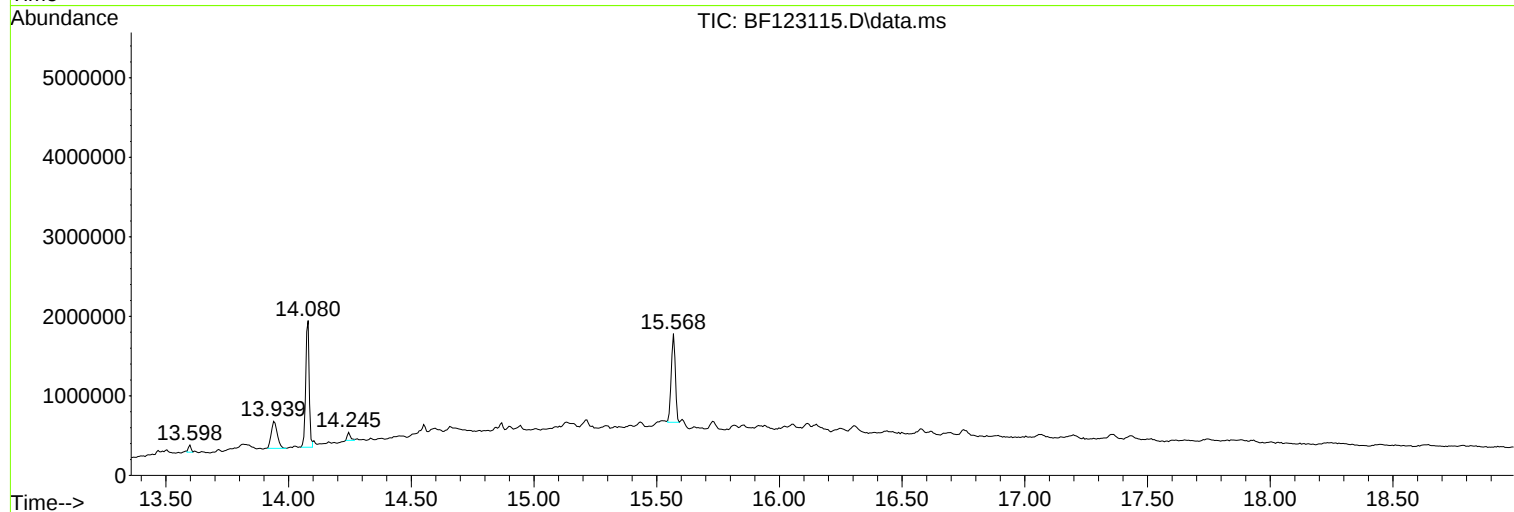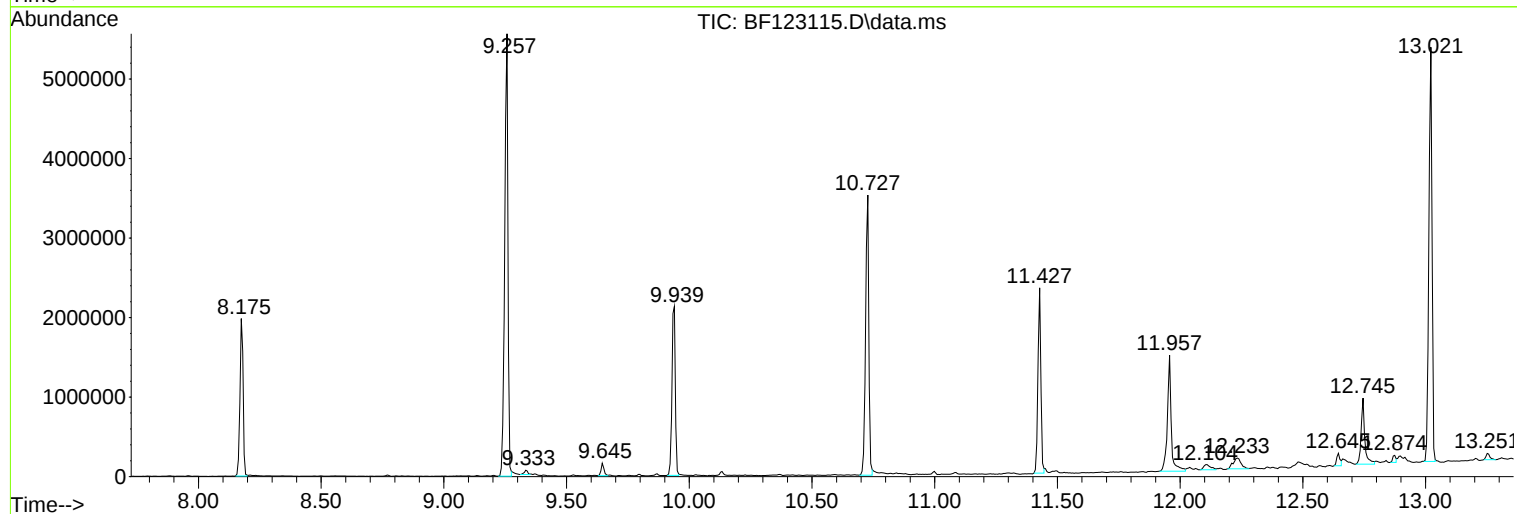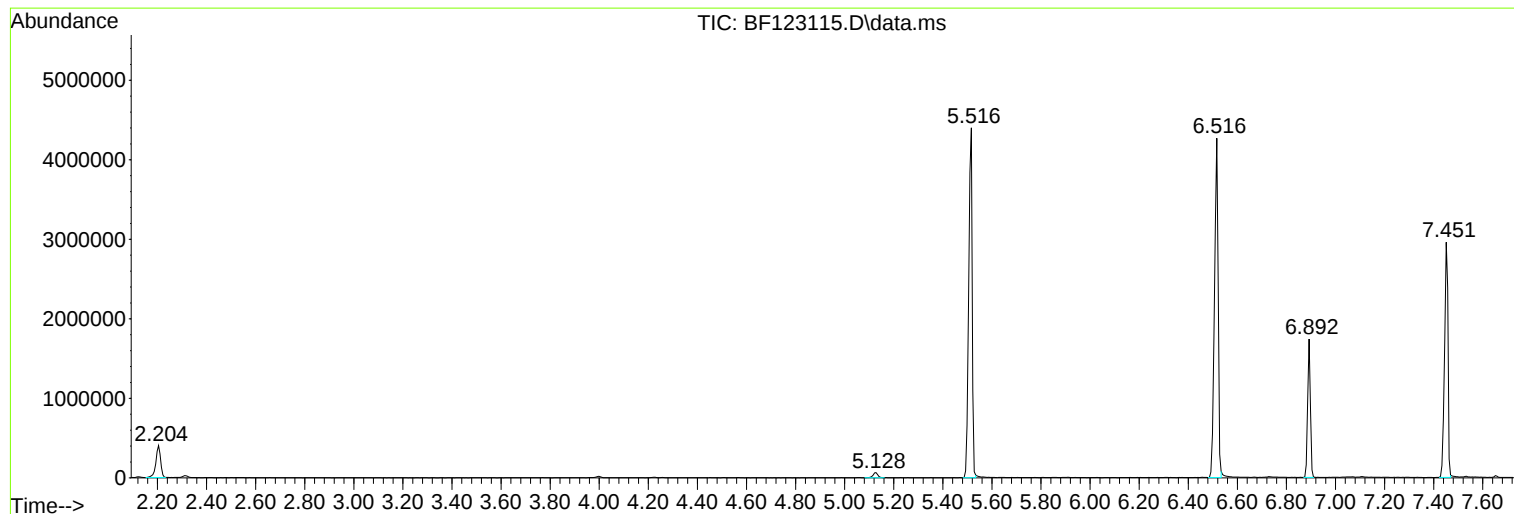

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020421\
Data File : BF123115.D
Acq On : 4 Feb 2021 15:10
Operator : JU/CG
Sample : M1291-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU421-008-0002

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020421\
Data File : BF123115.D
Acq On : 4 Feb 2021 15:10
Operator : JU/CG
Sample : M1291-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU421-008-0002

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------