

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020421\
 Data File : BF123116.D
 Acq On : 4 Feb 2021 15:43
 Operator : JU/CG
 Sample : M1291-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU421-006-0002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF123116.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.157	6	12	19	rVB	519557	667899	13.56%	1.754%
2	5.116	510	515	521	rBV	104274	136519	2.77%	0.359%
3	5.510	577	582	585	rBV	4502216	4369641	88.73%	11.478%
4	6.516	748	753	766	rBV	3925382	4445364	90.27%	11.677%
5	6.734	785	790	792	rBV2	65915	75315	1.53%	0.198%
6	6.892	814	817	820	rBV	1753985	1324007	26.89%	3.478%
7	7.457	904	913	915	rBV	2863416	2908176	59.06%	7.639%
8	7.492	915	919	923	rVB	118098	109365	2.22%	0.287%
9	8.175	1030	1035	1038	rBV	1864056	1779975	36.15%	4.676%
10	8.198	1038	1039	1043	rVB	83549	69112	1.40%	0.182%
11	8.539	1093	1097	1105	rVB2	74063	90311	1.83%	0.237%
12	8.769	1133	1136	1141	rVB	136642	109504	2.22%	0.288%
13	8.892	1154	1157	1159	rVB	86898	68550	1.39%	0.180%
14	9.257	1214	1219	1222	rBV	5778201	4924431	100.00%	12.936%
15	9.339	1229	1233	1235	rBV	179522	171181	3.48%	0.450%
16	9.528	1260	1265	1267	rBV2	78820	99492	2.02%	0.261%
17	9.592	1273	1276	1278	rBV2	75909	72046	1.46%	0.189%
18	9.645	1283	1285	1289	rBV2	217990	212224	4.31%	0.557%
19	9.798	1307	1311	1315	rBV	139741	150373	3.05%	0.395%
20	9.869	1318	1323	1325	rBV2	115977	101378	2.06%	0.266%
21	9.939	1328	1335	1338	rBV	2051353	1867473	37.92%	4.906%
22	10.139	1366	1369	1371	rVB2	72165	70063	1.42%	0.184%
23	10.369	1406	1408	1411	rVB	125118	87564	1.78%	0.230%
24	10.728	1464	1469	1472	rBV	3126559	2742449	55.69%	7.204%
25	10.857	1486	1491	1494	rBV3	176588	274819	5.58%	0.722%
26	11.292	1563	1565	1568	rBV	84488	69124	1.40%	0.182%
27	11.427	1585	1588	1591	rBV	1815801	1556506	31.61%	4.089%
28	11.451	1591	1592	1595	rVB	296195	168363	3.42%	0.442%
29	11.957	1675	1678	1685	rVB	1240099	1242269	25.23%	3.263%
30	12.645	1793	1795	1798	rBV	372499	295722	6.01%	0.777%
31	12.745	1809	1812	1816	rBV2	703059	746385	15.16%	1.961%
32	12.874	1832	1834	1837	rBV	370636	340616	6.92%	0.895%
33	13.021	1855	1859	1867	rVB	4314691	4207039	85.43%	11.051%
34	13.951	2014	2017	2024	rVB2	696712	954423	19.38%	2.507%
35	14.086	2036	2040	2043	rBV	1360505	1561168	31.70%	4.101%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020421\
Data File : BF123116.D
Acq On : 4 Feb 2021 15:43
Operator : JU/CG
Sample : M1291-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU421-006-0002

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION




Sum of corrected areas: 38068846

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020421\
Data File : BF123116.D
Acq On : 4 Feb 2021 15:43
Operator : JU/CG
Sample : M1291-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU421-006-0002

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

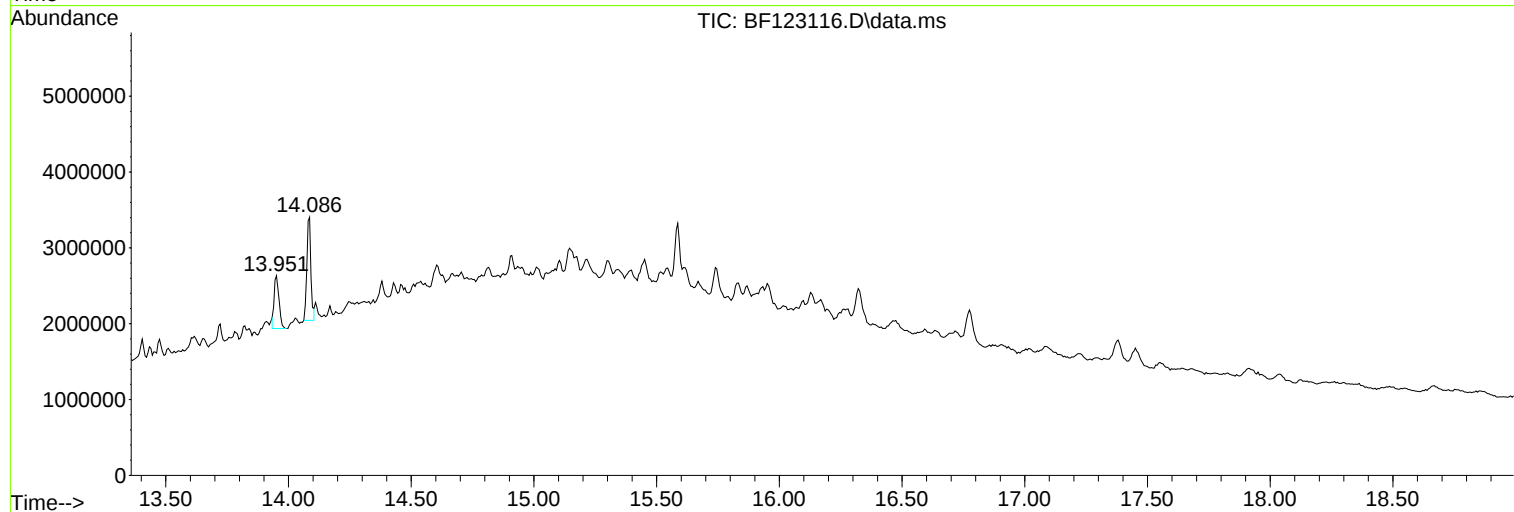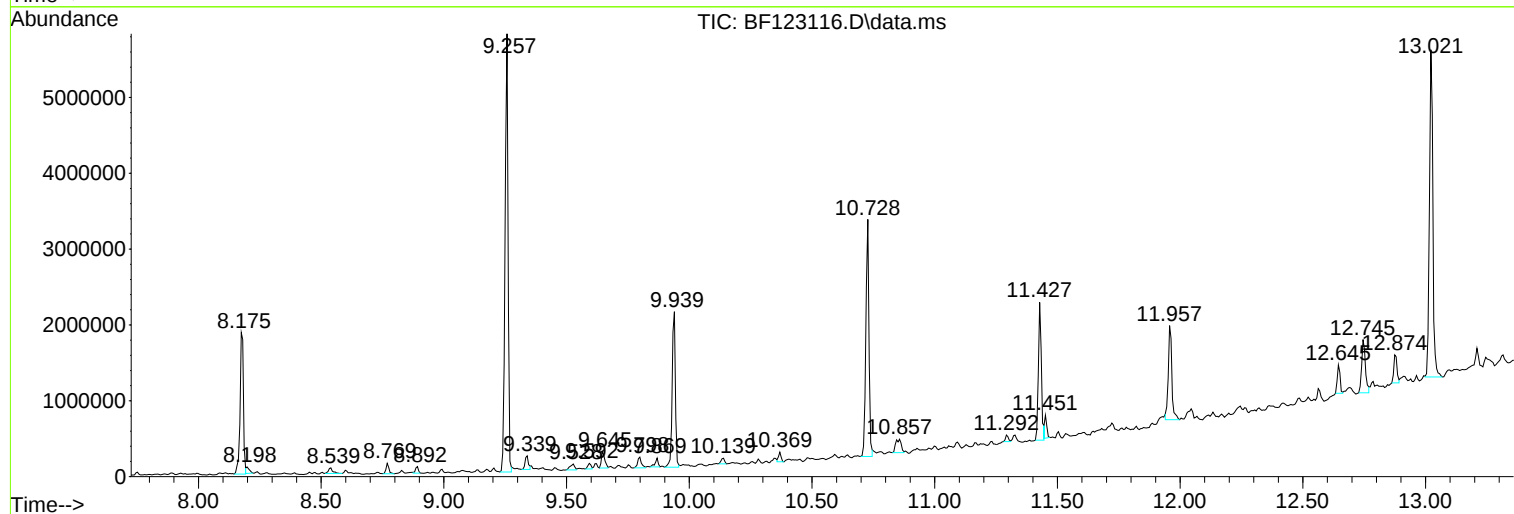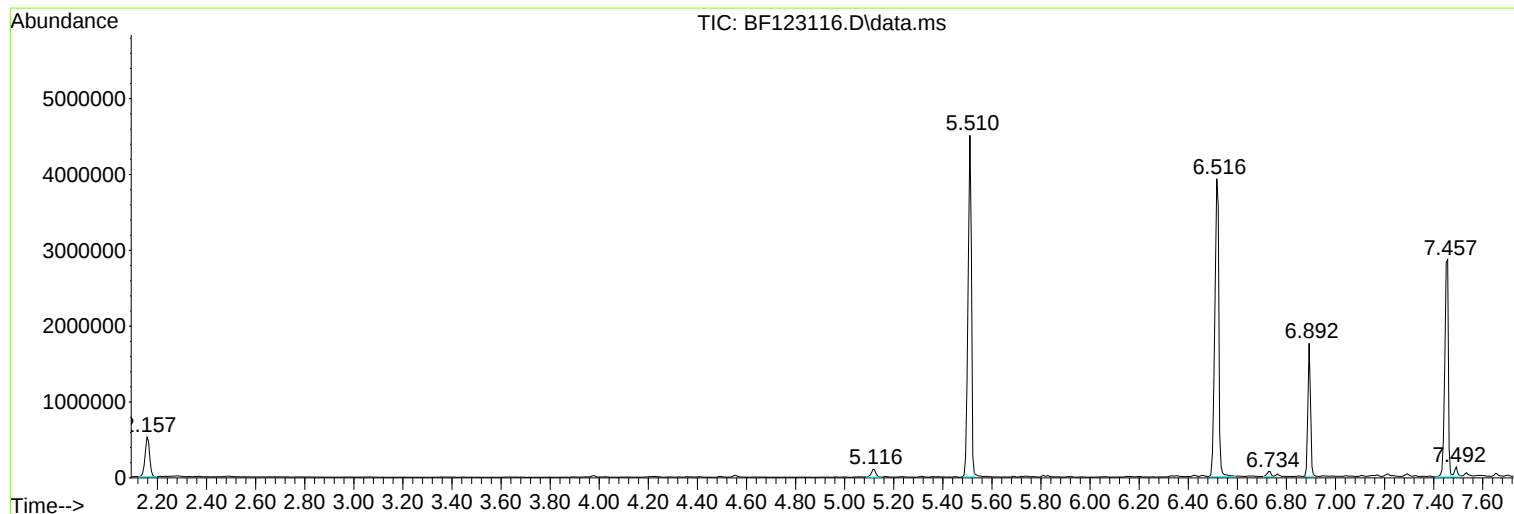

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020421\
Data File : BF123116.D
Acq On : 4 Feb 2021 15:43
Operator : JU/CG
Sample : M1291-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU421-006-0002

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020421\
Data File : BF123116.D
Acq On : 4 Feb 2021 15:43
Operator : JU/CG
Sample : M1291-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU421-006-0002

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------