
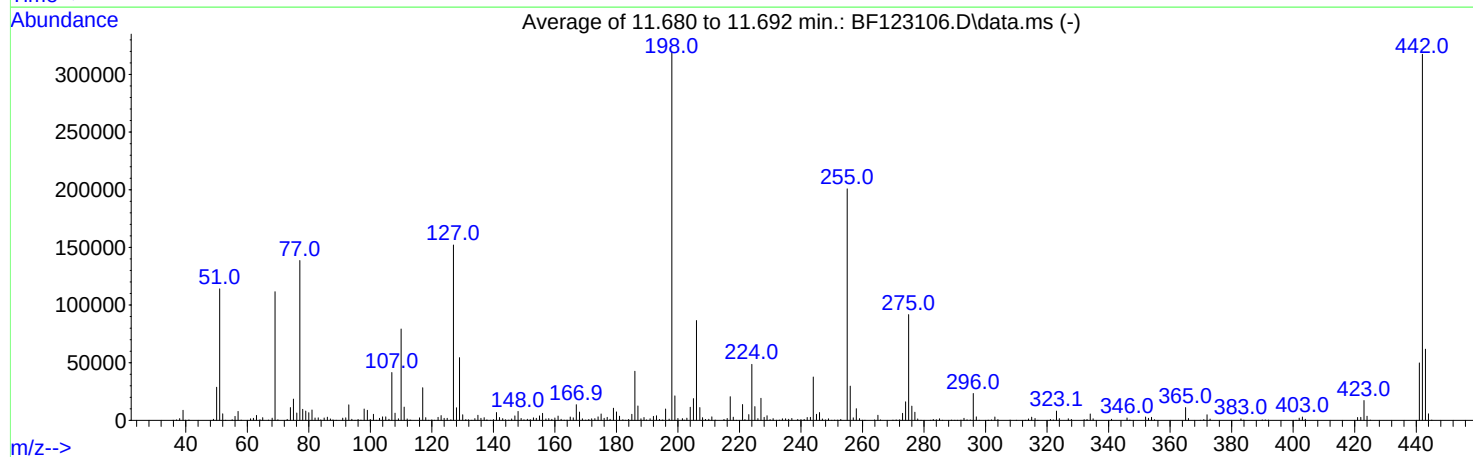


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020421\
 Data File : BF123106.D
 Acq On : 4 Feb 2021 9:19
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 29 12:29:00 2021

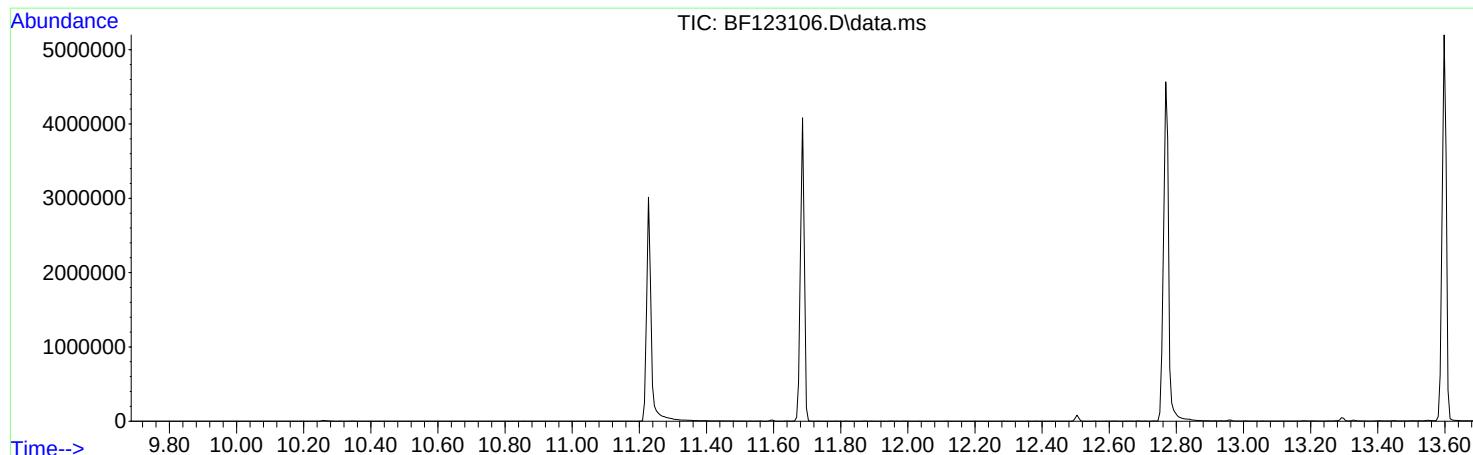

AutoFind: Scans 1631, 1632, 1633; Background Corrected with Scan 1625

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.8	114091	PASS
68	69	0.00	2	1.7	1893	PASS
69	198	0.00	100	35.0	111560	PASS
70	69	0.00	2	0.5	559	PASS
127	198	10	80	47.7	152163	PASS
197	198	0.00	2	0.3	1057	PASS
198	198	100	100	100.0	319040	PASS
199	198	5	9	6.6	21202	PASS
275	198	10	60	28.7	91680	PASS
365	198	1	100	3.5	11040	PASS
441	198	0.01	100	15.6	49875	PASS
442	442	50	100	100.0	317525	PASS
443	442	15	24	19.4	61755	PASS

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/4/2021	BNA_F	<u>BF123106.D</u>
Compound Name	Response	Retention Time
DDT	910150	13.598
DDD	11704	13.298
DDE	2796	12.957
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14500	924650	1.57

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020421\
 Data File : BF123106.D
 Acq On : 4 Feb 2021 9:19
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Feb 05 01:29:27 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 29 12:29:00 2021
 Response via : Initial Calibration

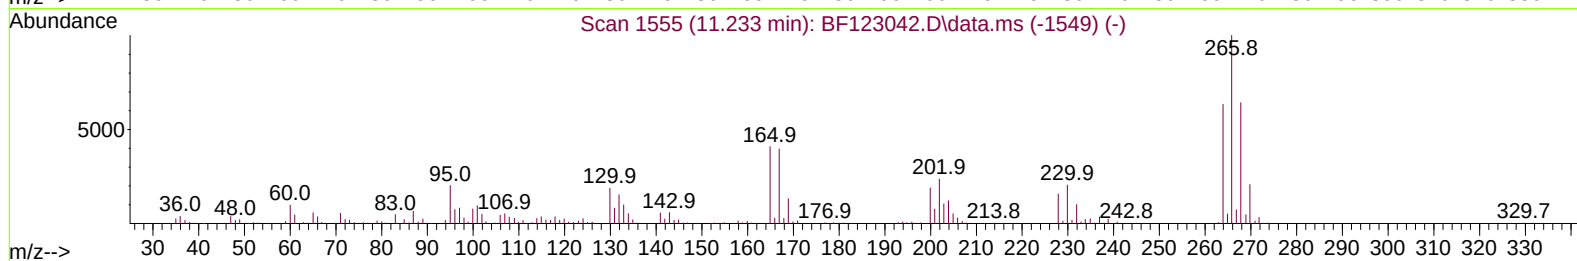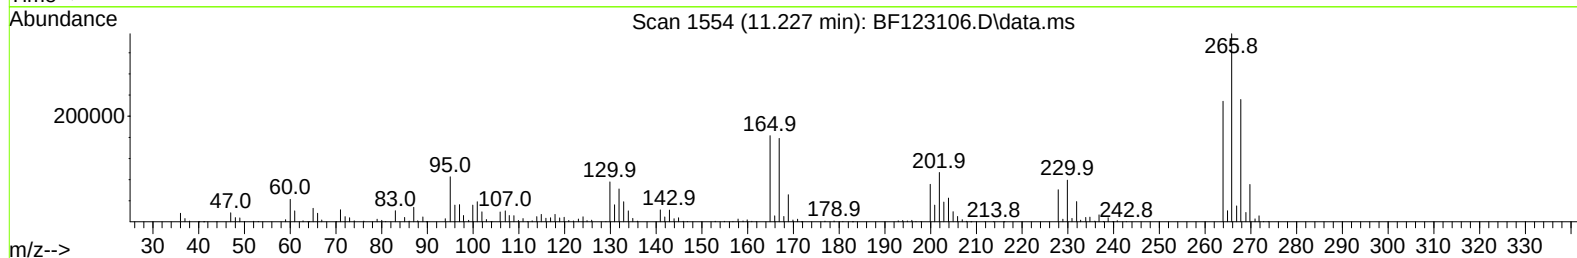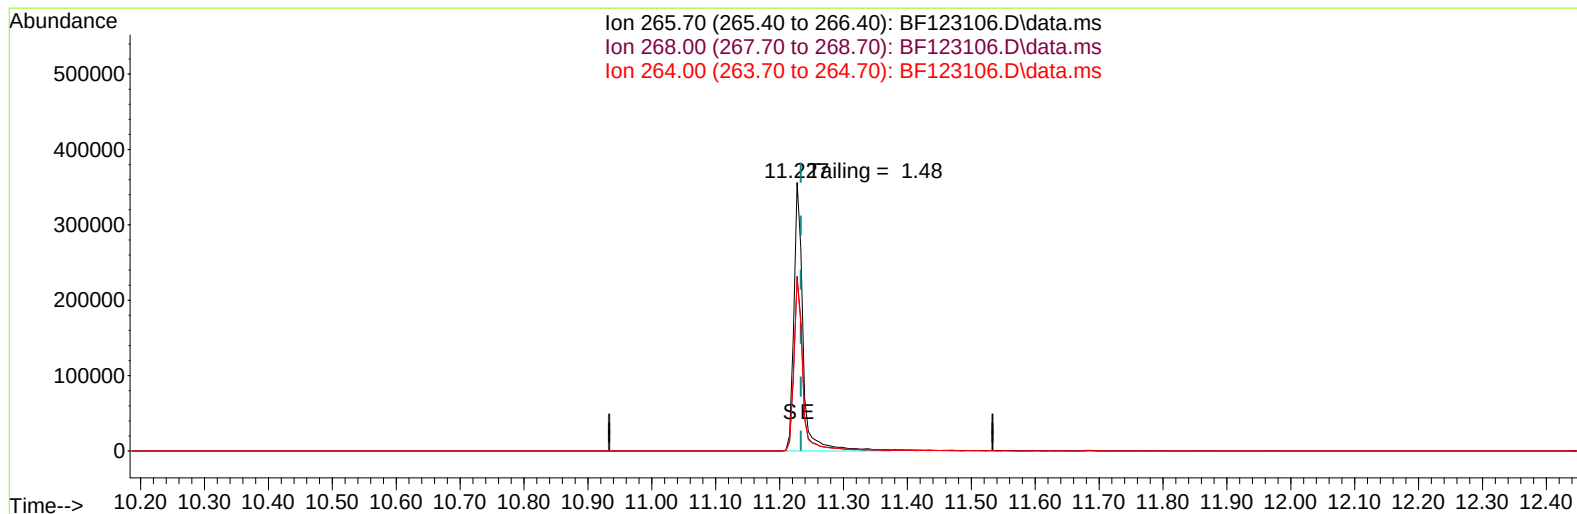

TIC: BF123106.D\data.ms

(70) Pentachlorophenol (C)

11.227min (-0.006) 33650.22 ng

response 361968

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	65.07
264.00	62.30	64.10
0.00	0.00	0.00

