
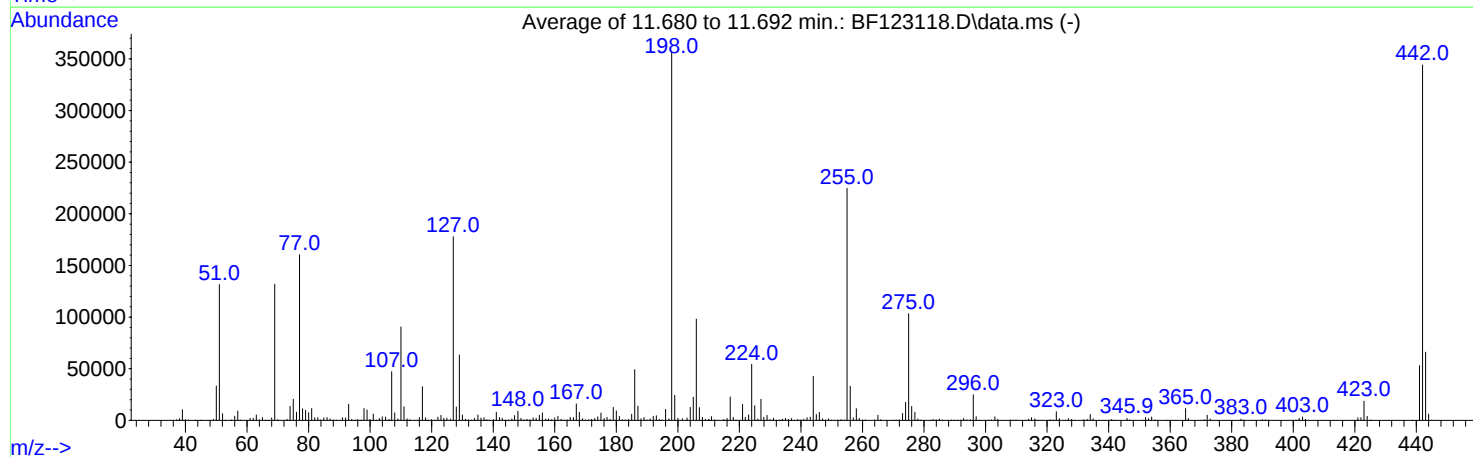


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020421\
 Data File : BF123118.D
 Acq On : 4 Feb 2021 17:37
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 29 12:29:00 2021

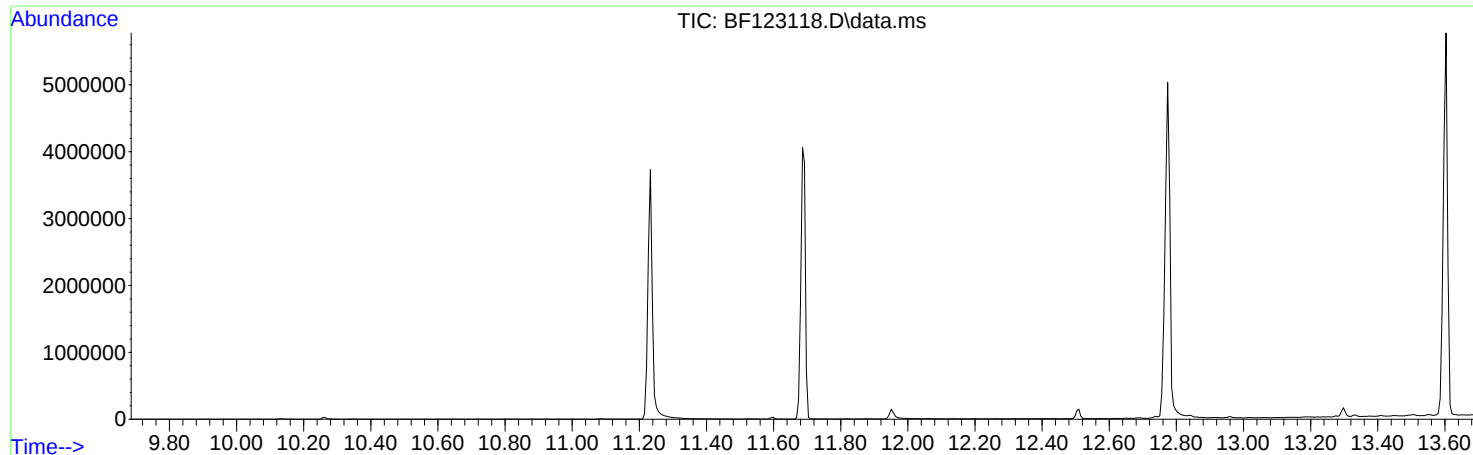

AutoFind: Scans 1631, 1632, 1633; Background Corrected with Scan 1626

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.9	131557	PASS
68	69	0.00	2	1.8	2385	PASS
69	198	0.00	100	37.0	131787	PASS
70	69	0.00	2	0.5	657	PASS
127	198	10	80	49.9	177776	PASS
197	198	0.00	2	0.4	1524	PASS
198	198	100	100	100.0	356160	PASS
199	198	5	9	6.8	24388	PASS
275	198	10	60	29.0	103317	PASS
365	198	1	100	3.2	11415	PASS
441	198	0.01	100	14.9	52962	PASS
442	442	50	100	100.0	344155	PASS
443	442	15	24	19.2	65992	PASS