
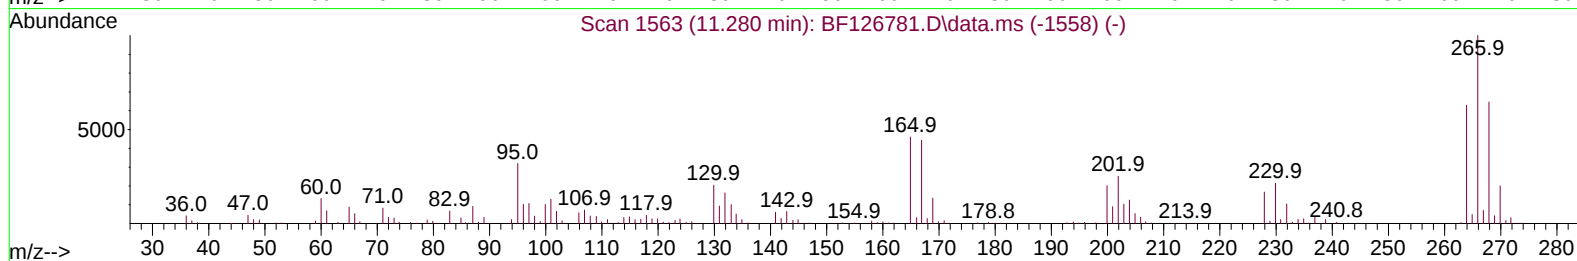
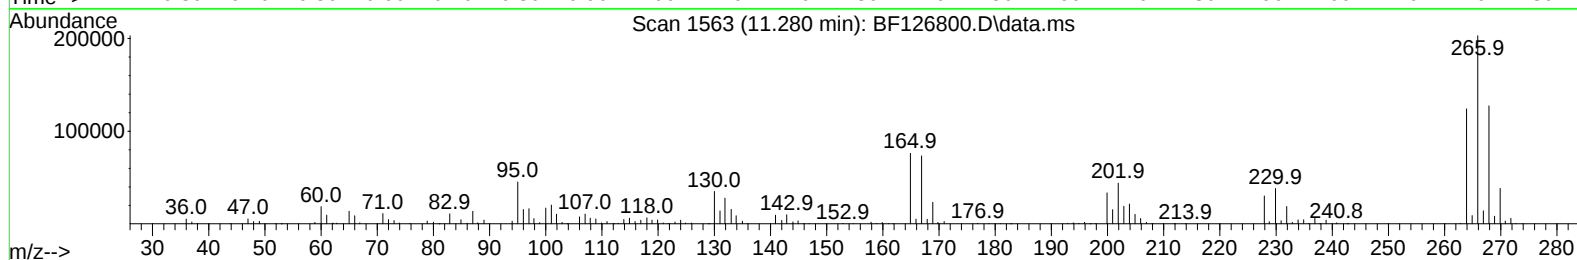


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF020422\  
 Data File : BF126800.D  
 Acq On : 04 Feb 2022 08:21  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 04 10:52:17 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF020222.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Feb 02 15:08:47 2022  
 Response via : Initial Calibration

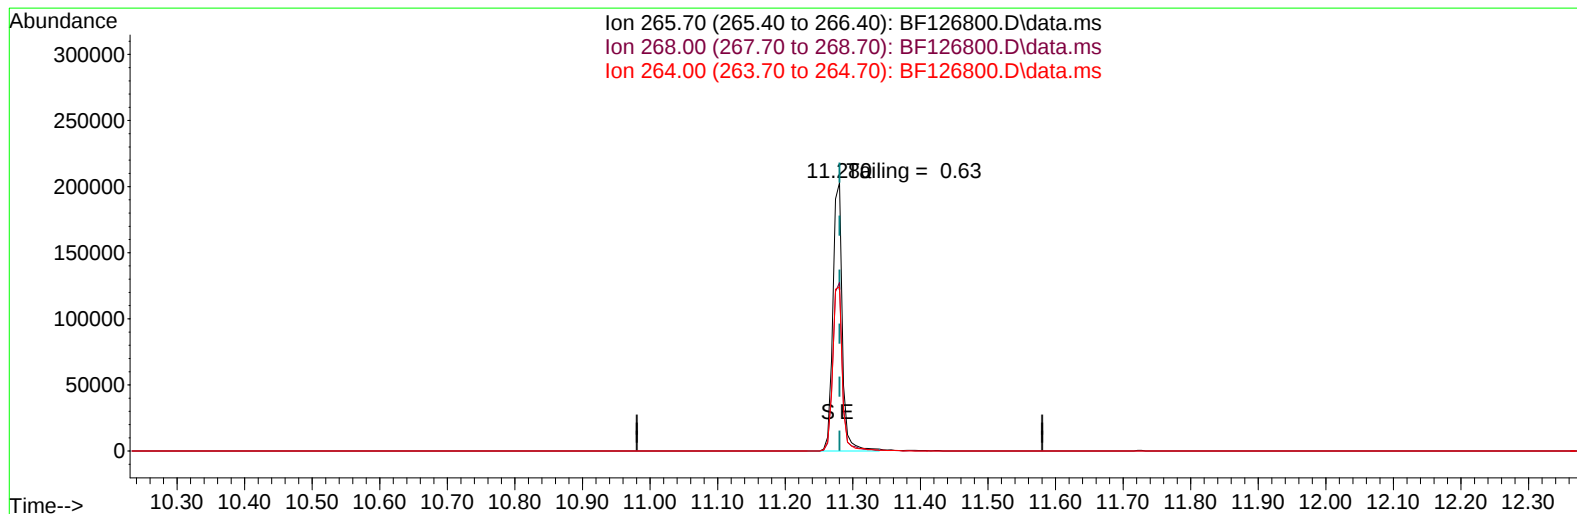

TIC: BF126800.D\data.ms

**(70) Pentachlorophenol (C)**

11.280min (-0.000) 13811.50 ng

response 198213

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 65.40  | 62.78  |
| 264.00 | 63.00  | 61.15  |
| 0.00   | 0.00   | 0.00   |