

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020422\
 Data File : BF126809.D
 Acq On : 04 Feb 2022 14:28
 Operator : CG/JU
 Sample : N1381-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DB-11(32-34)-02-02-22

Quant Time: Feb 04 23:53:45 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 02 15:08:47 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.945	152	145545	20.000	ng	0.00
21) Naphthalene-d8	8.228	136	578810	20.000	ng	0.00
39) Acenaphthene-d10	9.986	164	313661	20.000	ng	0.00
64) Phenanthrene-d10	11.480	188	536902	20.000	ng	0.00
76) Chrysene-d12	14.121	240	275128	20.000	ng	#-0.01
86) Perylene-d12	15.639	264	276662	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.569	112	940445	88.501	ng	0.00
7) Phenol-d6	6.563	99	1276875	86.868	ng	0.00
23) Nitrobenzene-d5	7.510	82	891168	57.622	ng	0.00
42) 2,4,6-Tribromophenol	10.775	330	189175	58.113	ng	-0.01
45) 2-Fluorobiphenyl	9.304	172	1149723	60.694	ng	0.00
79) Terphenyl-d14	13.069	244	1100486	66.912	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020422\
Data File : BF126809.D
Acq On : 04 Feb 2022 14:28
Operator : CG/JU
Sample : N1381-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DB-11(32-34)-02-02-22

Quant Time: Feb 04 23:53:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 02 15:08:47 2022
Response via : Initial Calibration




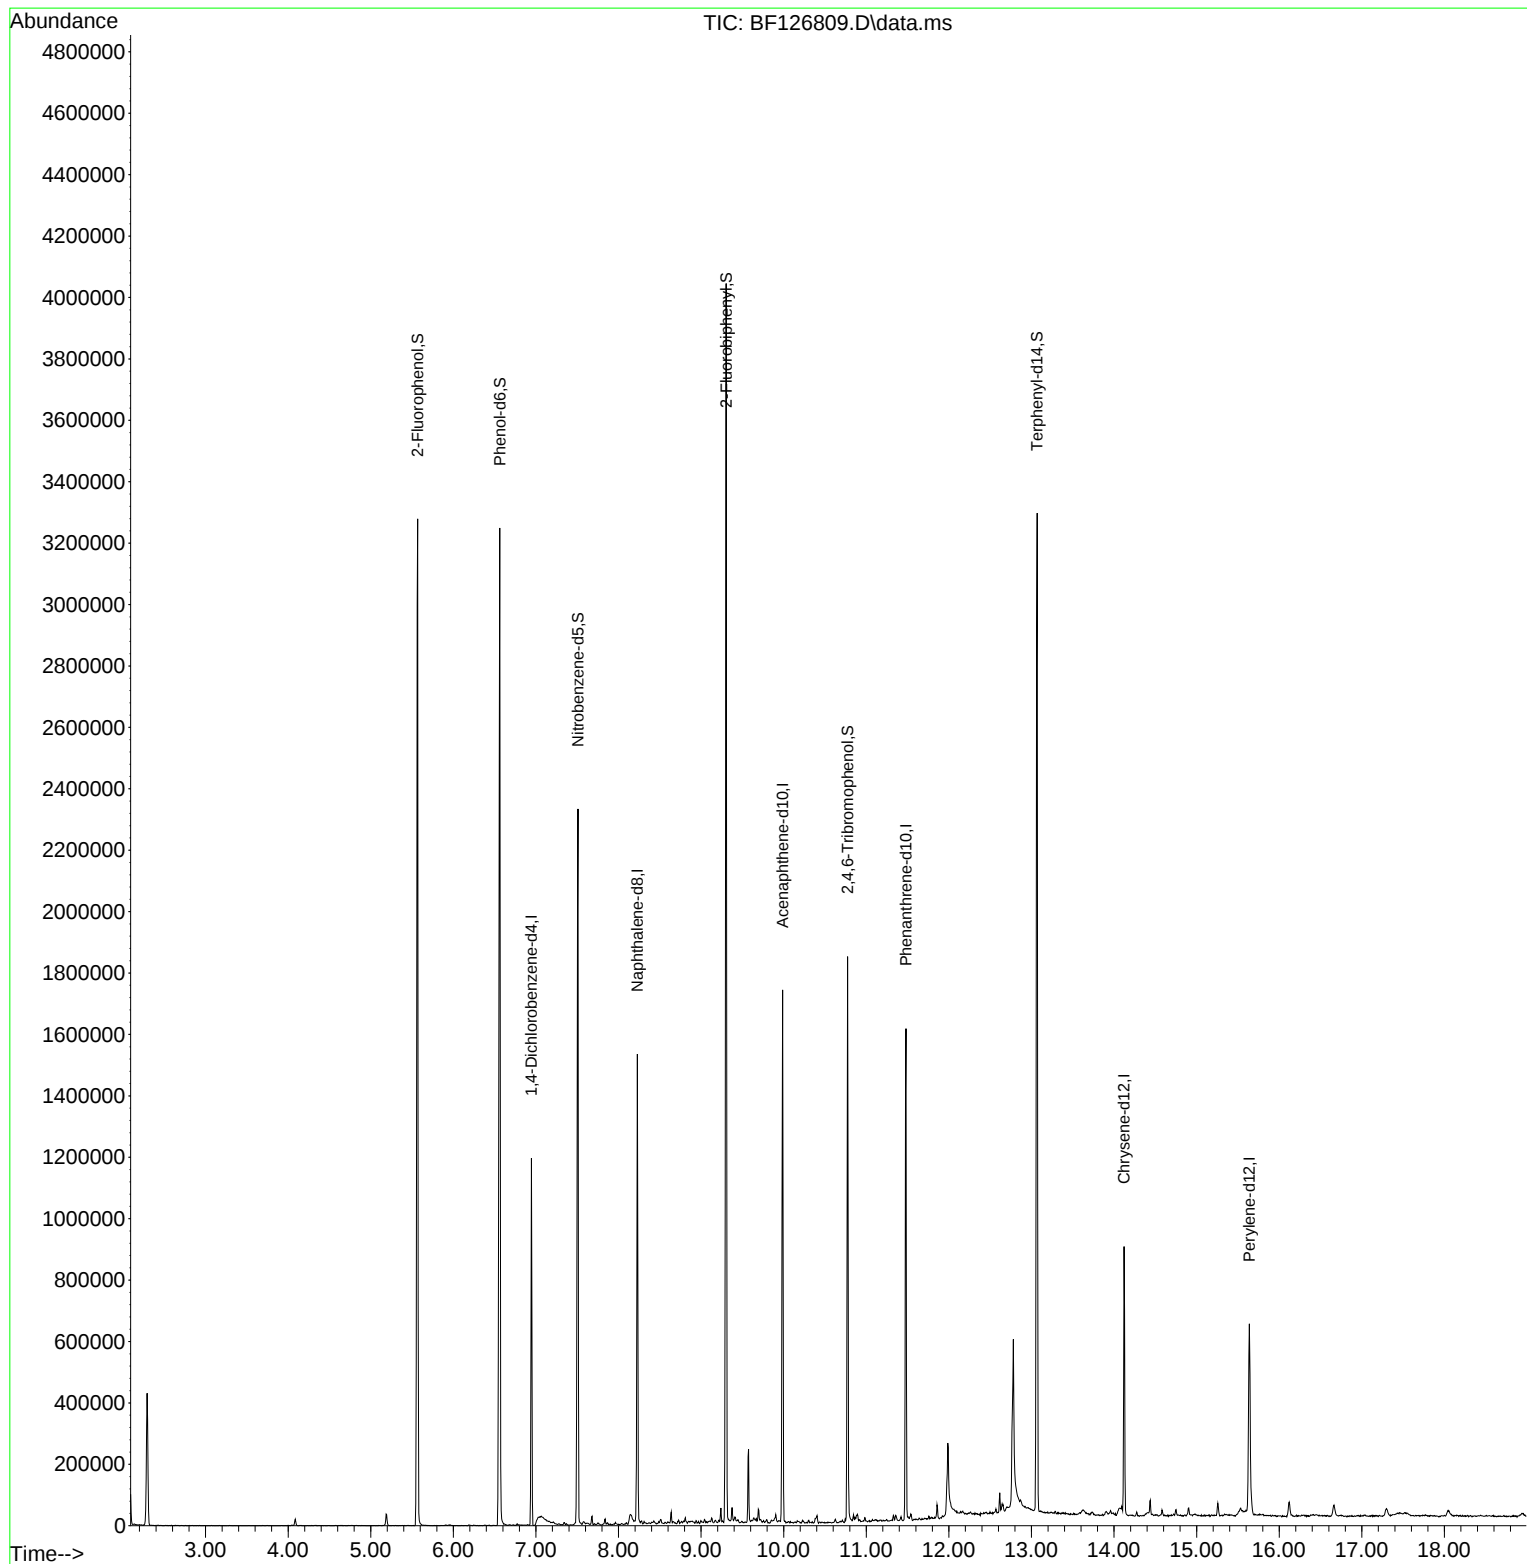


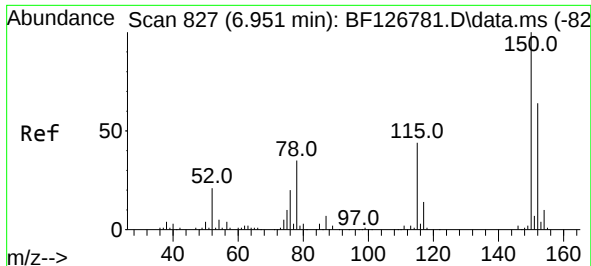

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.945 min Scan# 81
Delta R.T. -0.006 min
Lab File: BF126809.D
Acq: 04 Feb 2022 14:28




Instrument :
BNA_F
ClientSampleId :
DB-11(32-34)-02-02-22


Tgt Ion:152 Resp: 145545
Ion Ratio Lower Upper
152 100
150 158.0 128.1 192.1
115 69.3 56.7 85.1

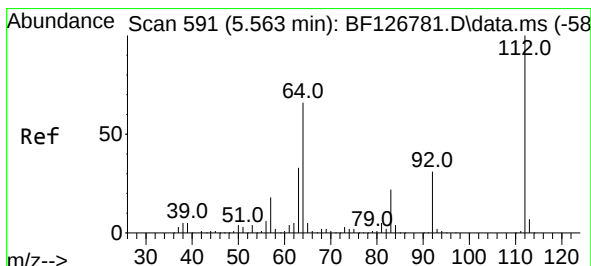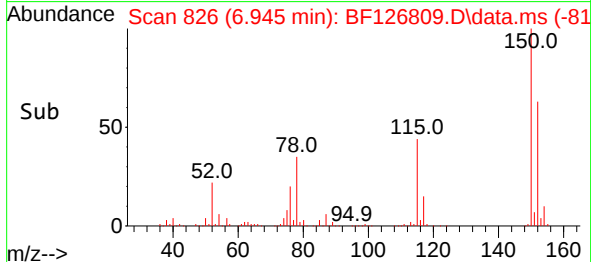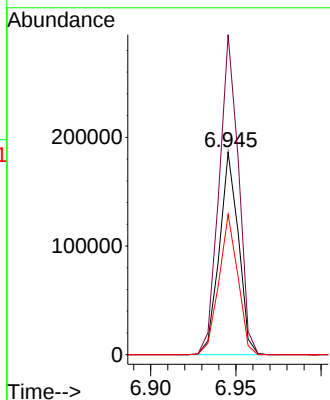

#5
2-Fluorophenol
Concen: 88.501 ng
RT: 5.569 min Scan# 592
Delta R.T. 0.006 min
Lab File: BF126809.D
Acq: 04 Feb 2022 14:28

Tgt Ion:112 Resp: 940445
Ion Ratio Lower Upper
112 100
64 61.3 49.5 74.3
63 30.3 23.9 35.9

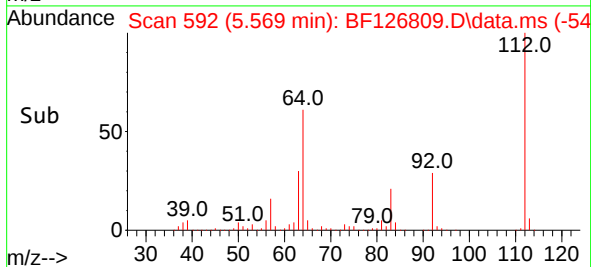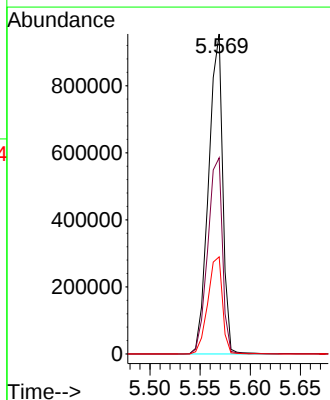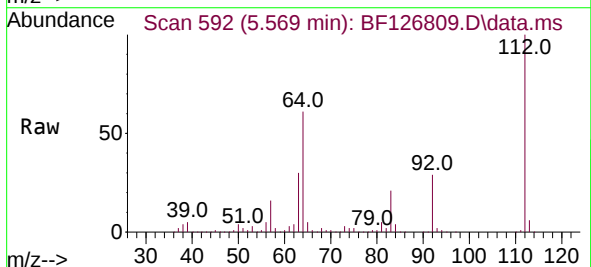



#7

Phenol-d6

Concen: 86.868 ng

RT: 6.563 min Scan# 7

Delta R.T. -0.006 min

Lab File: BF126809.D

Acq: 04 Feb 2022 14:28

Instrument :





BNA_F

ClientSampleId :

DB-11(32-34)-02-02-22

Tgt Ion: 99 Resp: 1276875

Ion	Ratio	Lower	Upper
99	100		
42	14.3	14.2	21.4
71	36.9	24.3	36.5

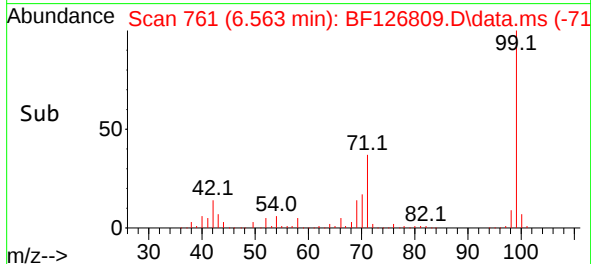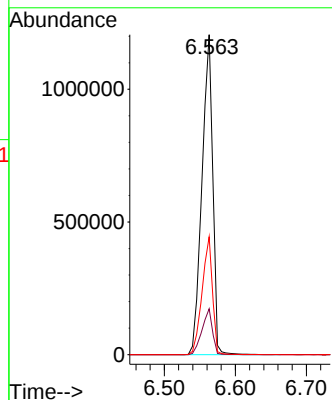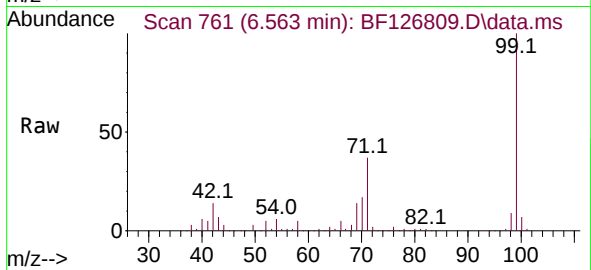

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.228 min Scan# 1044




Delta R.T. -0.006 min


Lab File: BF126809.D

Acq: 04 Feb 2022 14:28

Tgt Ion: 136 Resp: 578810

Ion	Ratio	Lower	Upper
136	100		
137	10.8	8.6	13.0
54	8.8	7.8	11.6
68	8.6	6.3	9.5

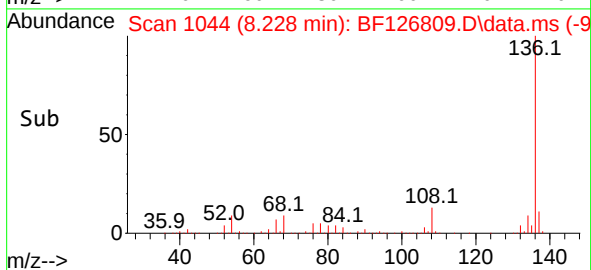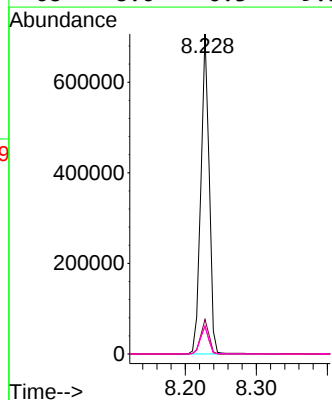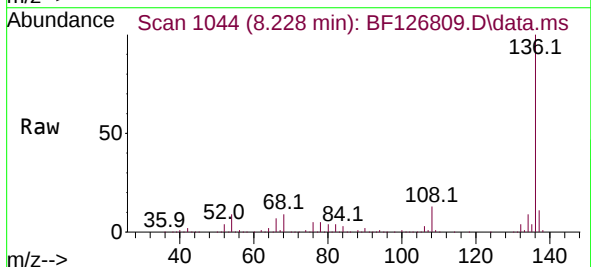

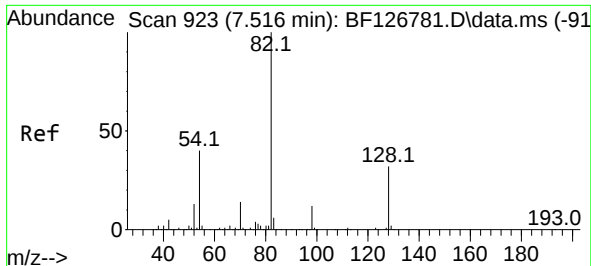

#23

Nitrobenzene-d5

Concen: 57.622 ng

RT: 7.510 min Scan# 91

Delta R.T. -0.006 min

Lab File: BF126809.D

Acq: 04 Feb 2022 14:28

Instrument :

BNA_F

ClientSampleId :

DB-11(32-34)-02-02-22





Tgt Ion: 82 Resp: 891168

Ion Ratio Lower Upper

82 100

128 34.3 32.7 49.1

54 38.4 41.7 62.5#

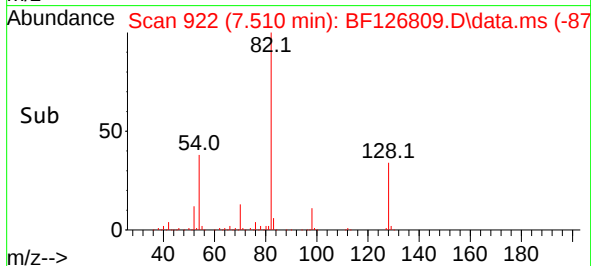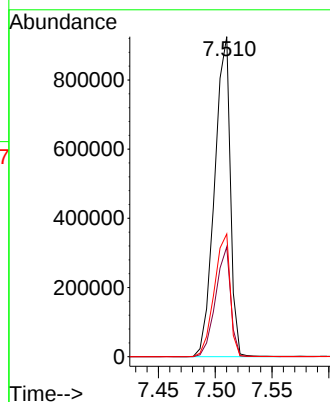

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.986 min Scan# 1343

Delta R.T. -0.006 min

Lab File: BF126809.D

Acq: 04 Feb 2022 14:28




Tgt Ion: 164 Resp: 313661


Ion Ratio Lower Upper

164 100

162 100.1 81.4 122.0

160 42.5 36.6 54.8


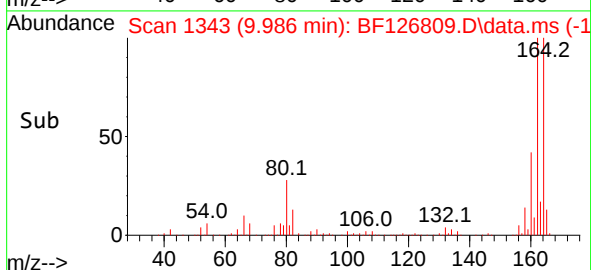
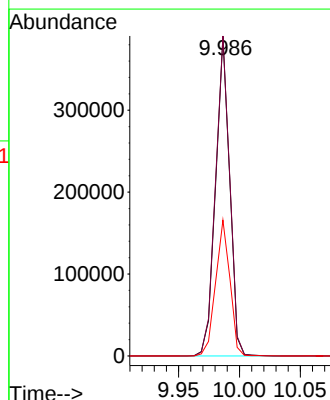
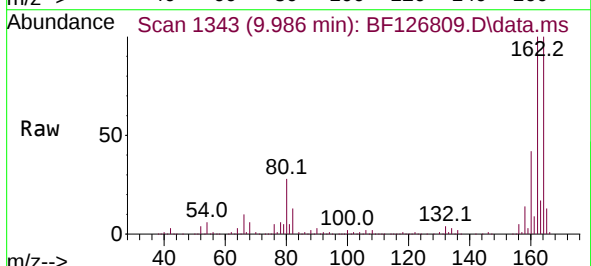




#42
2,4,6-Tribromophenol
Concen: 58.113 ng
RT: 10.775 min Scan# 1479
Delta R.T. -0.012 min
Lab File: BF126809.D
Acq: 04 Feb 2022 14:28




Instrument :
BNA_F
ClientSampleId :
DB-11(32-34)-02-02-22


Tgt Ion: 330 Resp: 189175
Ion Ratio Lower Upper
330 100
332 96.8 76.0 114.0
141 35.3 30.1 45.1

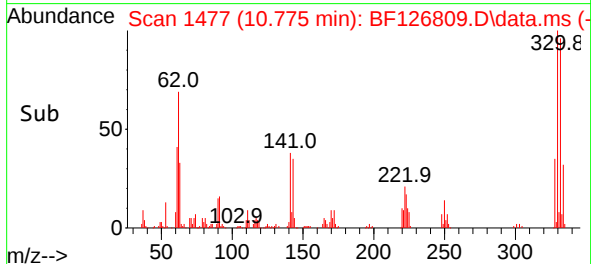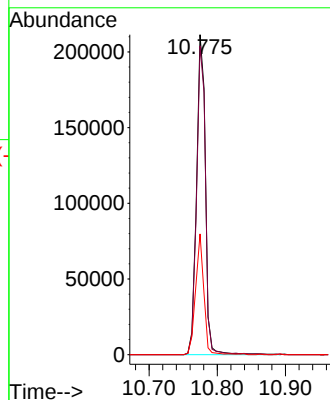

#45
2-Fluorobiphenyl
Concen: 60.694 ng
RT: 9.304 min Scan# 1227
Delta R.T. -0.006 min
Lab File: BF126809.D
Acq: 04 Feb 2022 14:28

Tgt Ion: 172 Resp: 1149723
Ion Ratio Lower Upper
172 100
171 35.0 28.3 42.5
170 23.3 19.0 28.6


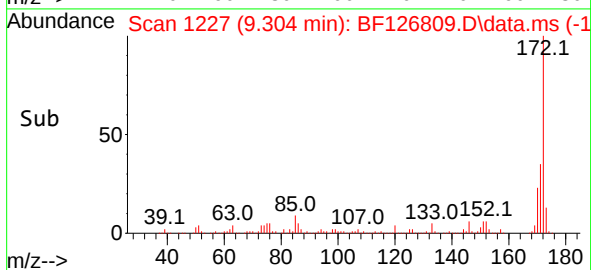
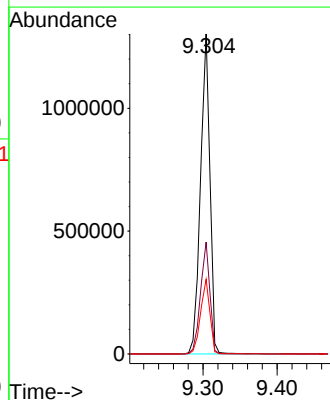
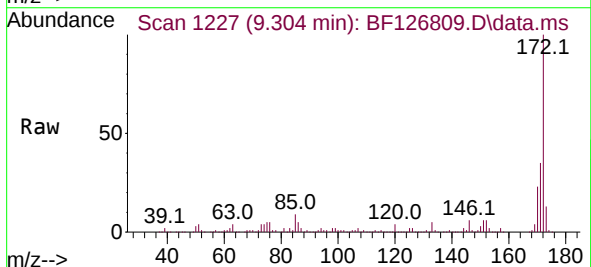




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.480 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF126809.D
Acq: 04 Feb 2022 14:28




Instrument :
BNA_F
ClientSampleId :
DB-11(32-34)-02-02-22


Tgt Ion:188 Resp: 536902
Ion Ratio Lower Upper
188 100
94 12.5 10.1 15.1
80 13.8 11.8 17.6

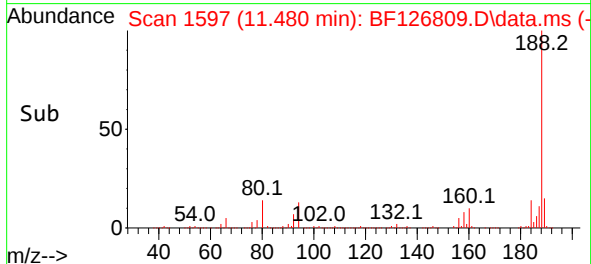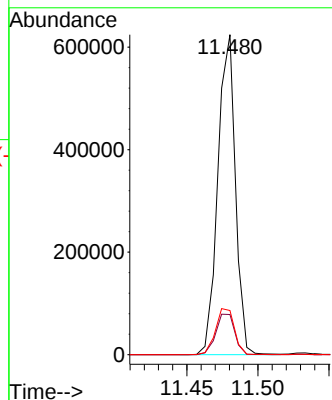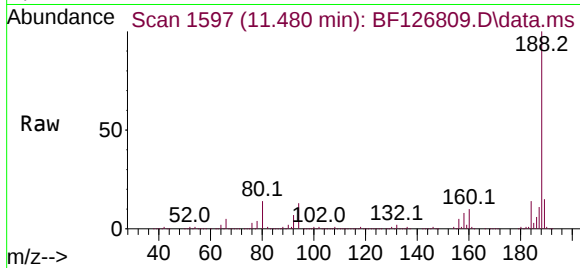

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.121 min Scan# 2046
Delta R.T. -0.012 min
Lab File: BF126809.D
Acq: 04 Feb 2022 14:28

Tgt Ion:240 Resp: 275128
Ion Ratio Lower Upper
240 100
120 13.2 14.4 21.6#
236 25.2 20.5 30.7


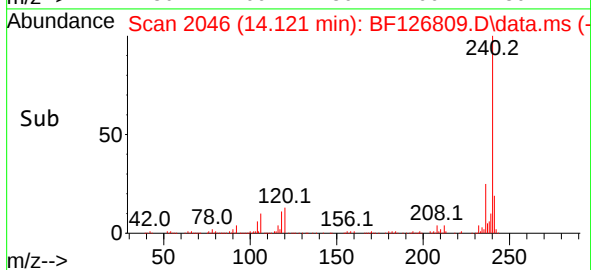
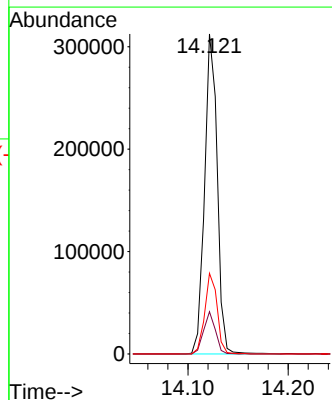
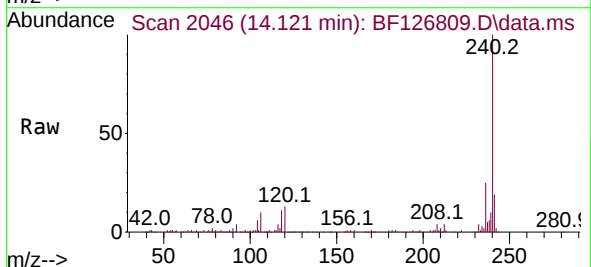


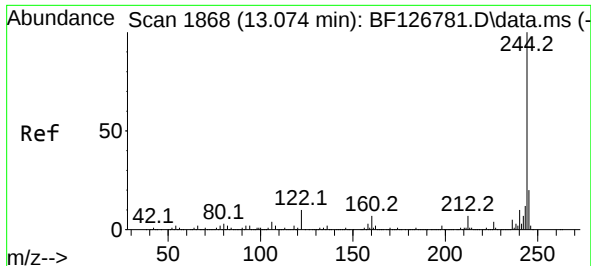

#79
 Terphenyl-d14
 Concen: 66.912 ng
 RT: 13.069 min Scan# 11
 Delta R.T. -0.006 min
 Lab File: BF126809.D
 Acq: 04 Feb 2022 14:28

Instrument :
 BNA_F
 ClientSampleId :
 DB-11(32-34)-02-02-22

Tgt Ion:244 Resp: 1100486
 Ion Ratio Lower Upper
 244 100
 212 6.4 5.0 7.4
 122 10.1 13.3 19.9#

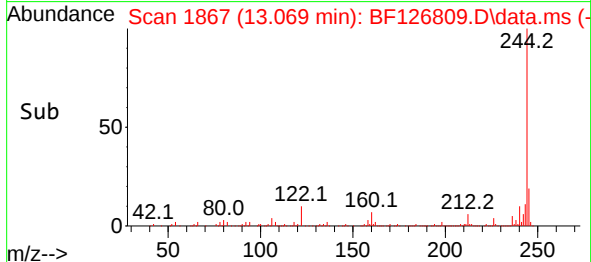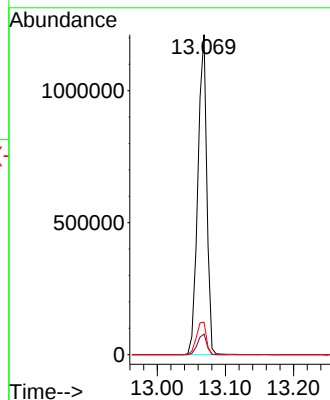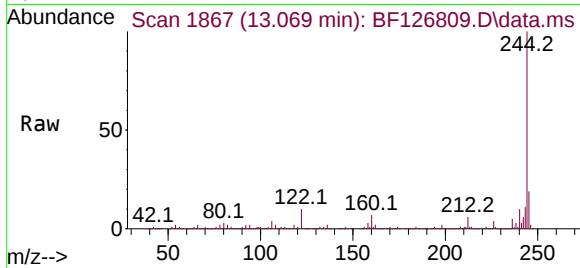

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.639 min Scan# 2304
 Delta R.T. -0.006 min
 Lab File: BF126809.D
 Acq: 04 Feb 2022 14:28

Tgt Ion:264 Resp: 276662
 Ion Ratio Lower Upper
 264 100
 260 23.6 19.2 28.8
 265 20.5 17.4 26.2

