

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020422\
 Data File : BF126803.D
 Acq On : 04 Feb 2022 10:17
 Operator : CG/JU
 Sample : PB142492BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB142492BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF126803.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.575	587	593	596	rBV	4383965	4711895	87.87%	13.931%
2	6.569	755	762	765	rBV	3995707	4854550	90.53%	14.352%
3	6.945	822	826	830	rBV	1214262	959528	17.89%	2.837%
4	7.510	916	922	925	rBV	3017330	3256020	60.72%	9.626%
5	8.228	1039	1044	1048	rBV	1498094	1292233	24.10%	3.820%
6	9.304	1221	1227	1230	rBV	4931710	5049167	94.16%	14.928%
7	9.986	1338	1343	1346	rBV	1850282	1494012	27.86%	4.417%
8	10.781	1473	1478	1481	rBV	3435219	3182455	59.35%	9.409%
9	11.480	1593	1597	1600	rBV	1841001	1528963	28.51%	4.520%
10	13.074	1862	1868	1871	rBV	5369018	5362490	100.00%	15.854%
11	14.127	2043	2047	2050	rBV	1271822	1171605	21.85%	3.464%
12	15.639	2299	2304	2313	rBV	650190	849949	15.85%	2.513%
13	16.127	2381	2387	2392	rBV2	34432	55018	1.03%	0.163%
14	16.662	2471	2478	2485	rBV	29493	56213	1.05%	0.166%




Sum of corrected areas: 33824098

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020422\
Data File : BF126803.D
Acq On : 04 Feb 2022 10:17
Operator : CG/JU
Sample : PB142492BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142492BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

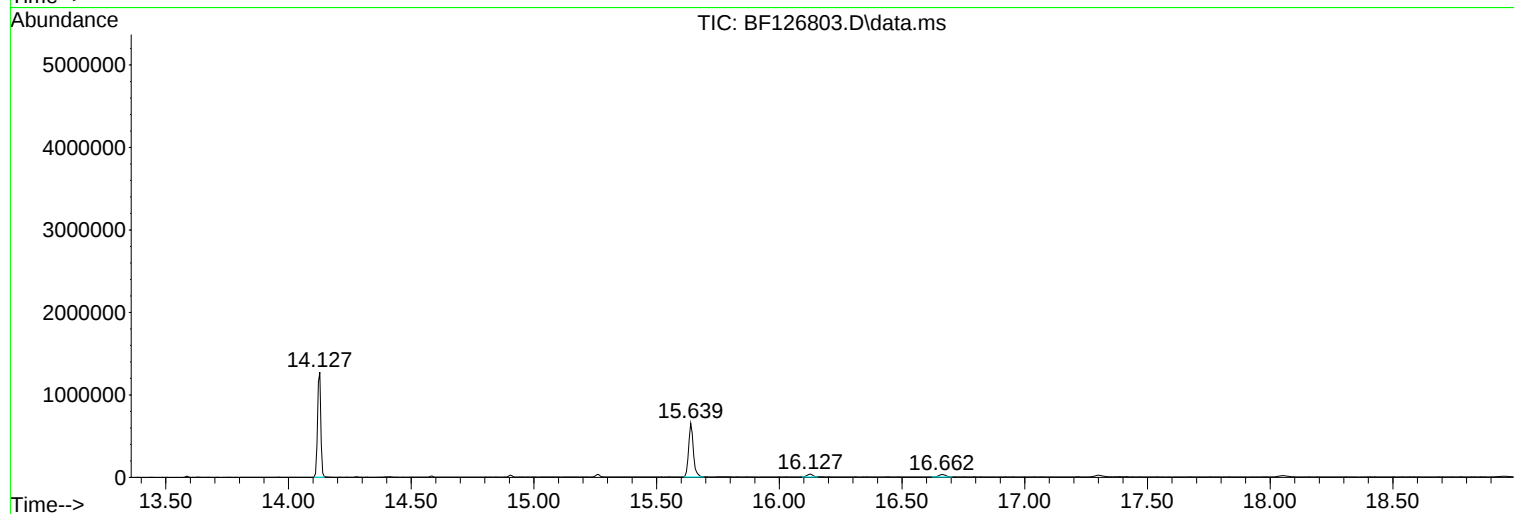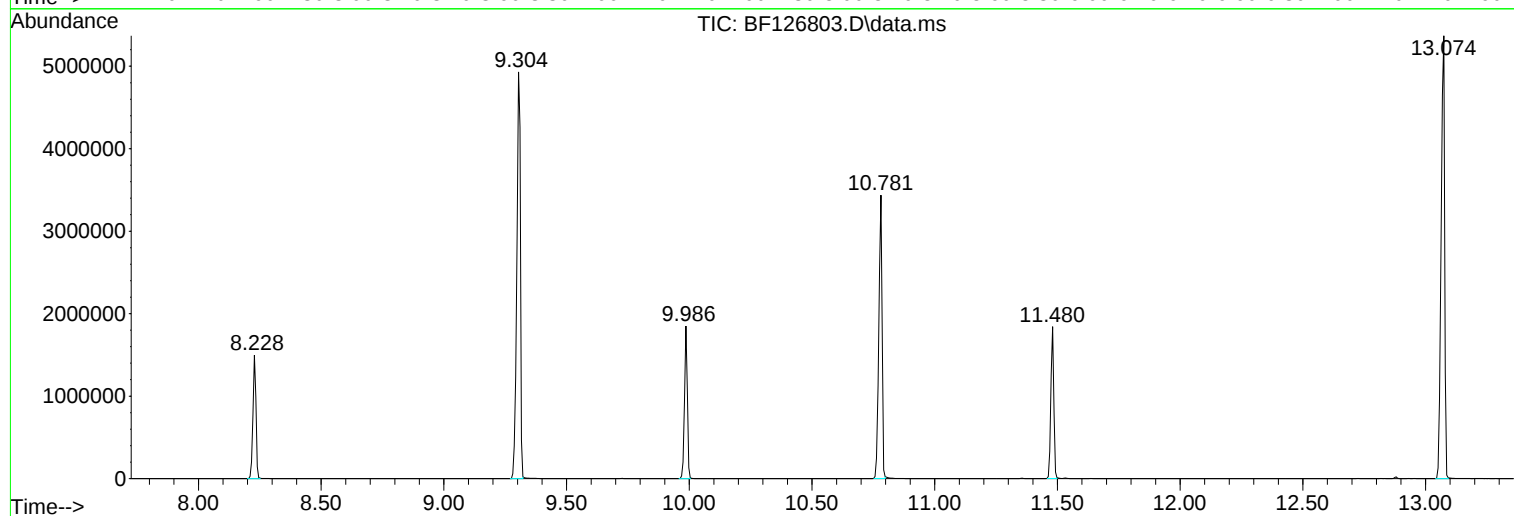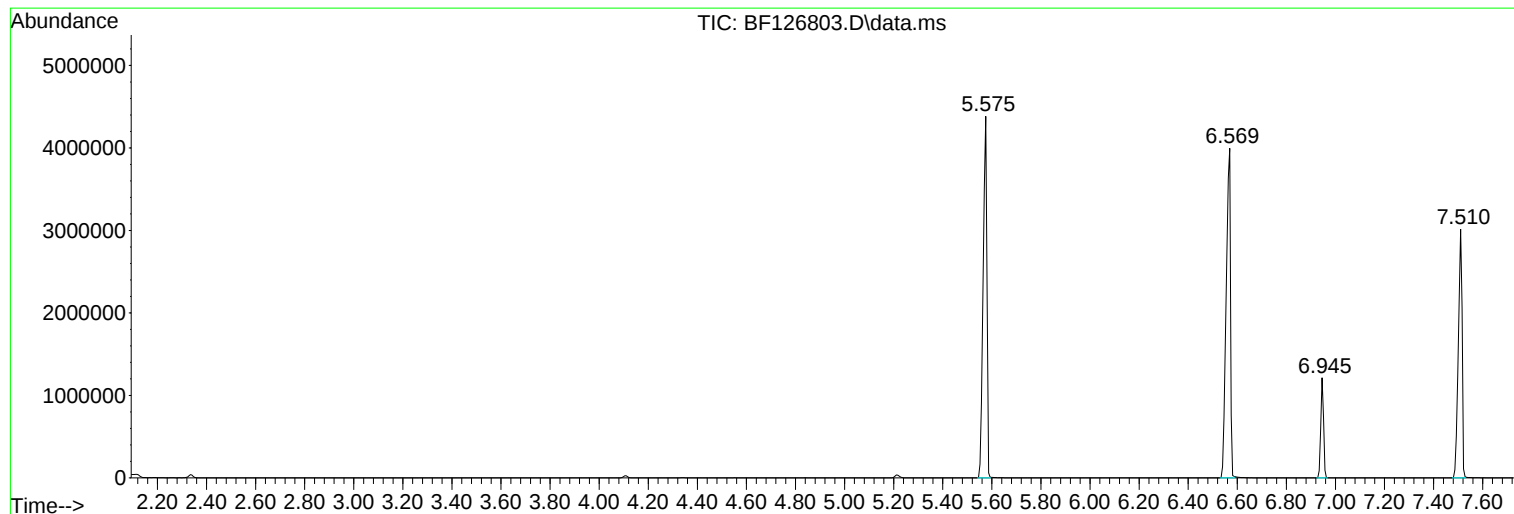

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020422\
Data File : BF126803.D
Acq On : 04 Feb 2022 10:17
Operator : CG/JU
Sample : PB142492BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142492BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020422\
Data File : BF126803.D
Acq On : 04 Feb 2022 10:17
Operator : CG/JU
Sample : PB142492BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142492BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------