

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020422\
 Data File : BF126808.D
 Acq On : 04 Feb 2022 14:00
 Operator : CG/JU
 Sample : N1381-08
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DB-07(20-22)-02-02-22

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF126808.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.287	29	34	43	rVB	368578	499421	10.93%	1.336%
2	5.569	587	592	595	rBV	3669917	3640748	79.69%	9.737%
3	6.563	756	761	773	rBV	3212244	3837742	84.00%	10.264%
4	6.945	822	826	829	rBV	1217993	924522	20.24%	2.473%
5	7.510	916	922	925	rBV	2577708	2475522	54.19%	6.621%
6	8.157	1024	1032	1040	rBV	44152	88012	1.93%	0.235%
7	8.228	1040	1044	1047	rBV	1485611	1226542	26.85%	3.280%
8	9.304	1222	1227	1230	rBV	4301577	3836586	83.98%	10.261%
9	9.986	1339	1343	1346	rBV	1729997	1409540	30.85%	3.770%
10	10.292	1391	1395	1406	rBV	85746	154769	3.39%	0.414%
11	10.775	1473	1477	1486	rBV	1925250	1710664	37.44%	4.575%
12	11.480	1593	1597	1600	rBV	1649686	1417255	31.02%	3.790%
13	11.857	1657	1661	1665	rBV2	52381	83880	1.84%	0.224%
14	11.986	1675	1683	1700	rVB	1710435	2989997	65.45%	7.997%
15	12.257	1727	1729	1737	rVB4	39434	53807	1.18%	0.144%
16	12.645	1792	1795	1799	rBV	126619	166769	3.65%	0.446%
17	12.704	1800	1805	1809	rVV6	151015	386705	8.46%	1.034%
18	12.780	1811	1818	1833	rVB	2825123	4568519	100.00%	12.218%
19	13.069	1862	1867	1870	rBV	3990671	3553345	77.78%	9.503%
20	13.221	1886	1893	1902	rVB2	136976	340825	7.46%	0.912%
21	14.074	2030	2038	2043	rBV	225762	476944	10.44%	1.276%
22	14.121	2043	2046	2050	rVV	989389	914581	20.02%	2.446%
23	14.186	2054	2057	2069	rVB	36144	79271	1.74%	0.212%
24	14.721	2142	2148	2156	rBV2	166385	334331	7.32%	0.894%
25	14.904	2175	2179	2182	rVB	63136	65030	1.42%	0.174%
26	15.257	2235	2239	2244	rVB	81007	99343	2.17%	0.266%
27	15.404	2258	2264	2273	rVB2	96513	209433	4.58%	0.560%
28	15.639	2299	2304	2315	rVB	593283	874016	19.13%	2.338%
29	16.057	2364	2375	2377	rBV10	43861	127783	2.80%	0.342%
30	16.121	2382	2386	2391	rVV	107764	200171	4.38%	0.535%
31	16.186	2392	2397	2406	rVB4	77970	193697	4.24%	0.518%
32	16.627	2464	2472	2473	rBV3	46317	88096	1.93%	0.236%
33	16.657	2474	2477	2485	rVB	74246	146567	3.21%	0.392%
34	17.109	2549	2554	2563	rVB3	49860	131149	2.87%	0.351%
35	17.292	2581	2585	2593	rVB2	41809	84900	1.86%	0.227%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020422\
Data File : BF126808.D
Acq On : 04 Feb 2022 14:00
Operator : CG/JU
Sample : N1381-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DB-07(20-22)-02-02-22

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020222.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION




Sum of corrected areas: 37390482

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020422\
Data File : BF126808.D
Acq On : 04 Feb 2022 14:00
Operator : CG/JU
Sample : N1381-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DB-07(20-22)-02-02-22

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

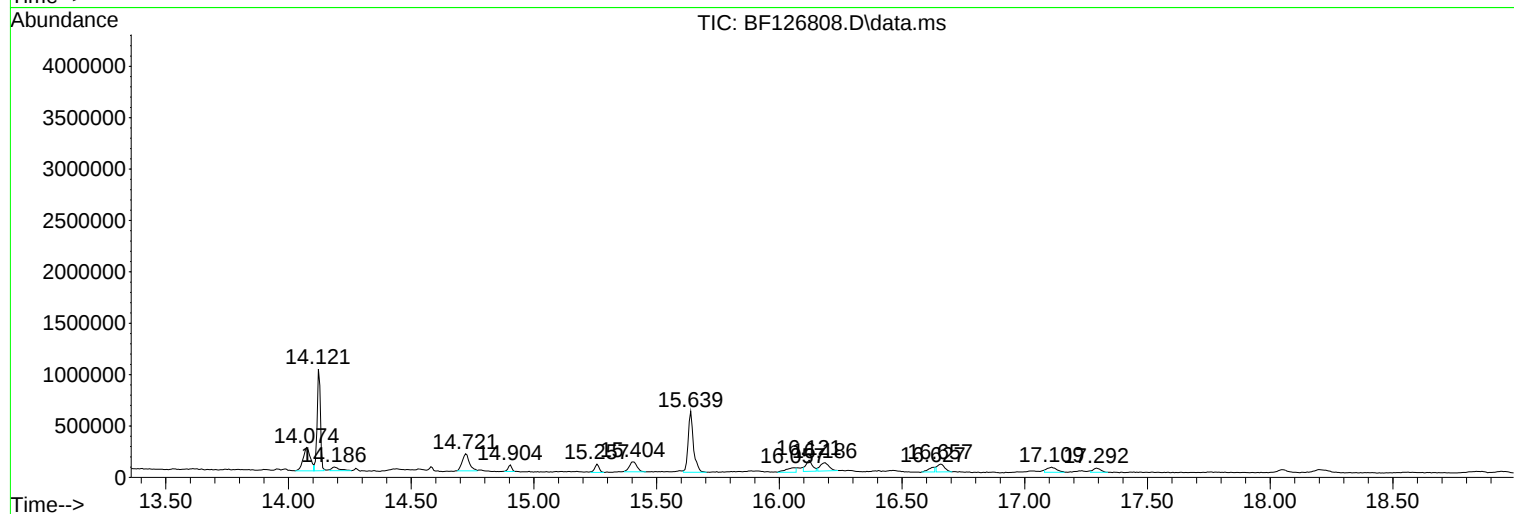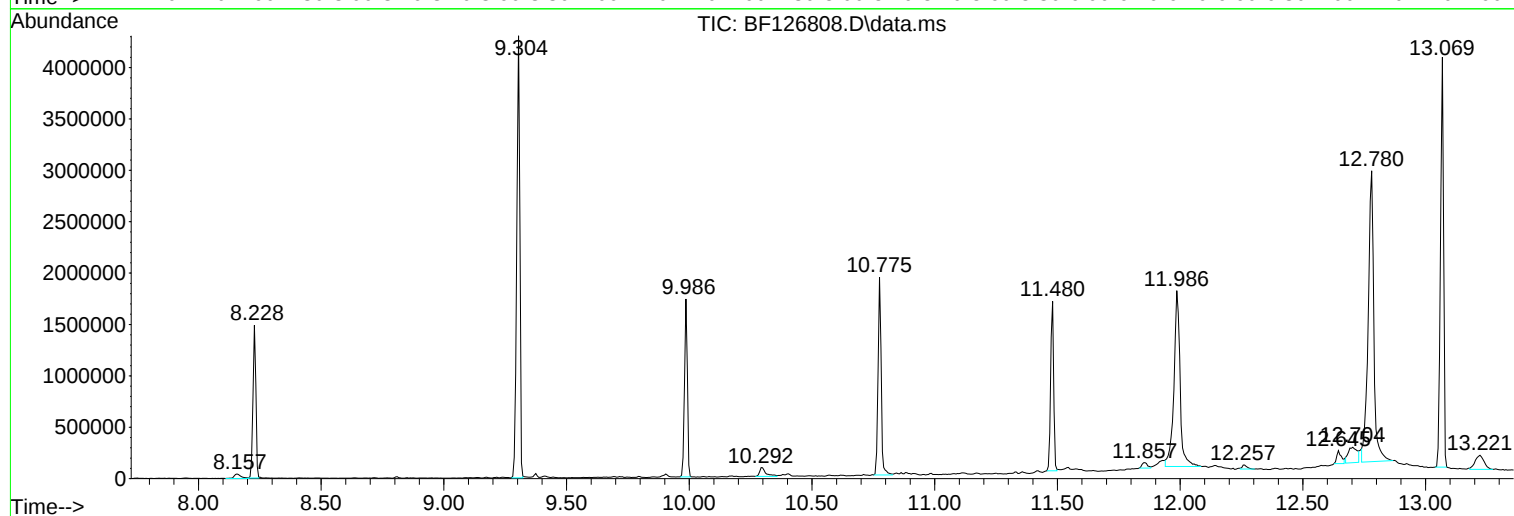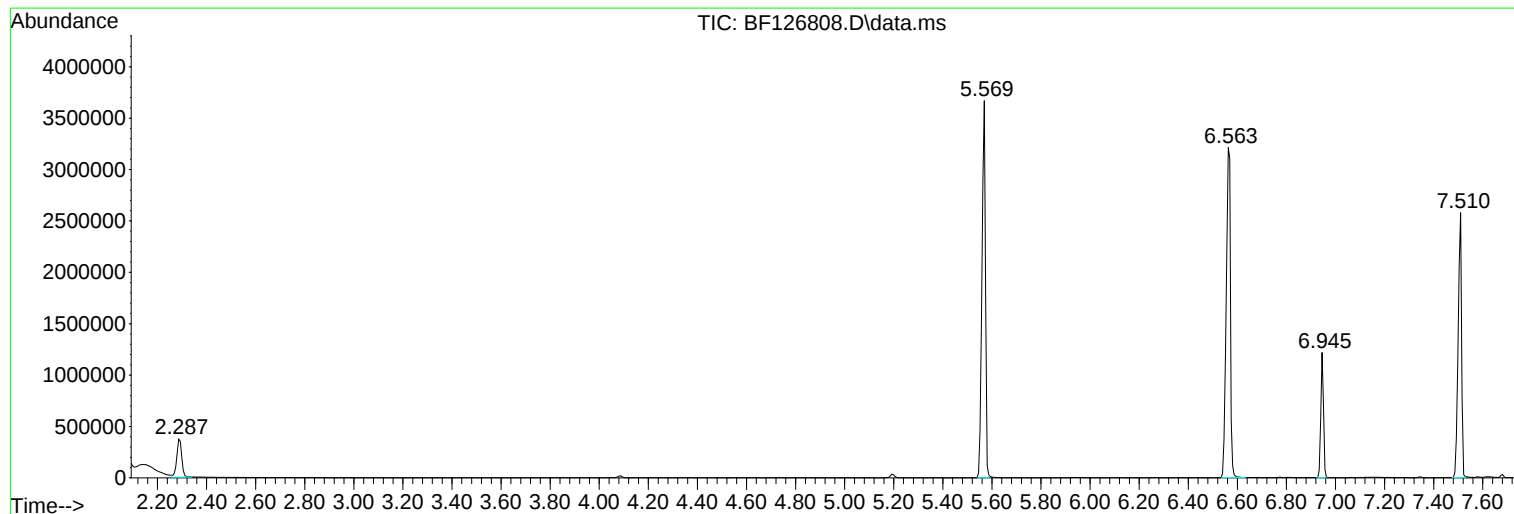

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020422\
Data File : BF126808.D
Acq On : 04 Feb 2022 14:00
Operator : CG/JU
Sample : N1381-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DB-07(20-22)-02-02-22

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020422\
Data File : BF126808.D
Acq On : 04 Feb 2022 14:00
Operator : CG/JU
Sample : N1381-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DB-07(20-22)-02-02-22

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc