


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020422\
 Data File : BF126800.D
 Acq On : 04 Feb 2022 08:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 02 15:08:47 2022

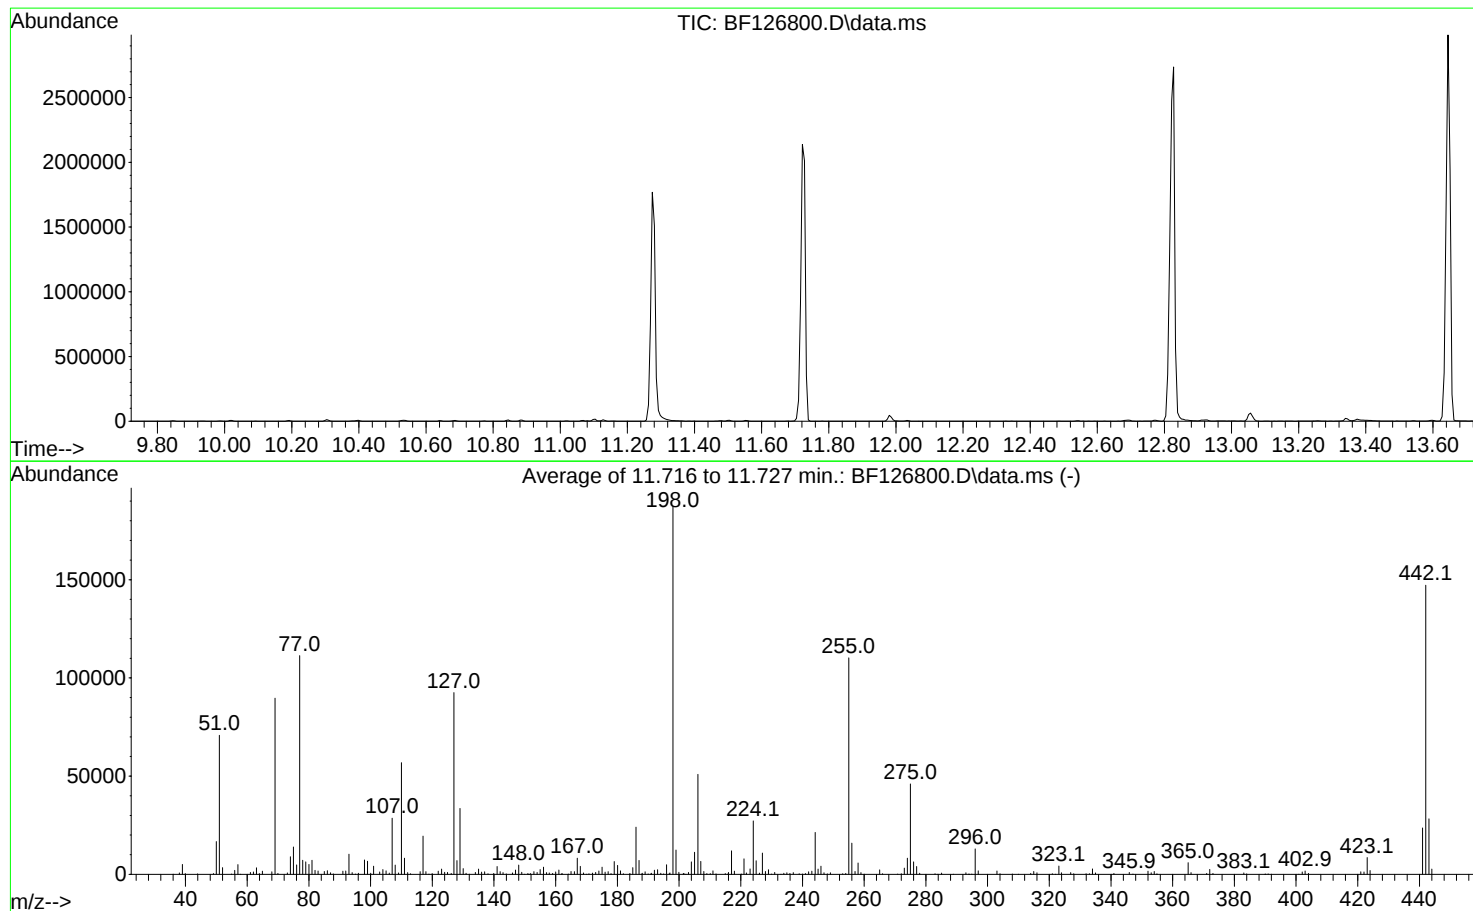

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.8	70808	PASS
68	69	0.00	2	1.5	1329	PASS
69	198	0.00	100	47.9	89701	PASS
70	69	0.00	2	0.5	464	PASS
127	198	10	80	49.4	92552	PASS
197	198	0.00	2	0.4	740	PASS
198	198	100	100	100.0	187272	PASS
199	198	5	9	6.6	12391	PASS
275	198	10	60	24.6	45997	PASS
365	198	1	100	3.2	5975	PASS
441	198	0.01	100	12.6	23643	PASS
442	442	50	100	100.0	147187	PASS
443	442	15	24	19.2	28284	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/4/2022	BNA_F	<u>BF126800.D</u>
Compound Name	Response	Retention Time
DDT	499403	13.64
DDD	4121	13.34
DDE	118	13
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4239	503642	0.84

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020422\
 Data File : BF126800.D
 Acq On : 04 Feb 2022 08:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Feb 04 10:52:17 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 02 15:08:47 2022
 Response via : Initial Calibration

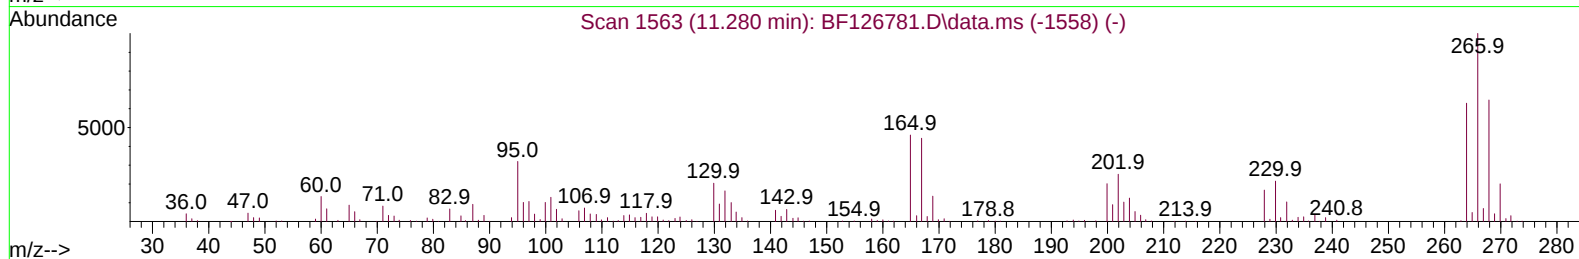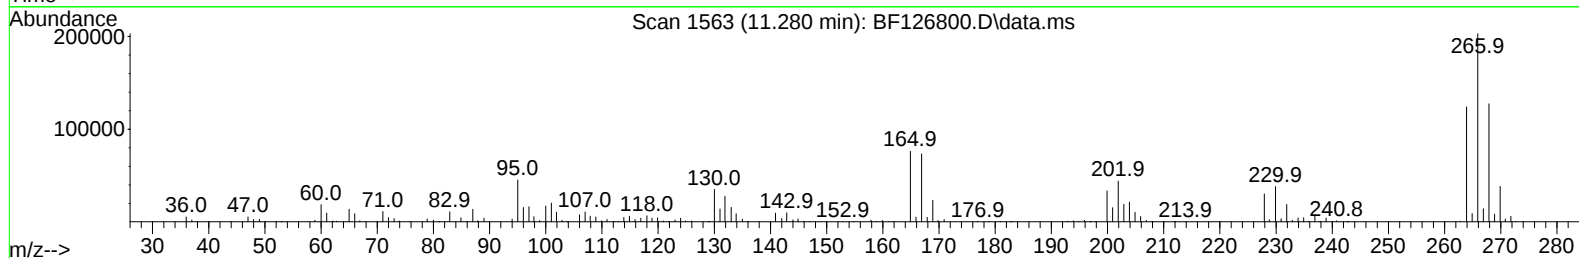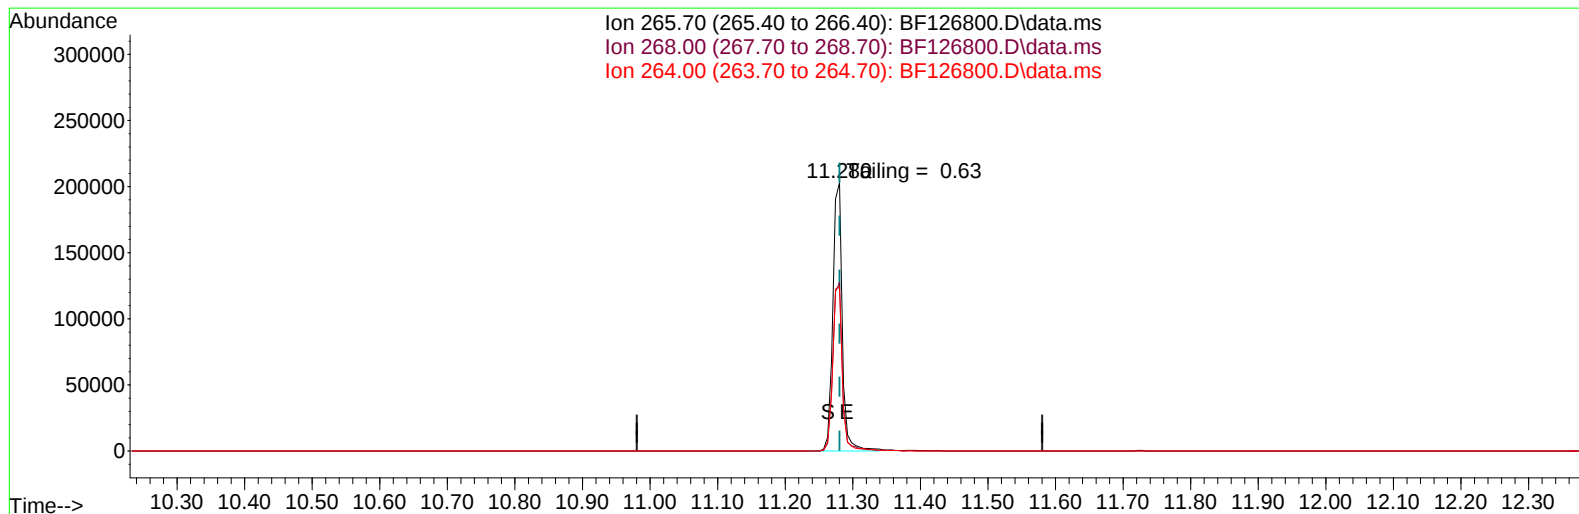

TIC: BF126800.D\data.ms

(70) Pentachlorophenol (C)

11.280min (-0.000) 13811.50 ng




response 198213

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	62.78
264.00	63.00	61.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020422\
 Data File : BF126800.D
 Acq On : 04 Feb 2022 08:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Feb 04 10:52:17 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 02 15:08:47 2022
 Response via : Initial Calibration

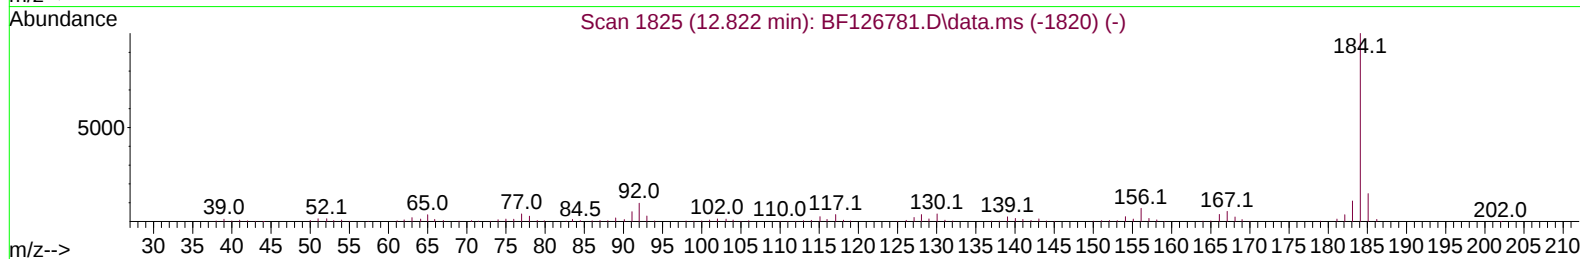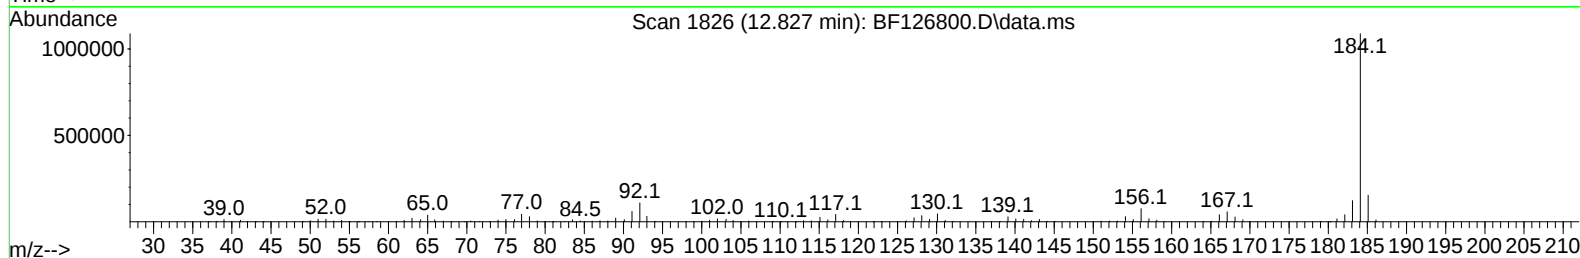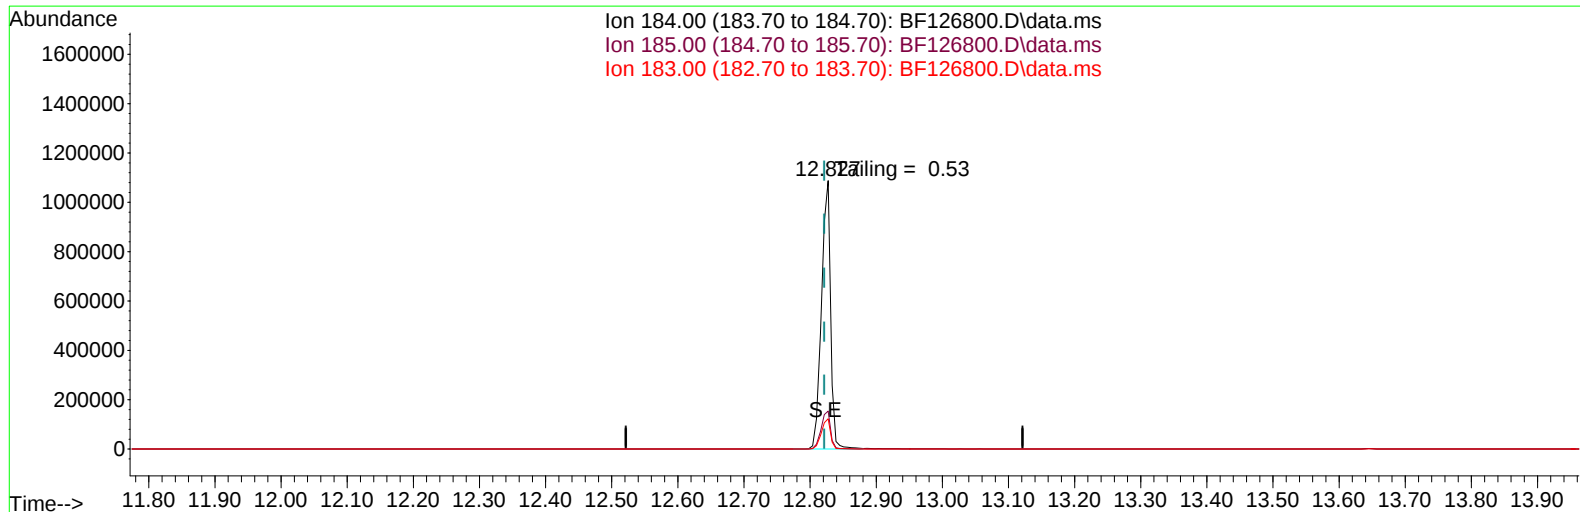

TIC: BF126800.D\data.ms

(77) Benzidine

12.827min (+ 0.006) 21251.59 ng

response 1049157

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.14
183.00	10.20	11.26
0.00	0.00	0.00