

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020425\
 Data File : BF141417.D
 Acq On : 04 Feb 2025 19:07
 Operator : RC/JU
 Sample : Q1241-16
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 JPP-5.4-013025

Quant Time: Feb 05 00:33:15 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 29 17:41:25 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.787	152	87662	20.000	ng	-0.02
21) Naphthalene-d8	8.069	136	356625	20.000	ng	#-0.02
39) Acenaphthene-d10	9.822	164	198235	20.000	ng	-0.02
64) Phenanthrene-d10	11.310	188	358571	20.000	ng	-0.02
76) Chrysene-d12	13.957	240	323769	20.000	ng	#-0.02
86) Perylene-d12	15.421	264	258055	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.422	112	723850	126.766	ng	0.01
7) Phenol-d6	6.428	99	838413	115.420	ng	-0.01
23) Nitrobenzene-d5	7.351	82	651522	96.308	ng	-0.02
42) 2,4,6-Tribromophenol	10.616	330	298675	164.346	ng	-0.02
45) 2-Fluorobiphenyl	9.145	172	1217841	94.559	ng	-0.02
79) Terphenyl-d14	12.904	244	1584137	75.456	ng	-0.01
Target Compounds						
						Qvalue
19) n-Nitroso-di-n-propyla...	7.351	70	90432	20.951	ng	# 76
25) Isophorone	7.351	82	646732	55.305	ng	# 64
50) Dimethylphthalate	9.822	163	27302	2.039	ng	# 1
51) 2,6-Dinitrotoluene	9.822	165	25568	8.225	ng	# 24
57) 2,4-Dinitrotoluene	9.822	165	25568	6.352	ng	# 23
67) 4-Bromophenyl-phenylether	10.616	248	20413	5.085	ng	# 1
77) Benzidine	12.904	184	21618	2.083	ng	# 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020425\
Data File : BF141417.D
Acq On : 04 Feb 2025 19:07
Operator : RC/JU
Sample : Q1241-16
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
JPP-5.4-013025

Quant Time: Feb 05 00:33:15 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 29 17:41:25 2025
Response via : Initial Calibration




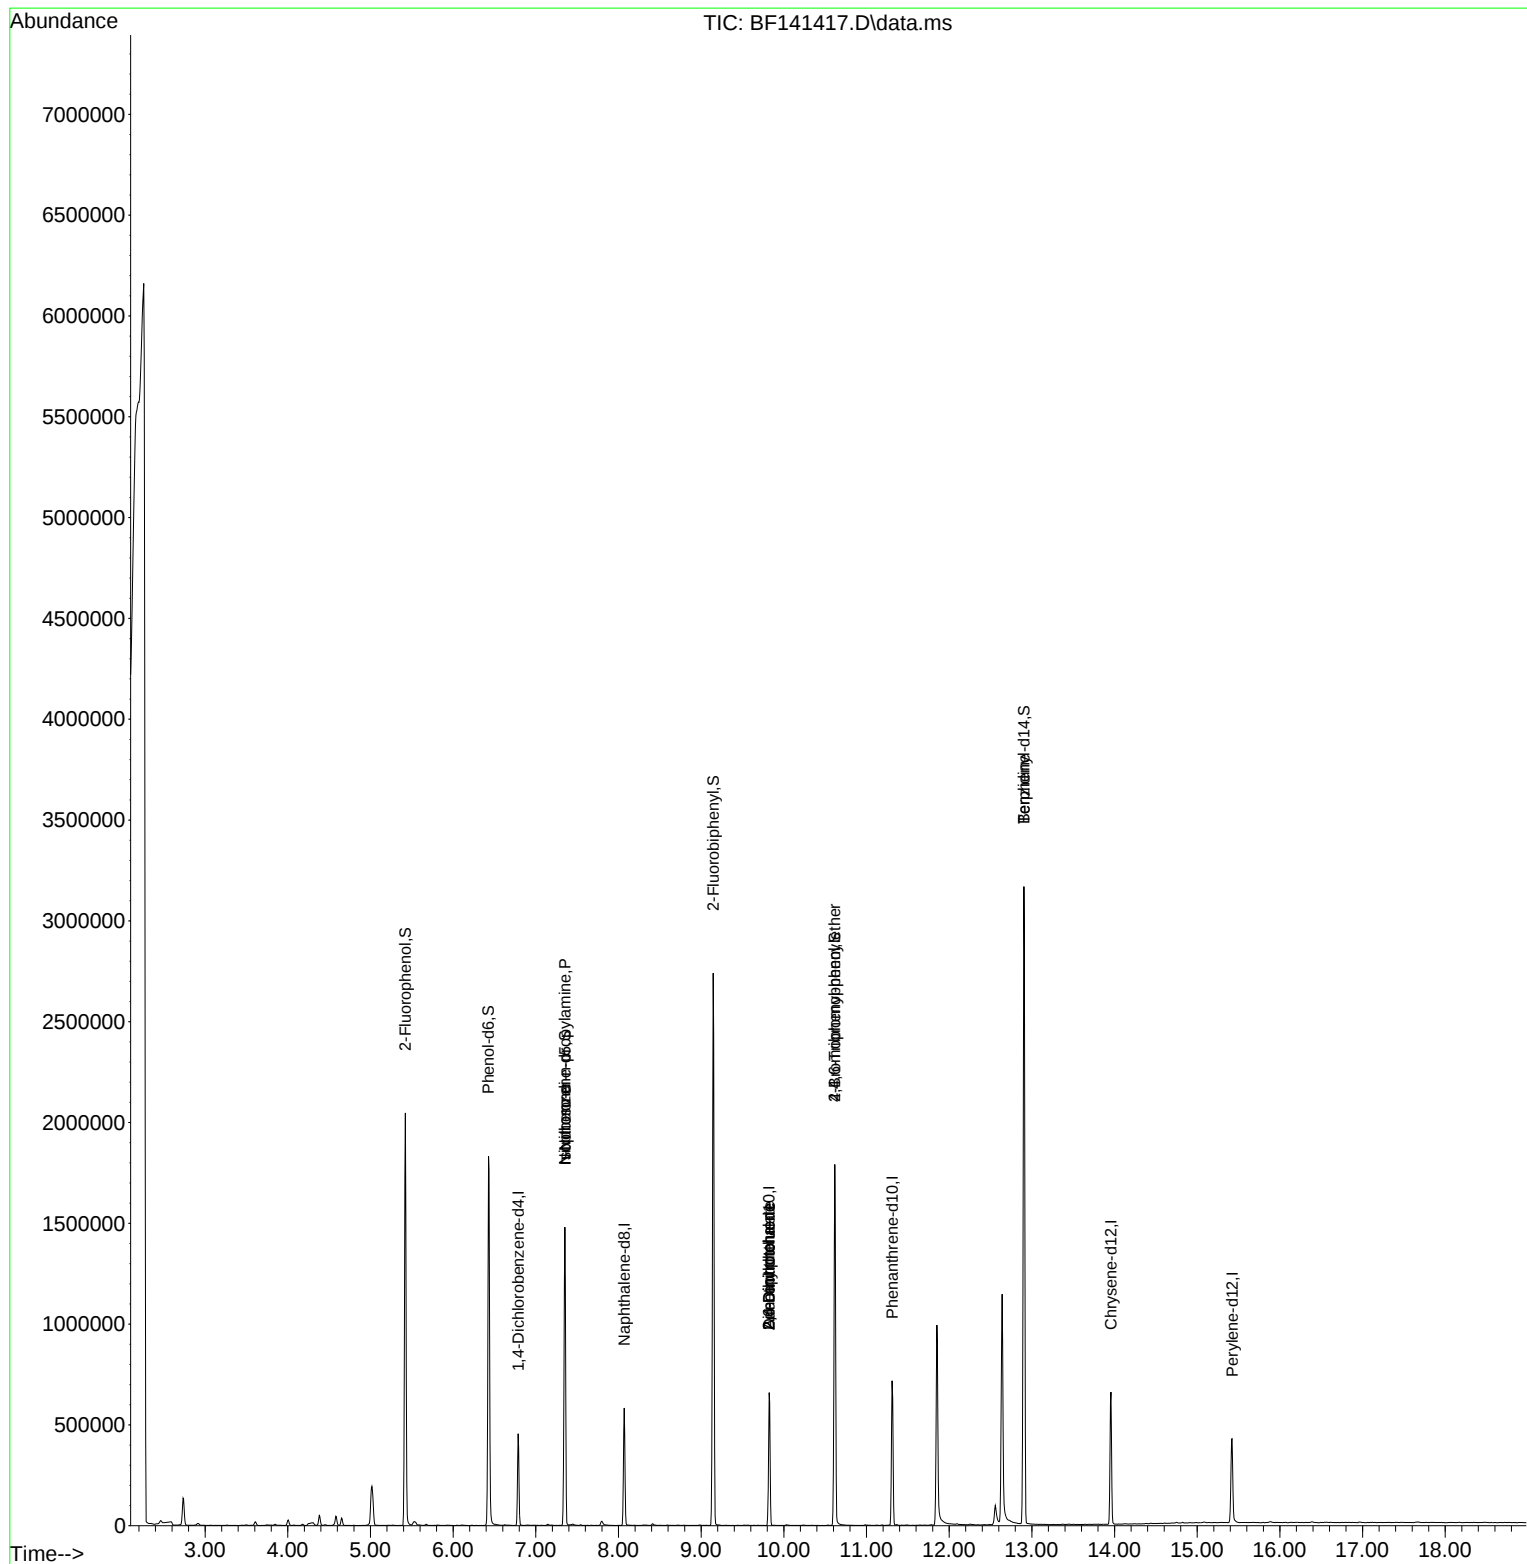




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.787 min Scan# 79
Delta R.T. -0.017 min
Lab File: BF141417.D
Acq: 04 Feb 2025 19:07




Instrument :
BNA_F
ClientSampleId :
JPP-5.4-013025


Tgt Ion:152 Resp: 87662
Ion Ratio Lower Upper
152 100
150 159.6 125.9 188.9
115 66.5 49.7 74.5

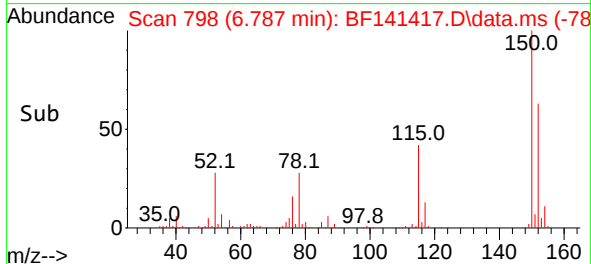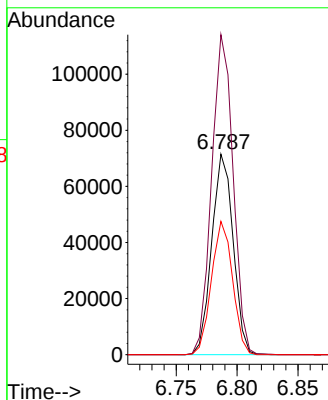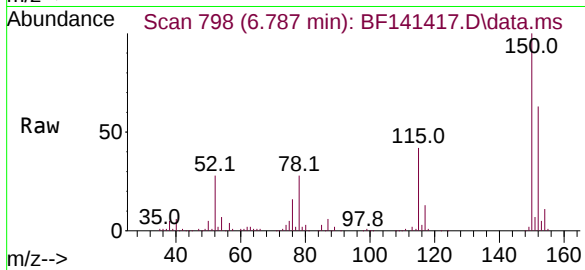

#5
2-Fluorophenol
Concen: 126.766 ng
RT: 5.422 min Scan# 566
Delta R.T. 0.012 min
Lab File: BF141417.D
Acq: 04 Feb 2025 19:07

Tgt Ion:112 Resp: 723850
Ion Ratio Lower Upper
112 100
64 62.6 49.8 74.8
63 35.0 26.1 39.1


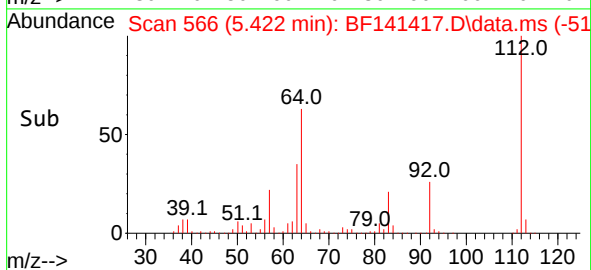
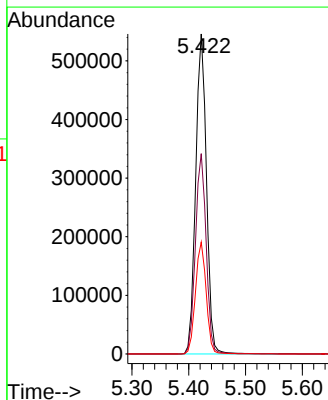
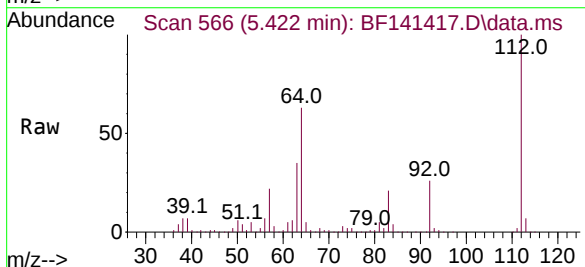




#7
Phenol-d6
Concen: 115.420 ng
RT: 6.428 min Scan# 71
Delta R.T. -0.012 min
Lab File: BF141417.D
Acq: 04 Feb 2025 19:07




Instrument :
BNA_F
ClientSampleId :
JPP-5.4-013025


Tgt Ion: 99 Resp: 838413
Ion Ratio Lower Upper
99 100
42 23.2 17.1 25.7
71 38.8 26.9 40.3

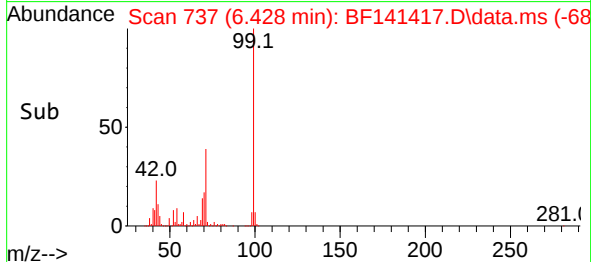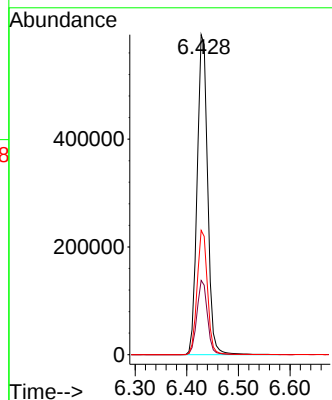

#19
n-Nitroso-di-n-propylamine
Concen: 20.951 ng
RT: 7.351 min Scan# 894
Delta R.T. 0.123 min
Lab File: BF141417.D
Acq: 04 Feb 2025 19:07

Tgt Ion: 70 Resp: 90432
Ion Ratio Lower Upper
70 100
42 55.7 56.8 85.2#
101 0.0 7.7 11.5#
130 1.9 16.8 25.2#

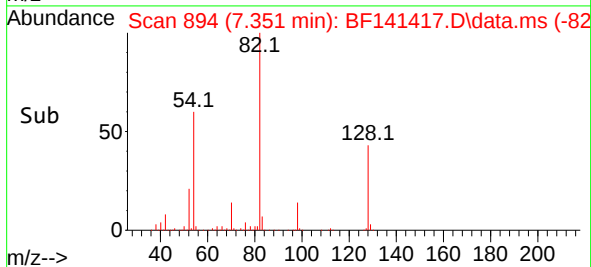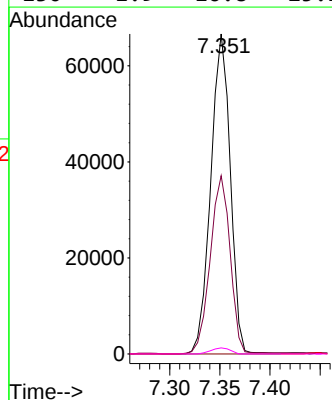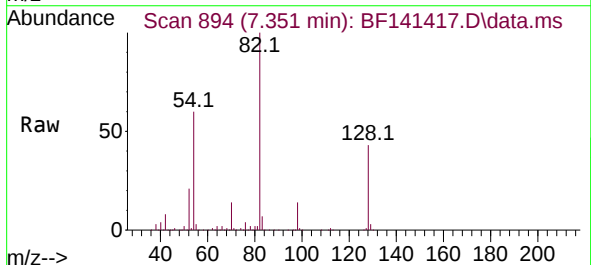







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.069 min Scan# 1018
Delta R.T. -0.018 min
Lab File: BF141417.D
Acq: 04 Feb 2025 19:07

Instrument :
BNA_F
ClientSampleId :
JPP-5.4-013025

Tgt Ion:136 Resp: 356625




Ion	Ratio	Lower	Upper
136	100		
137	10.6	8.6	13.0
54	9.0	7.8	11.8
68	4.7	4.9	7.3

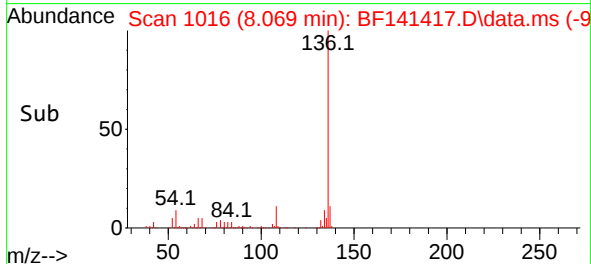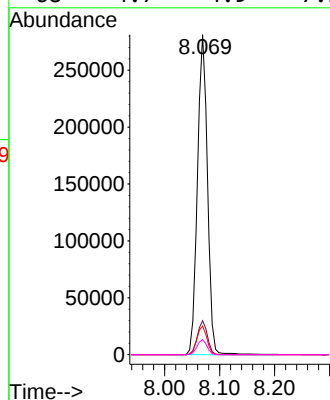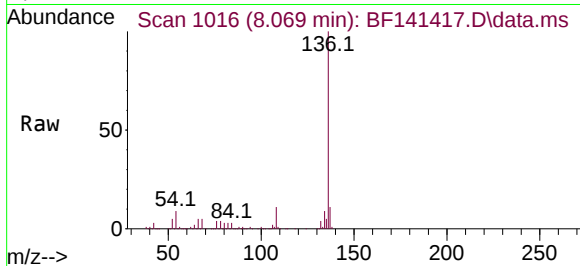


#23
Nitrobenzene-d5
Concen: 96.308 ng
RT: 7.351 min Scan# 894
Delta R.T. -0.018 min
Lab File: BF141417.D
Acq: 04 Feb 2025 19:07

Tgt Ion: 82 Resp: 651522

Ion	Ratio	Lower	Upper
82	100		
128	43.5	35.7	53.5
54	59.8	47.1	70.7


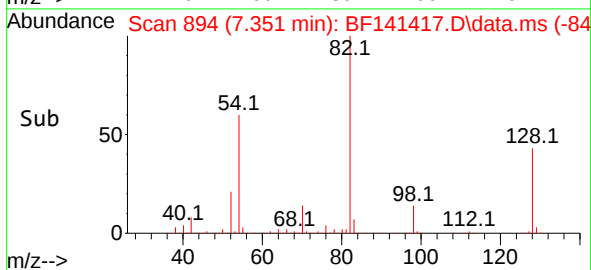
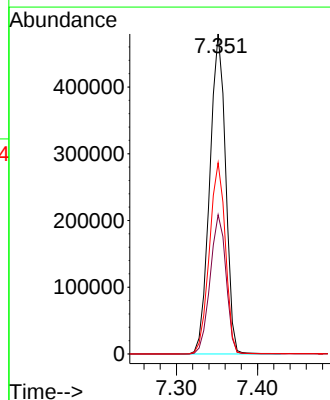
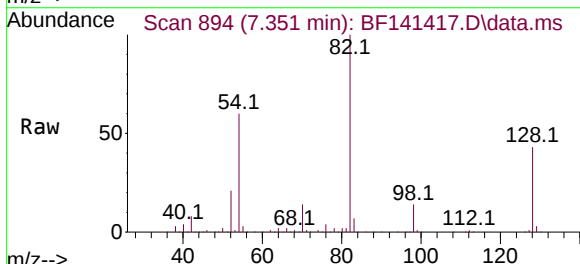




#25
Isophorone
Concen: 55.305 ng
RT: 7.351 min Scan# 894
Delta R.T. -0.277 min
Lab File: BF141417.D
Acq: 04 Feb 2025 19:07




Instrument :
BNA_F
ClientSampleId :
JPP-5.4-013025


Tgt Ion: 82 Resp: 646732
Ion Ratio Lower Upper
82 100
95 0.0 5.8 8.6#
138 0.0 14.7 22.1#

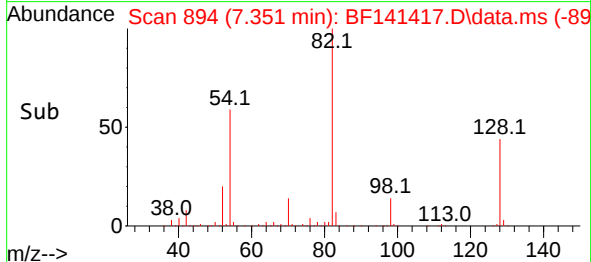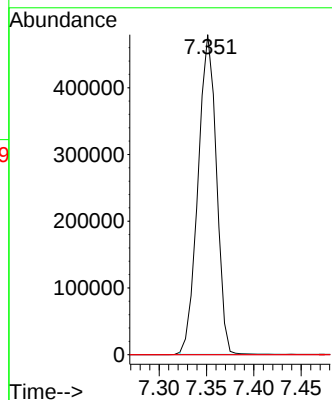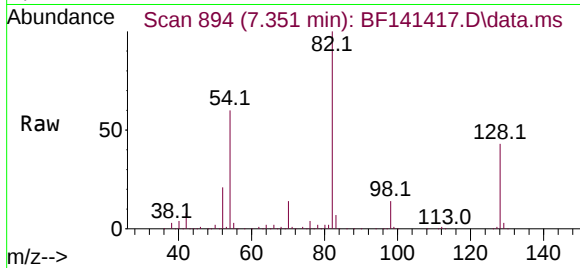

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.822 min Scan# 1314
Delta R.T. -0.018 min
Lab File: BF141417.D
Acq: 04 Feb 2025 19:07

Tgt Ion:164 Resp: 198235
Ion Ratio Lower Upper
164 100
162 102.6 80.6 121.0
160 46.0 35.8 53.6

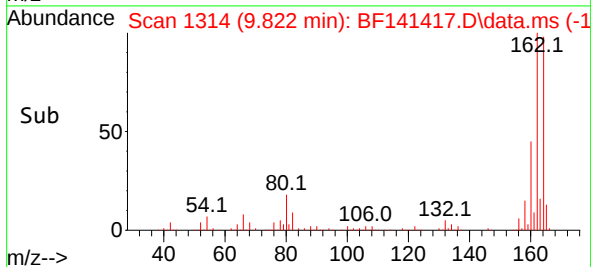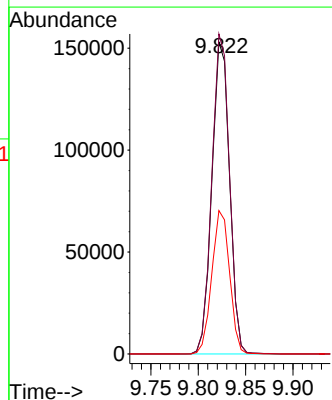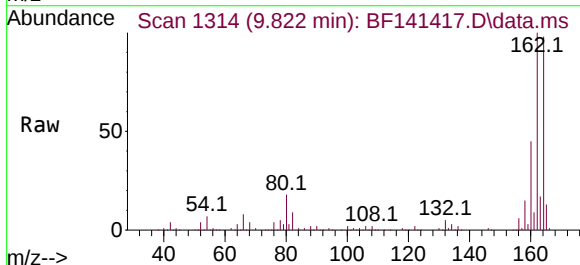



#42

2,4,6-Tribromophenol

Concen: 164.346 ng

RT: 10.616 min Scan# 1449

Delta R.T. -0.018 min

Lab File: BF141417.D


Acq: 04 Feb 2025 19:07

Instrument :

BNA_F

ClientSampleId :

JPP-5.4-013025

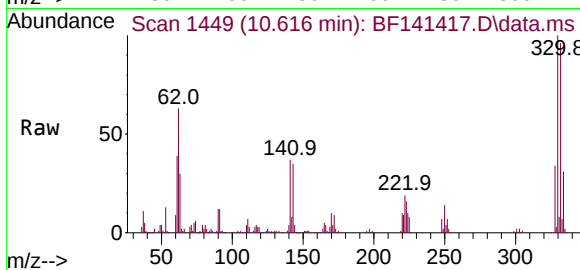




Tgt Ion:330 Resp: 298675

Ion Ratio Lower Upper

330 100

332 96.0 76.1 114.1

141 36.1 28.8 43.2

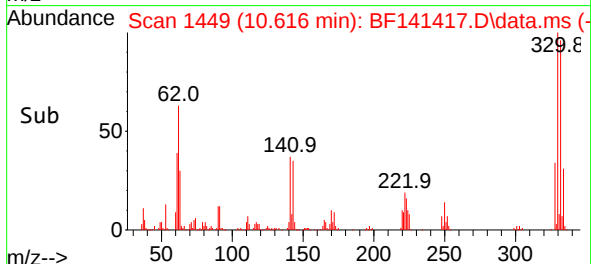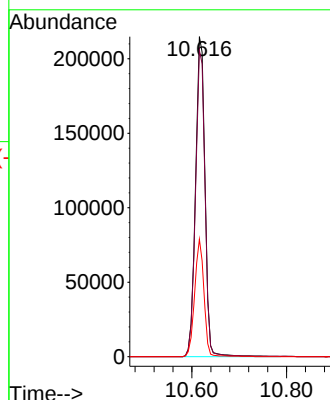

#45

2-Fluorobiphenyl

Concen: 94.559 ng

RT: 9.145 min Scan# 1199

Delta R.T. -0.018 min

Lab File: BF141417.D

Acq: 04 Feb 2025 19:07




Tgt Ion:172 Resp: 1217841


Ion Ratio Lower Upper

172 100

171 36.4 28.8 43.2

170 23.8 19.0 28.6


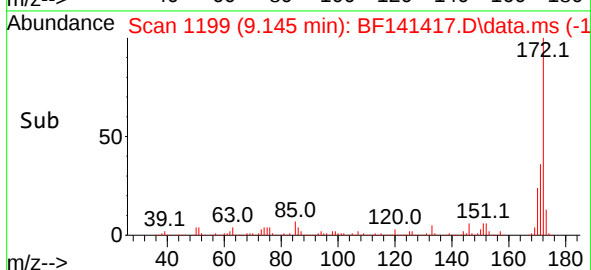

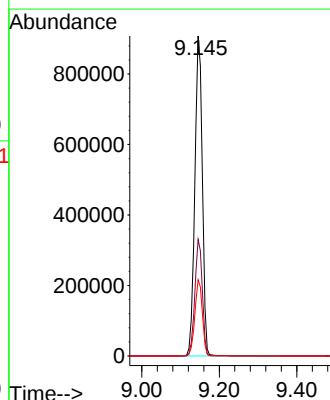




#50
Dimethylphthalate
Concen: 2.039 ng
RT: 9.822 min Scan# 1314
Delta R.T. 0.253 min
Lab File: BF141417.D
Acq: 04 Feb 2025 19:07




Instrument :
BNA_F
ClientSampleId :
JPP-5.4-013025


Tgt Ion:163 Resp: 27302
Ion Ratio Lower Upper
163 100
194 0.0 3.0 4.6#
164 585.2 8.0 12.0#

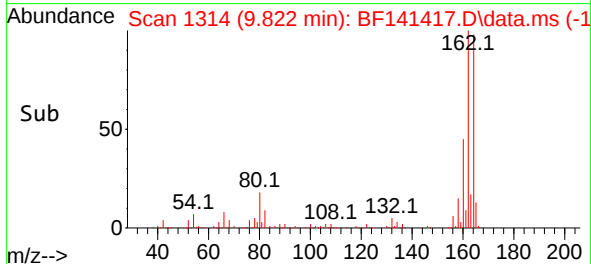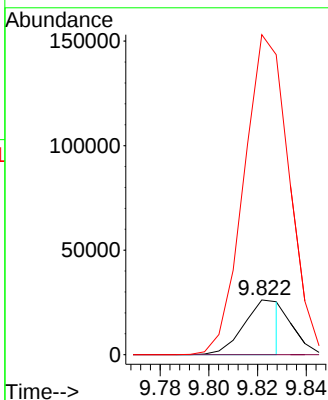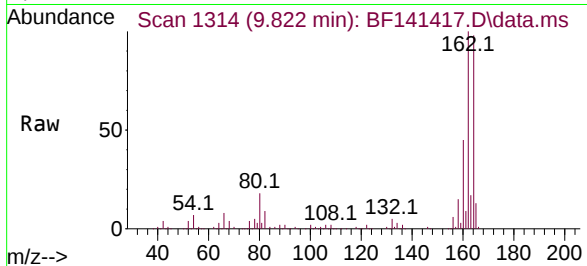

#51
2,6-Dinitrotoluene
Concen: 8.225 ng
RT: 9.822 min Scan# 1314
Delta R.T. 0.194 min
Lab File: BF141417.D
Acq: 04 Feb 2025 19:07


Tgt Ion:165 Resp: 25568
Ion Ratio Lower Upper
165 100
63 1.4 48.1 72.1#
89 1.5 44.9 67.3#

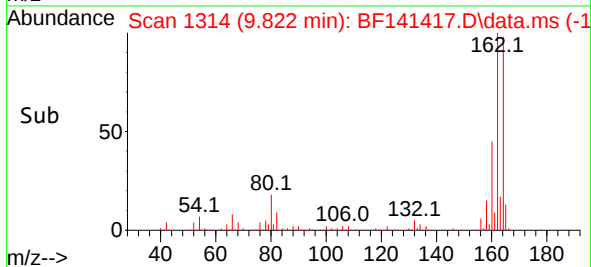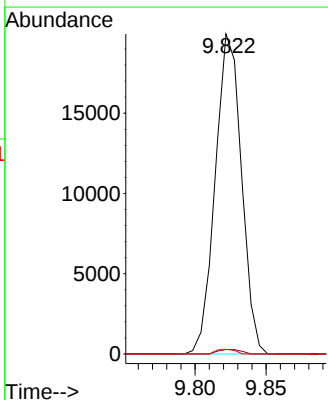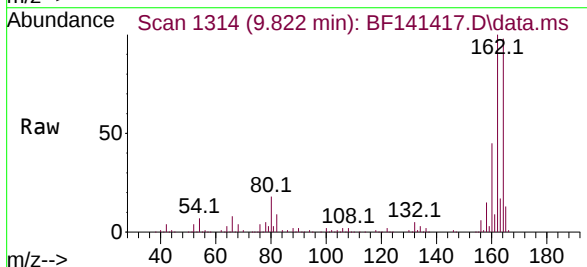






#57
2,4-Dinitrotoluene
Concen: 6.352 ng
RT: 9.822 min Scan# 11
Delta R.T. -0.212 min
Lab File: BF141417.D
Acq: 04 Feb 2025 19:07


Instrument :
BNA_F
ClientSampleId :
JPP-5.4-013025





Tgt Ion:165 Resp: 25568
Ion Ratio Lower Upper
165 100
63 1.4 39.2 58.8#
89 1.5 56.9 85.3#
182 0.0 2.2 3.2#

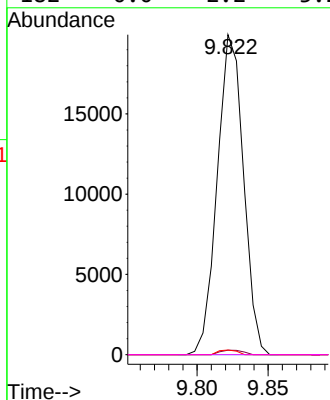


#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.310 min Scan# 1567
Delta R.T. -0.018 min
Lab File: BF141417.D
Acq: 04 Feb 2025 19:07

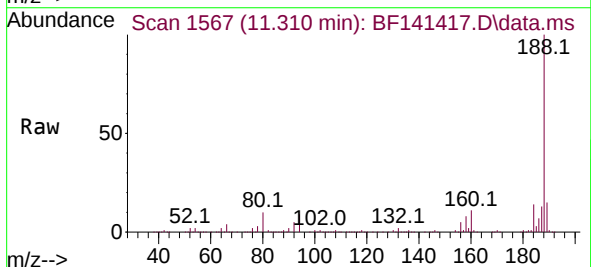

Tgt Ion:188 Resp: 358571
Ion Ratio Lower Upper
188 100
94 8.7 7.8 11.6
80 9.6 8.2 12.4



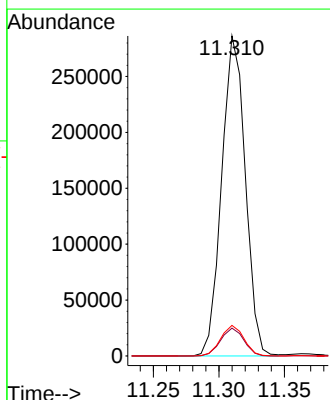





#67
4-Bromophenyl-phenylether
Concen: 5.085 ng
RT: 10.616 min Scan# 14
Delta R.T. -0.259 min
Lab File: BF141417.D
Acq: 04 Feb 2025 19:07




Instrument :
BNA_F
ClientSampleId :
JPP-5.4-013025


Tgt Ion:248 Resp: 20413
Ion Ratio Lower Upper
248 100
250 194.9 79.0 118.4#
141 514.8 63.7 95.5#

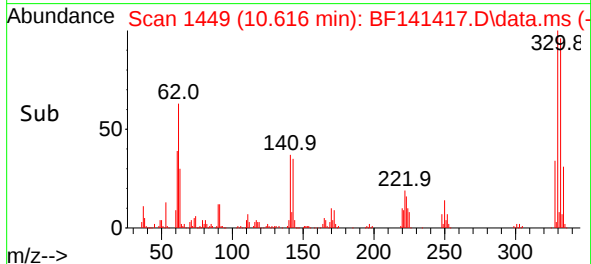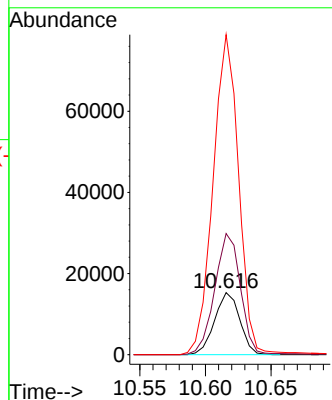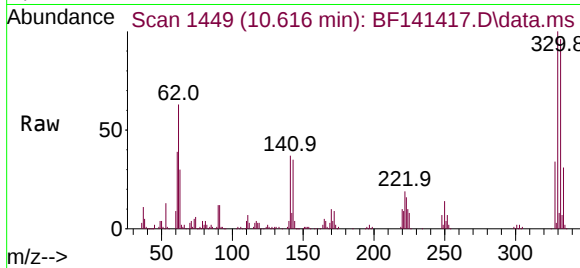

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.957 min Scan# 2017
Delta R.T. -0.018 min
Lab File: BF141417.D
Acq: 04 Feb 2025 19:07

Tgt Ion:240 Resp: 323769
Ion Ratio Lower Upper
240 100
120 9.5 10.0 15.0#
236 25.1 19.7 29.5


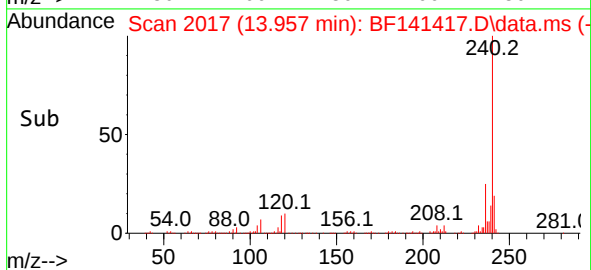
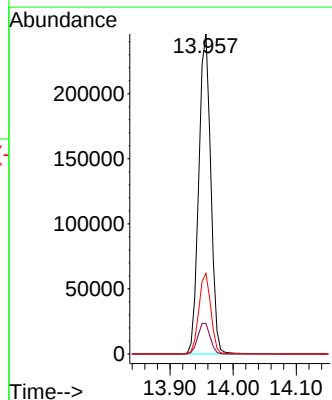
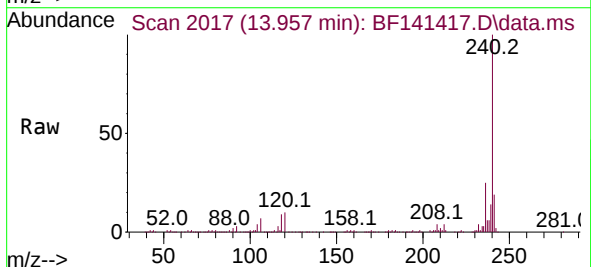




#77
Benzidine
Concen: 2.083 ng
RT: 12.904 min Scan# 1838
Delta R.T. 0.241 min
Lab File: BF141417.D
Acq: 04 Feb 2025 19:07




Instrument :
BNA_F
ClientSampleId :
JPP-5.4-013025


Tgt Ion:184 Resp: 21618
Ion Ratio Lower Upper
184 100
185 17.2 11.9 17.9
183 6.6 9.5 14.3#

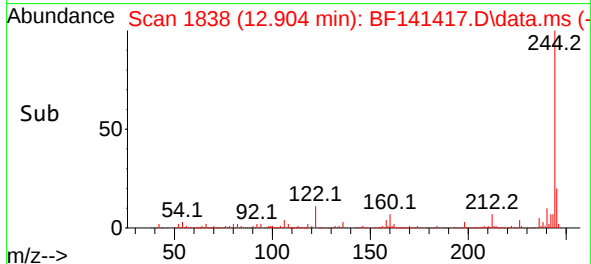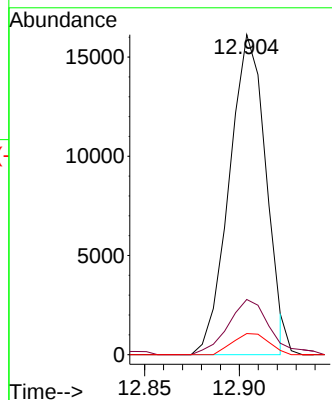

#79
Terphenyl-d14
Concen: 75.456 ng
RT: 12.904 min Scan# 1838
Delta R.T. -0.012 min
Lab File: BF141417.D
Acq: 04 Feb 2025 19:07


Tgt Ion:244 Resp: 1584137
Ion Ratio Lower Upper
244 100
212 7.2 5.4 8.0
122 11.2 8.8 13.2

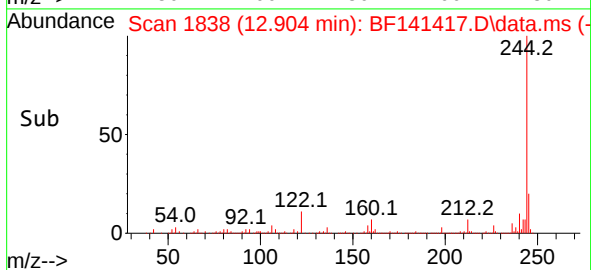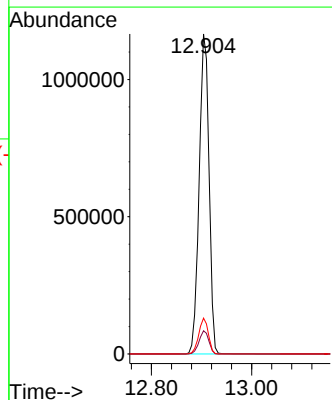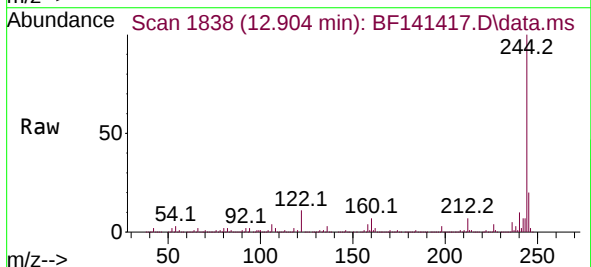



#86
Perylene-d12
Concen: 20.000 ng
RT: 15.421 min Scan# 21
Delta R.T. -0.018 min
Lab File: BF141417.D
Acq: 04 Feb 2025 19:07

Instrument :
BNA_F
ClientSampleId :
JPP-5.4-013025

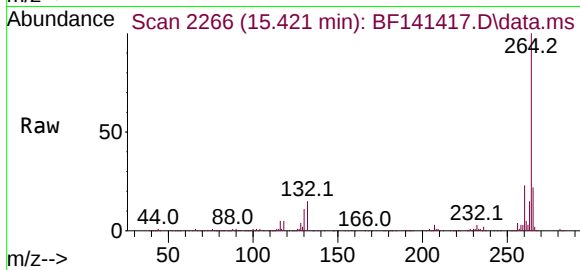

Tgt Ion:264 Resp: 258055

Ion	Ratio	Lower	Upper
264	100		
260	23.1	18.6	27.8
265	21.7	16.7	25.1

