
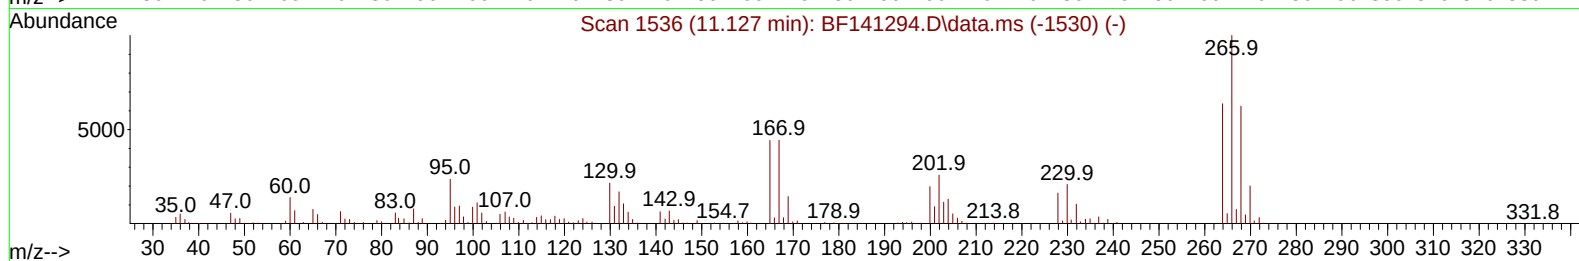
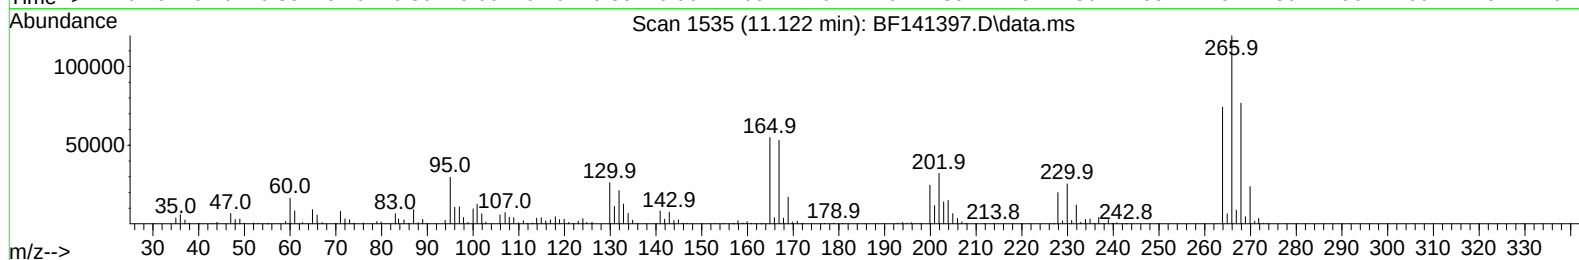


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020425\
Data File : BF141397.D
Acq On : 04 Feb 2025 10:16
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 04 11:33:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 29 17:41:25 2025
Response via : Initial Calibration

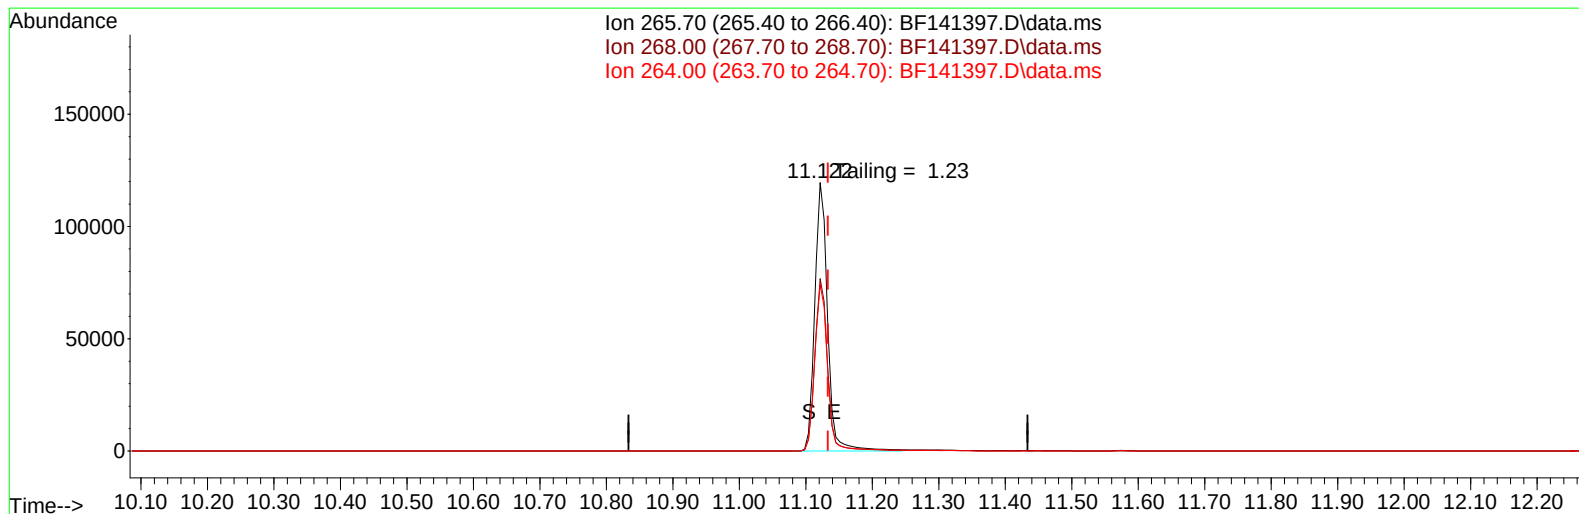

TIC: BF141397.D\data.ms

(70) Pentachlorophenol (C)




11.122min (-0.012) 45312.00 ng

response 160702

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	64.23
264.00	63.70	62.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020425\
Data File : BF141397.D
Acq On : 04 Feb 2025 10:16
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 04 11:33:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 29 17:41:25 2025
Response via : Initial Calibration

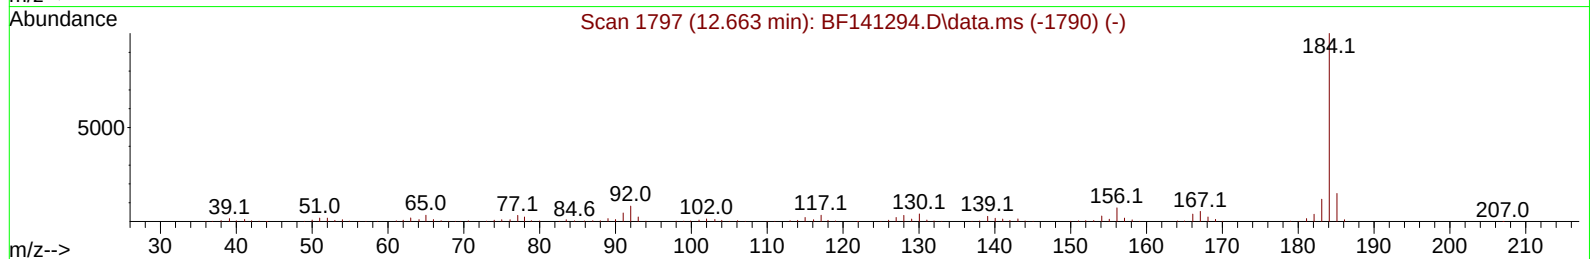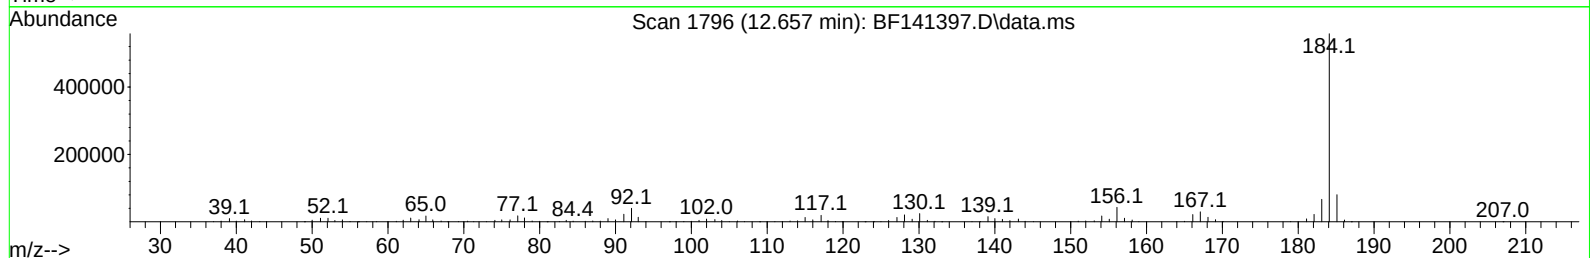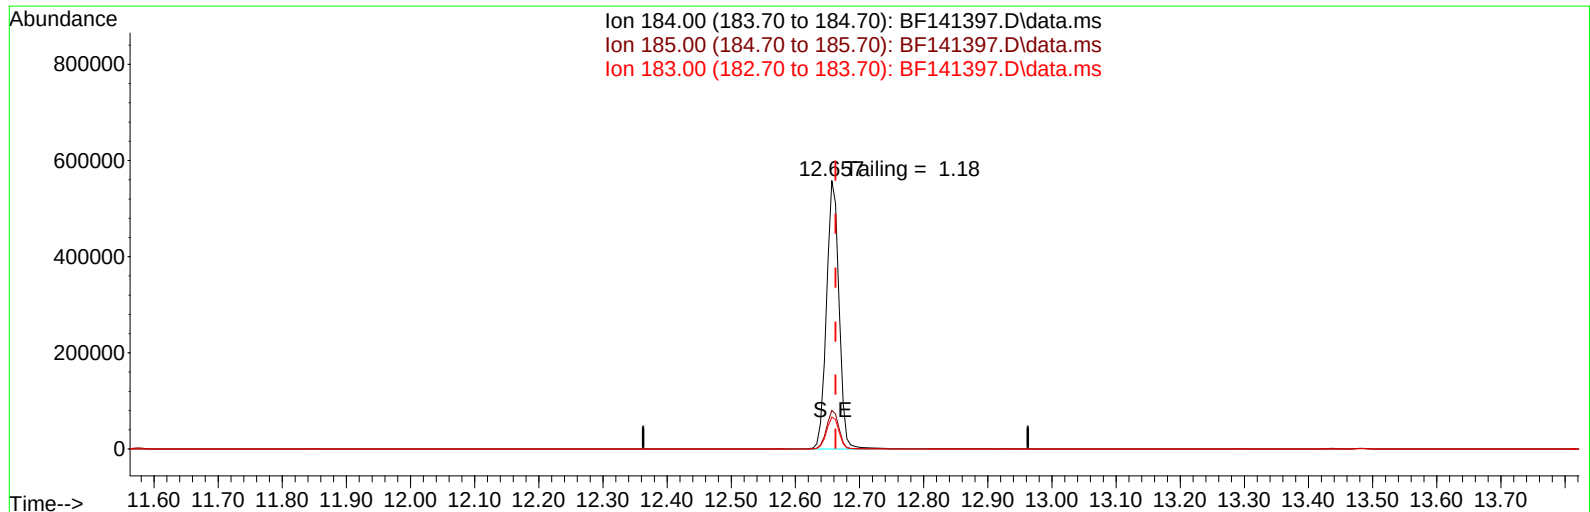

TIC: BF141397.D\data.ms

(77) Benzidine

12.657min (-0.006) 113140.91 ng

response 761695

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.38
183.00	11.90	11.93
0.00	0.00	0.00