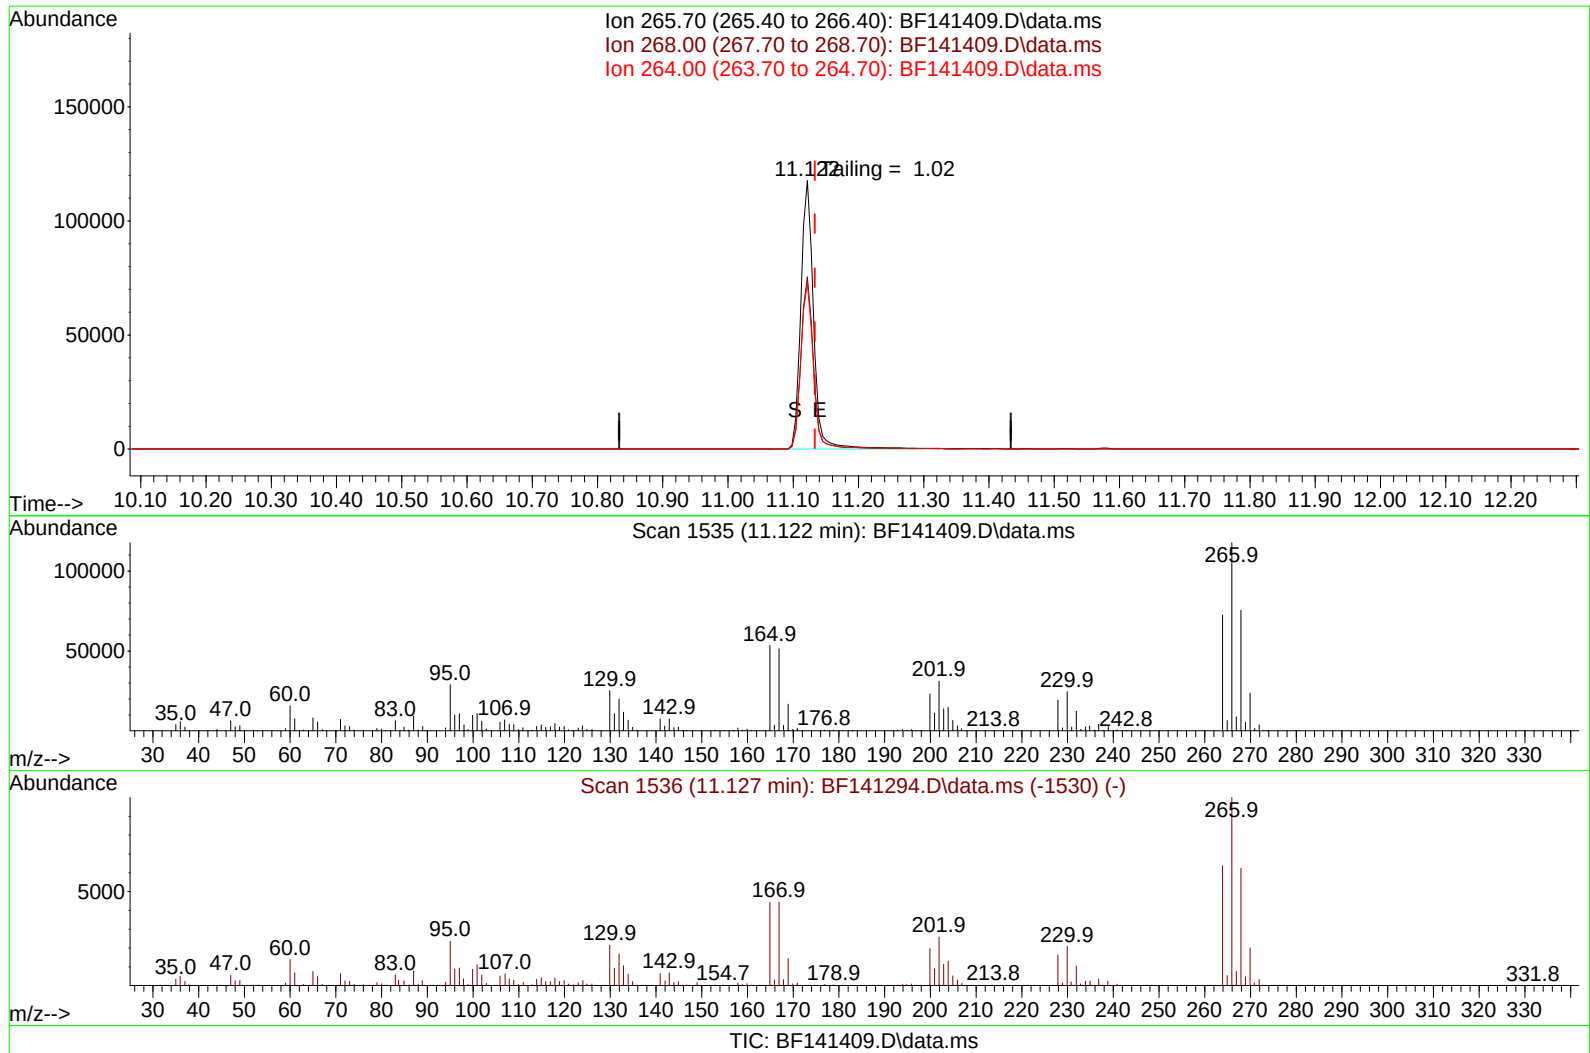


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020425\
Data File : BF141409.D
Acq On : 04 Feb 2025 15:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1




Quant Time: Feb 04 16:10:34 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 29 17:41:25 2025
Response via : Initial Calibration

**(70) Pentachlorophenol (C)****11.122min (-0.012) 188004.57 ng****response 159502**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	64.16
264.00	63.70	61.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020425\
Data File : BF141409.D
Acq On : 04 Feb 2025 15:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 04 16:10:34 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 29 17:41:25 2025
Response via : Initial Calibration

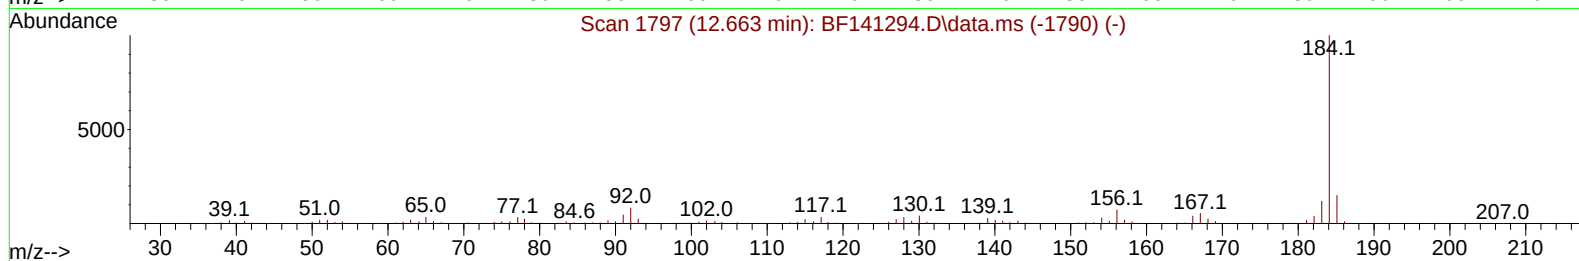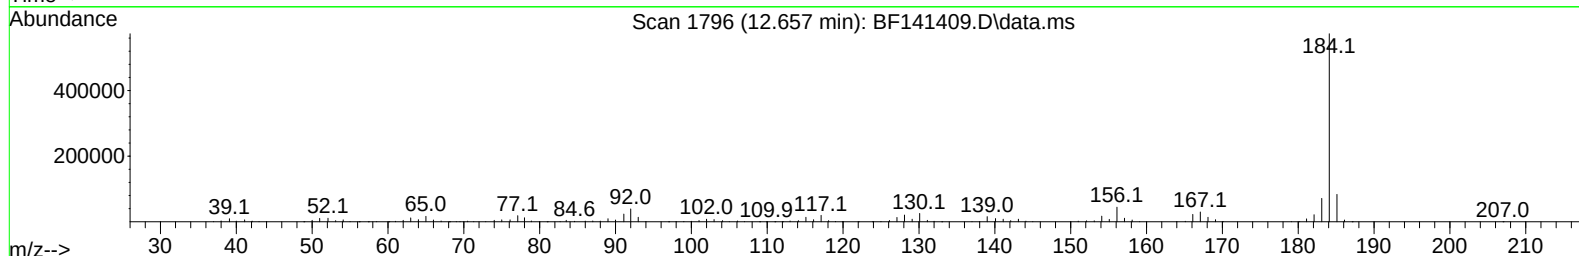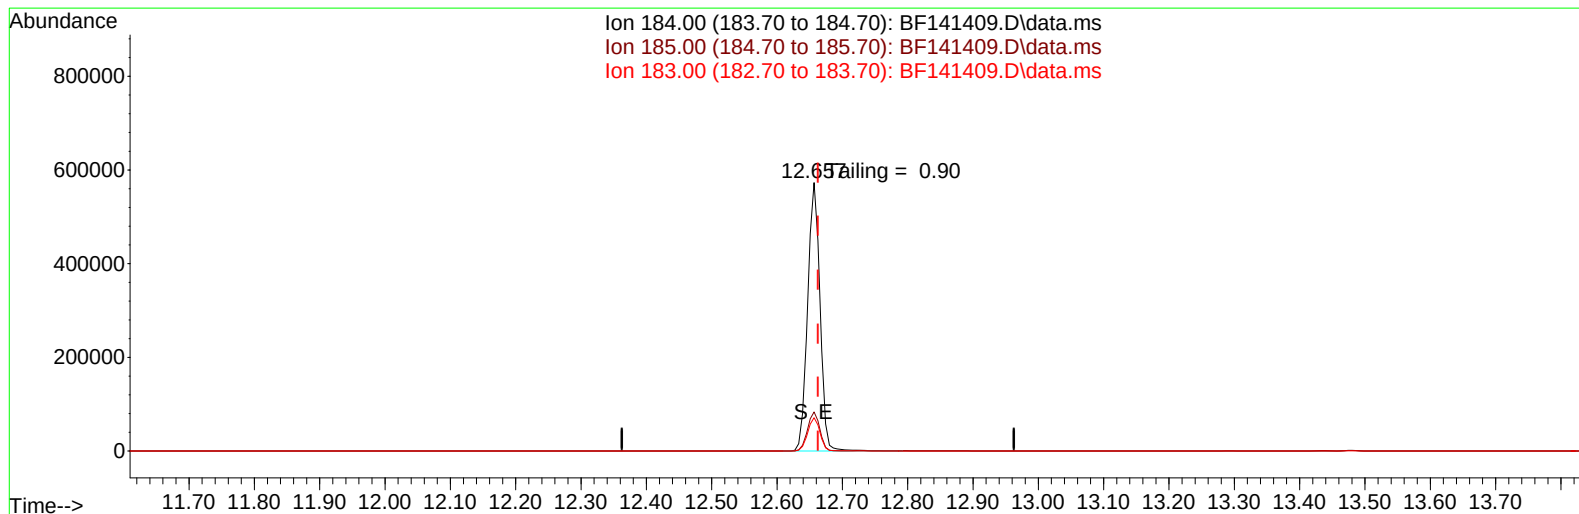

TIC: BF141409.D\data.ms

(77) Benzidine

12.657min (-0.006) 200133.30 ng m

response 757083

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.56
183.00	11.90	12.42
0.00	0.00	0.00