

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020425\
 Data File : BF141403.D
 Acq On : 04 Feb 2025 12:54
 Operator : RC/JU
 Sample : PB166465BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB166465BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141403.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.152	6	10	16	rVB	27883	44219	1.21%	0.216%
2	5.410	559	564	585	rBV	2009897	2747740	75.33%	13.437%
3	6.428	731	737	765	rBV	2069394	2756235	75.56%	13.479%
4	6.787	793	798	803	rBV	440665	533488	14.63%	2.609%
5	7.351	887	894	899	rBV	1347936	1815091	49.76%	8.876%
6	8.069	1011	1016	1028	rBV	548698	700467	19.20%	3.426%
7	9.145	1193	1199	1205	rBV	2454524	3311331	90.78%	16.193%
8	9.827	1309	1315	1327	rVB	614441	803845	22.04%	3.931%
9	10.616	1443	1449	1466	rBV	1564653	2048736	56.17%	10.019%
10	11.310	1562	1567	1575	rBV	632164	823927	22.59%	4.029%
11	12.904	1832	1838	1843	rBV	2750228	3647515	100.00%	17.838%
12	13.957	2012	2017	2028	rBV	541926	687194	18.84%	3.361%
13	15.415	2259	2265	2276	rBV	340204	528773	14.50%	2.586%




Sum of corrected areas: 20448561

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020425\
Data File : BF141403.D
Acq On : 04 Feb 2025 12:54
Operator : RC/JU
Sample : PB166465BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166465BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

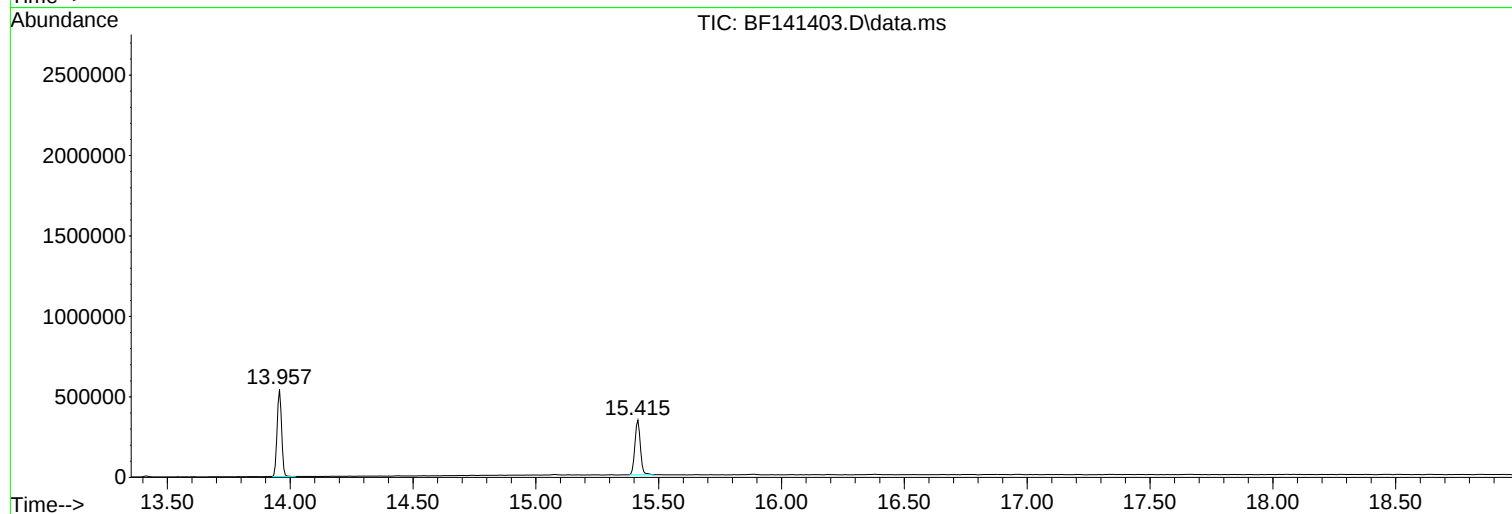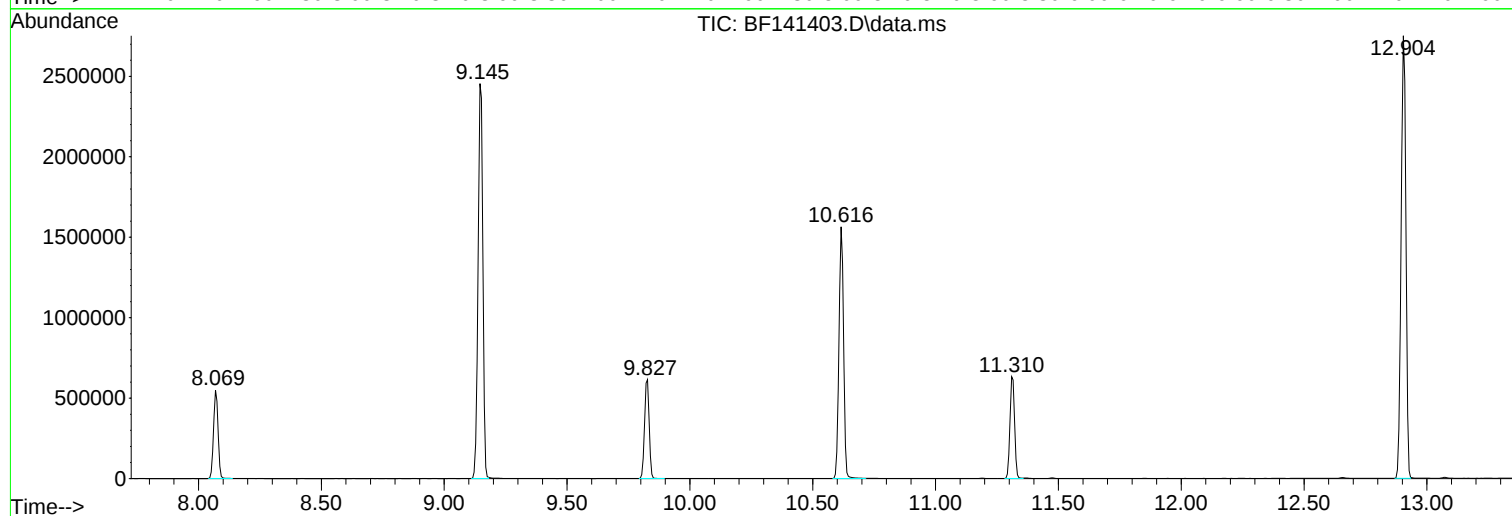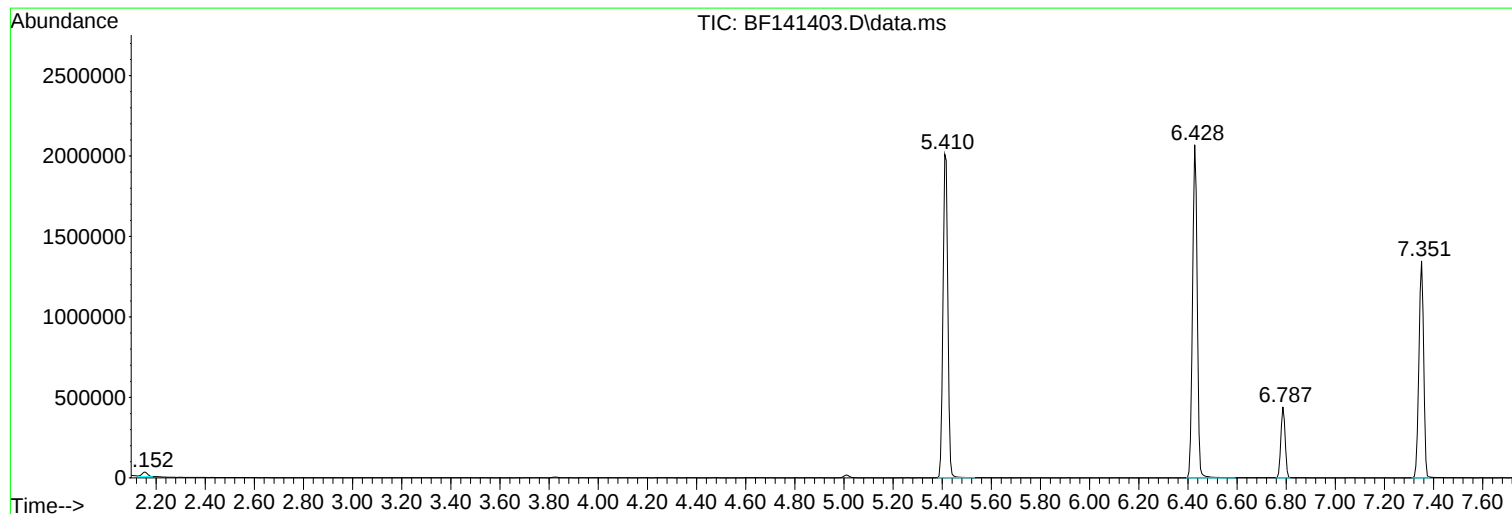

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020425\
Data File : BF141403.D
Acq On : 04 Feb 2025 12:54
Operator : RC/JU
Sample : PB166465BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166465BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020425\
Data File : BF141403.D
Acq On : 04 Feb 2025 12:54
Operator : RC/JU
Sample : PB166465BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166465BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------