

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020425\
Data File : BF141411.D
Acq On : 04 Feb 2025 16:24
Operator : RC/JU
Sample : PB166525BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166525BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141411.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.410	559	564	586	rBV	1955386	2680296	74.60%	13.594%
2	6.428	731	737	757	rBV	2009340	2708551	75.38%	13.738%
3	6.787	793	798	803	rBV	397838	477990	13.30%	2.424%
4	7.351	887	894	899	rBV	1311570	1808830	50.34%	9.174%
5	8.069	1010	1016	1027	rBV	498562	635279	17.68%	3.222%
6	9.145	1193	1199	1204	rBV	2489084	3300294	91.85%	16.739%
7	9.822	1309	1314	1329	rVB	556625	724468	20.16%	3.674%
8	10.616	1443	1449	1472	rBV	1531175	2000568	55.68%	10.147%
9	11.310	1562	1567	1574	rBV	564788	726842	20.23%	3.687%
10	12.904	1832	1838	1843	rBV	2736233	3593095	100.00%	18.224%
11	13.957	2011	2017	2030	rBV	463153	598421	16.65%	3.035%
12	15.421	2259	2266	2281	rBV	283634	461659	12.85%	2.342%




Sum of corrected areas: 19716293

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020425\
Data File : BF141411.D
Acq On : 04 Feb 2025 16:24
Operator : RC/JU
Sample : PB166525BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166525BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

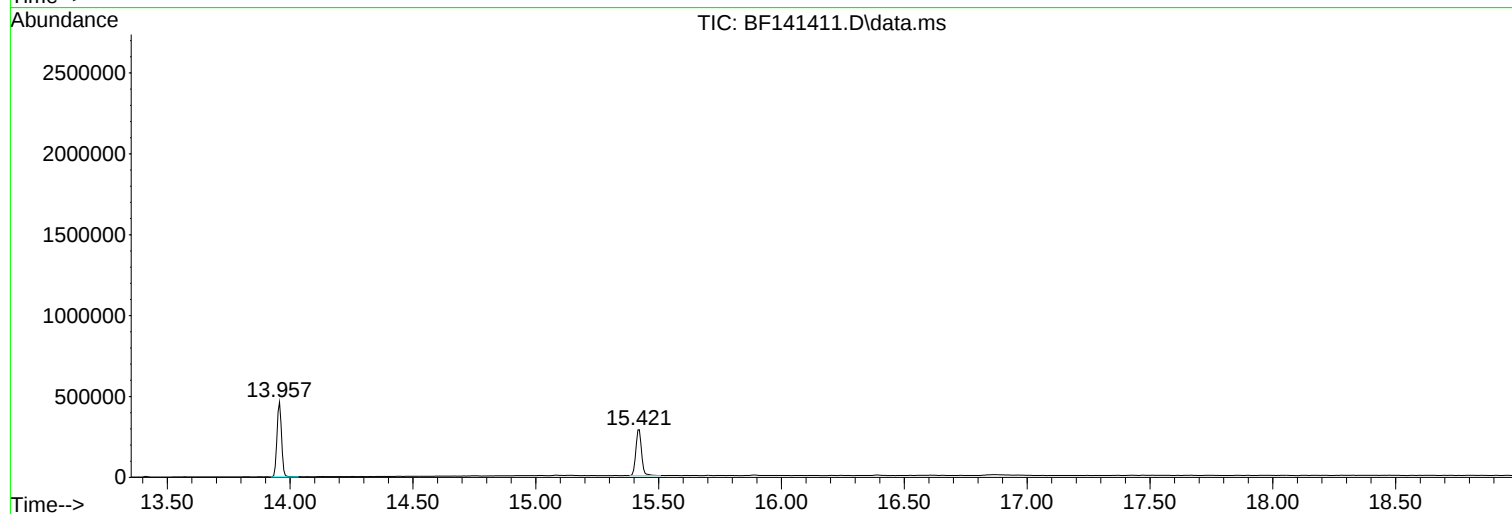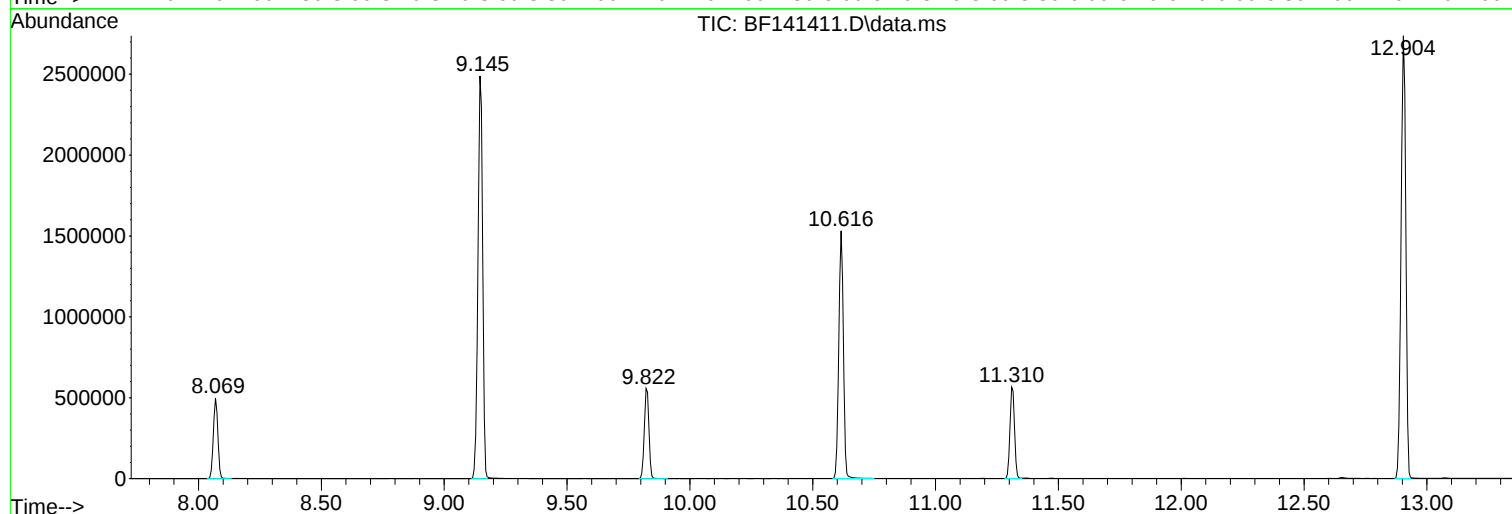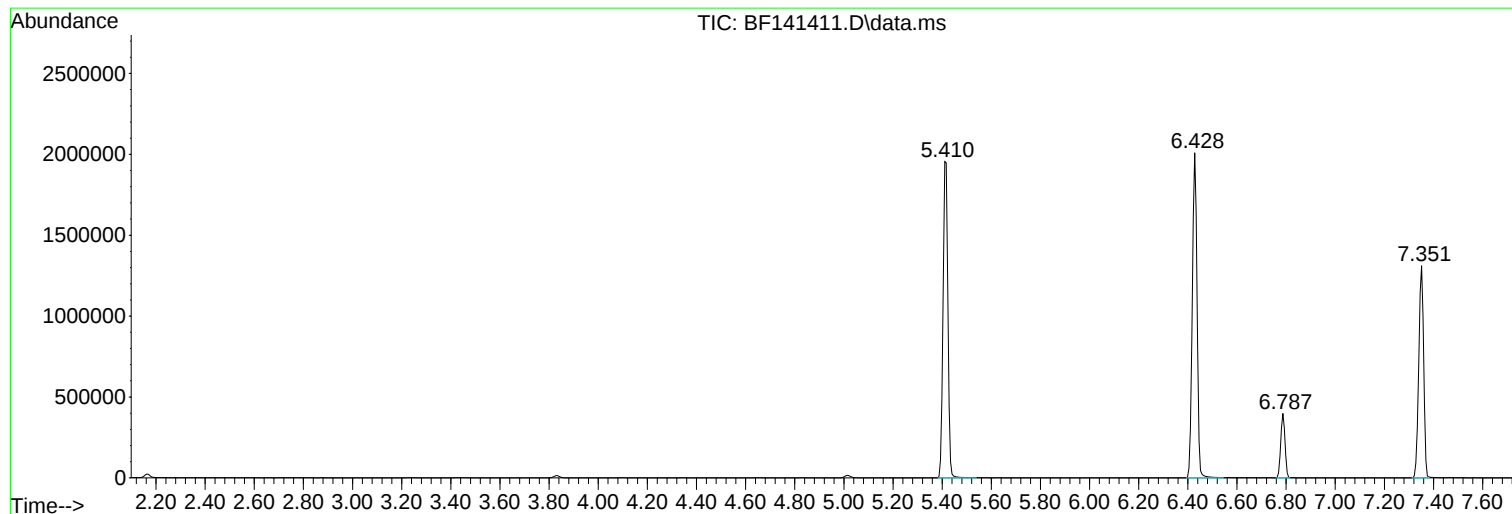

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020425\
Data File : BF141411.D
Acq On : 04 Feb 2025 16:24
Operator : RC/JU
Sample : PB166525BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166525BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020425\
Data File : BF141411.D
Acq On : 04 Feb 2025 16:24
Operator : RC/JU
Sample : PB166525BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166525BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------