


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020425\
Data File : BF141397.D
Acq On : 04 Feb 2025 10:16
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jan 29 17:41:25 2025

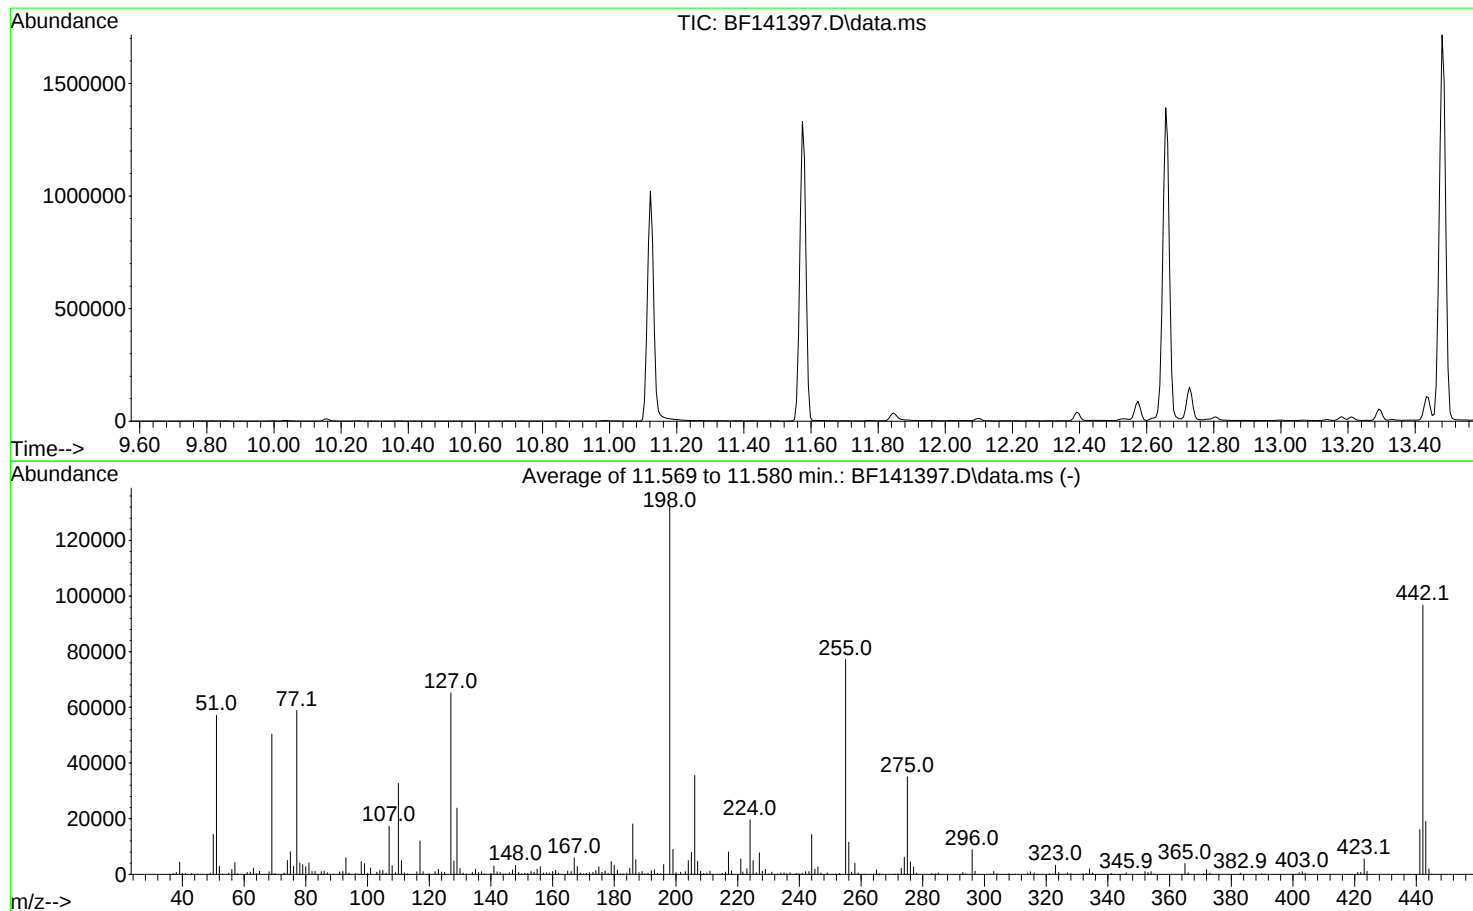

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.3	57171	PASS
68	69	0.00	2	1.9	947	PASS
69	198	0.00	100	38.1	50408	PASS
70	69	0.00	2	0.6	288	PASS
127	198	10	80	49.4	65259	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	132187	PASS
199	198	5	9	6.8	8986	PASS
275	198	10	60	26.5	35069	PASS
365	198	1	100	3.0	3931	PASS
441	198	0.01	100	12.2	16076	PASS
442	442	50	100	100.0	96717	PASS
443	442	15	24	19.7	19012	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/4/2025	BNA_F	<u>BF141397.D</u>
Compound Name	Response	Retention Time
DDT	430190	13.48
DDD	8939	13.18
DDE	241	12.845
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9180	439370	2.09

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020425\
Data File : BF141397.D
Acq On : 04 Feb 2025 10:16
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 04 11:33:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 29 17:41:25 2025
Response via : Initial Calibration

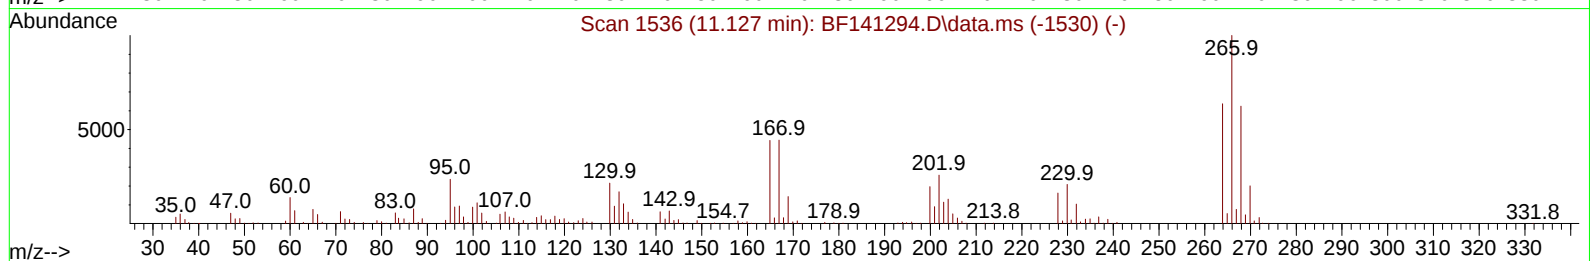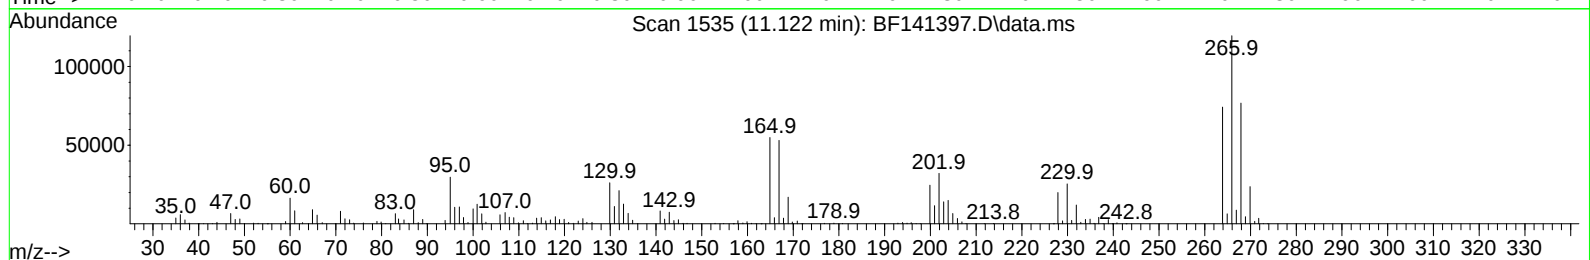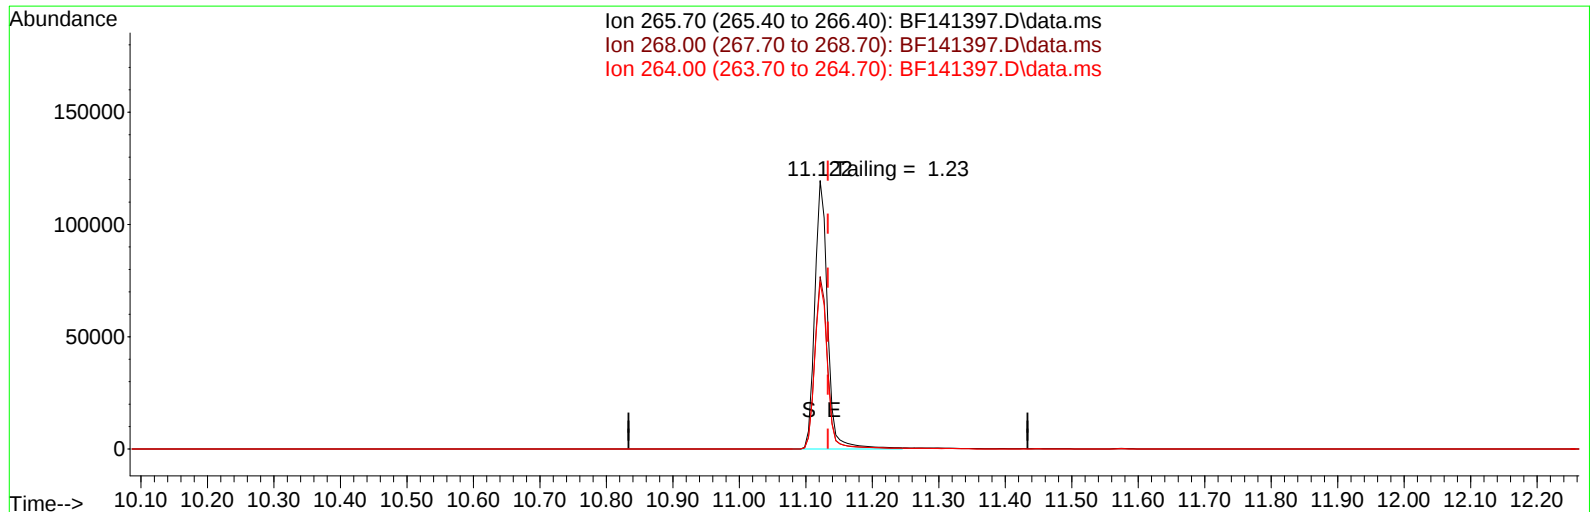

TIC: BF141397.D\data.ms

(70) Pentachlorophenol (C)

11.122min (-0.012) 45312.00 ng




response 160702

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	64.23
264.00	63.70	62.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020425\
Data File : BF141397.D
Acq On : 04 Feb 2025 10:16
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 04 11:33:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 29 17:41:25 2025
Response via : Initial Calibration

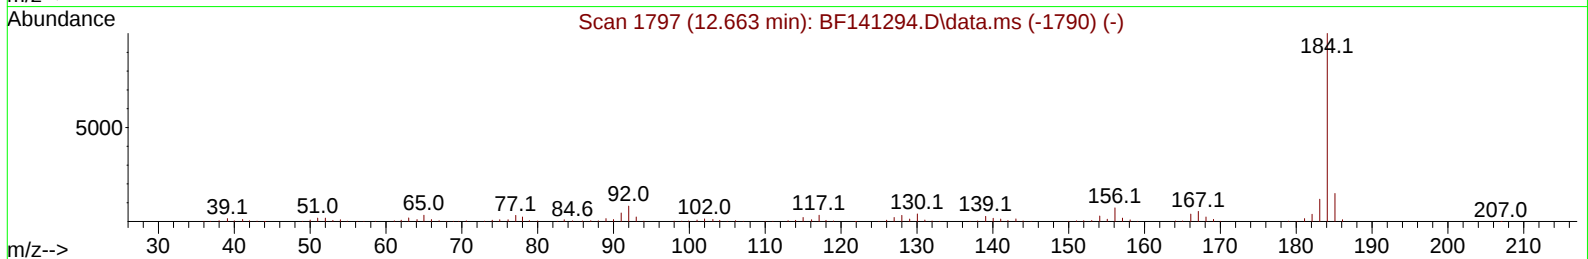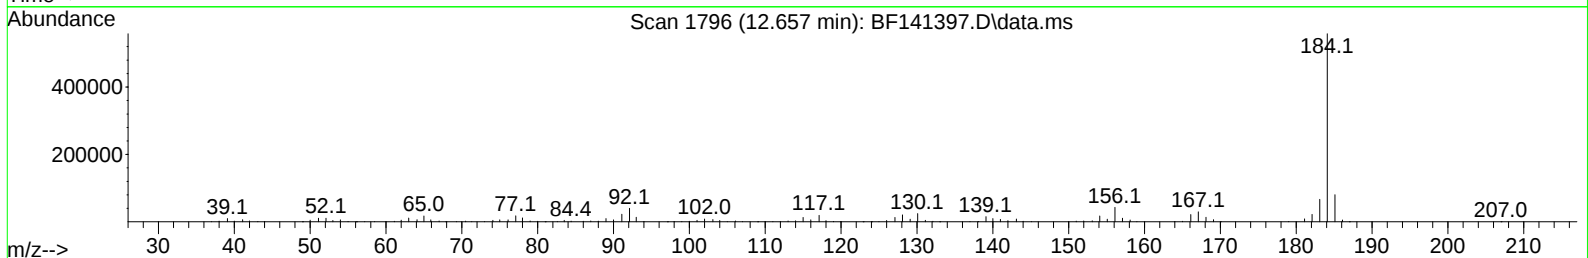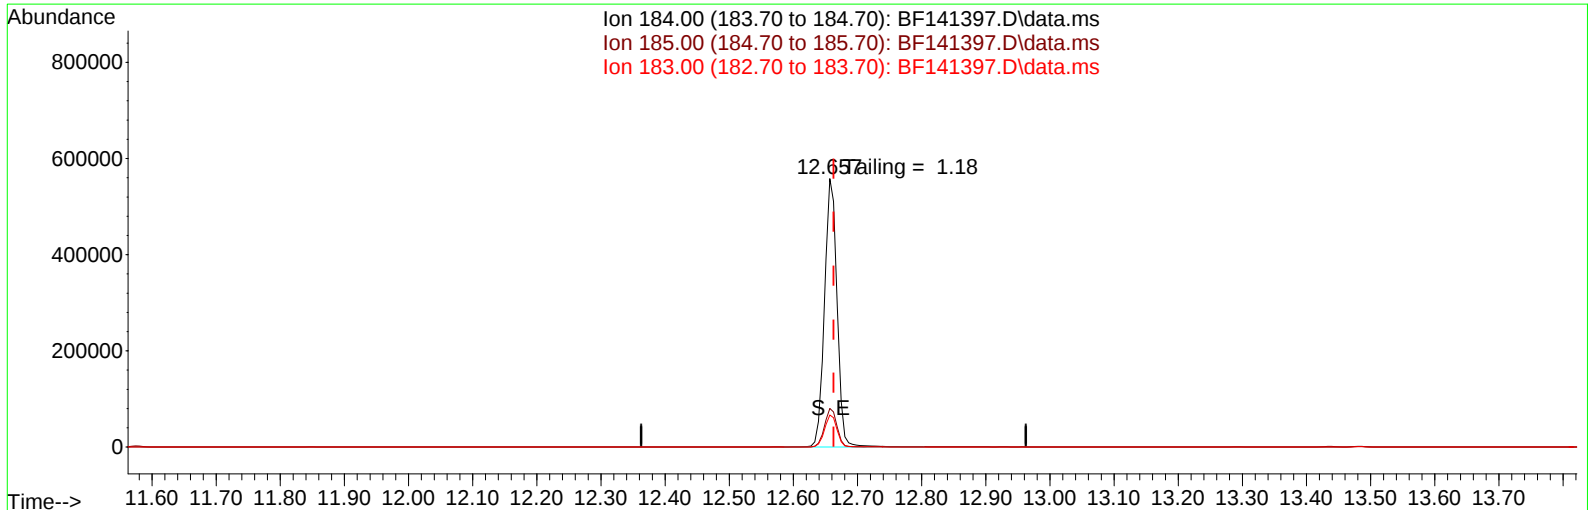

TIC: BF141397.D\data.ms

(77) Benzidine

12.657min (-0.006) 113140.91 ng

response 761695

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.38
183.00	11.90	11.93
0.00	0.00	0.00