

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020515\
 Data File : BF077189.D
 Acq On : 5 Feb 2015 17:40
 Operator : TP/IZ
 Sample : G1215-03
 Misc : W/DOD
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DCW-RB02-2315

Quant Time: Feb 06 00:32:28 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 06 00:12:25 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	29060	20.00	ng	0.00
21) Naphthalene-d8	10.59	136	118711	20.00	ng	0.00
38) Acenaphthene-d10	14.71	164	65178	20.00	ng	-0.01
63) Phenanthrene-d10	17.56	188	112286	20.00	ng	0.00
75) Chrysene-d12	21.07	240	121059	20.00	ng	0.00
86) Perylene-d12	22.71	264	106358	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	4.70	112	56951	32.22	ng	0.01
7) Phenol-d6	7.10	99	38717	17.36	ng	0.02
23) Nitrobenzene-d5	8.99	82	135965	63.45	ng	0.00
41) 2,4,6-Tribromophenol	16.44	330	41938	79.27	ng	0.00
44) 2-Fluorobiphenyl	13.24	172	276804	64.63	ng	0.00
78) Terphenyl-d14	19.81	244	279214	53.10	ng	0.00


Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020515\
Data File : BF077189.D
Acq On : 5 Feb 2015 17:40
Operator : TP/IZ
Sample : G1215-03
Misc : W/DOD
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DCW-RB02-2315

Quant Time: Feb 06 00:32:28 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 06 00:12:25 2015
Response via : Initial Calibration

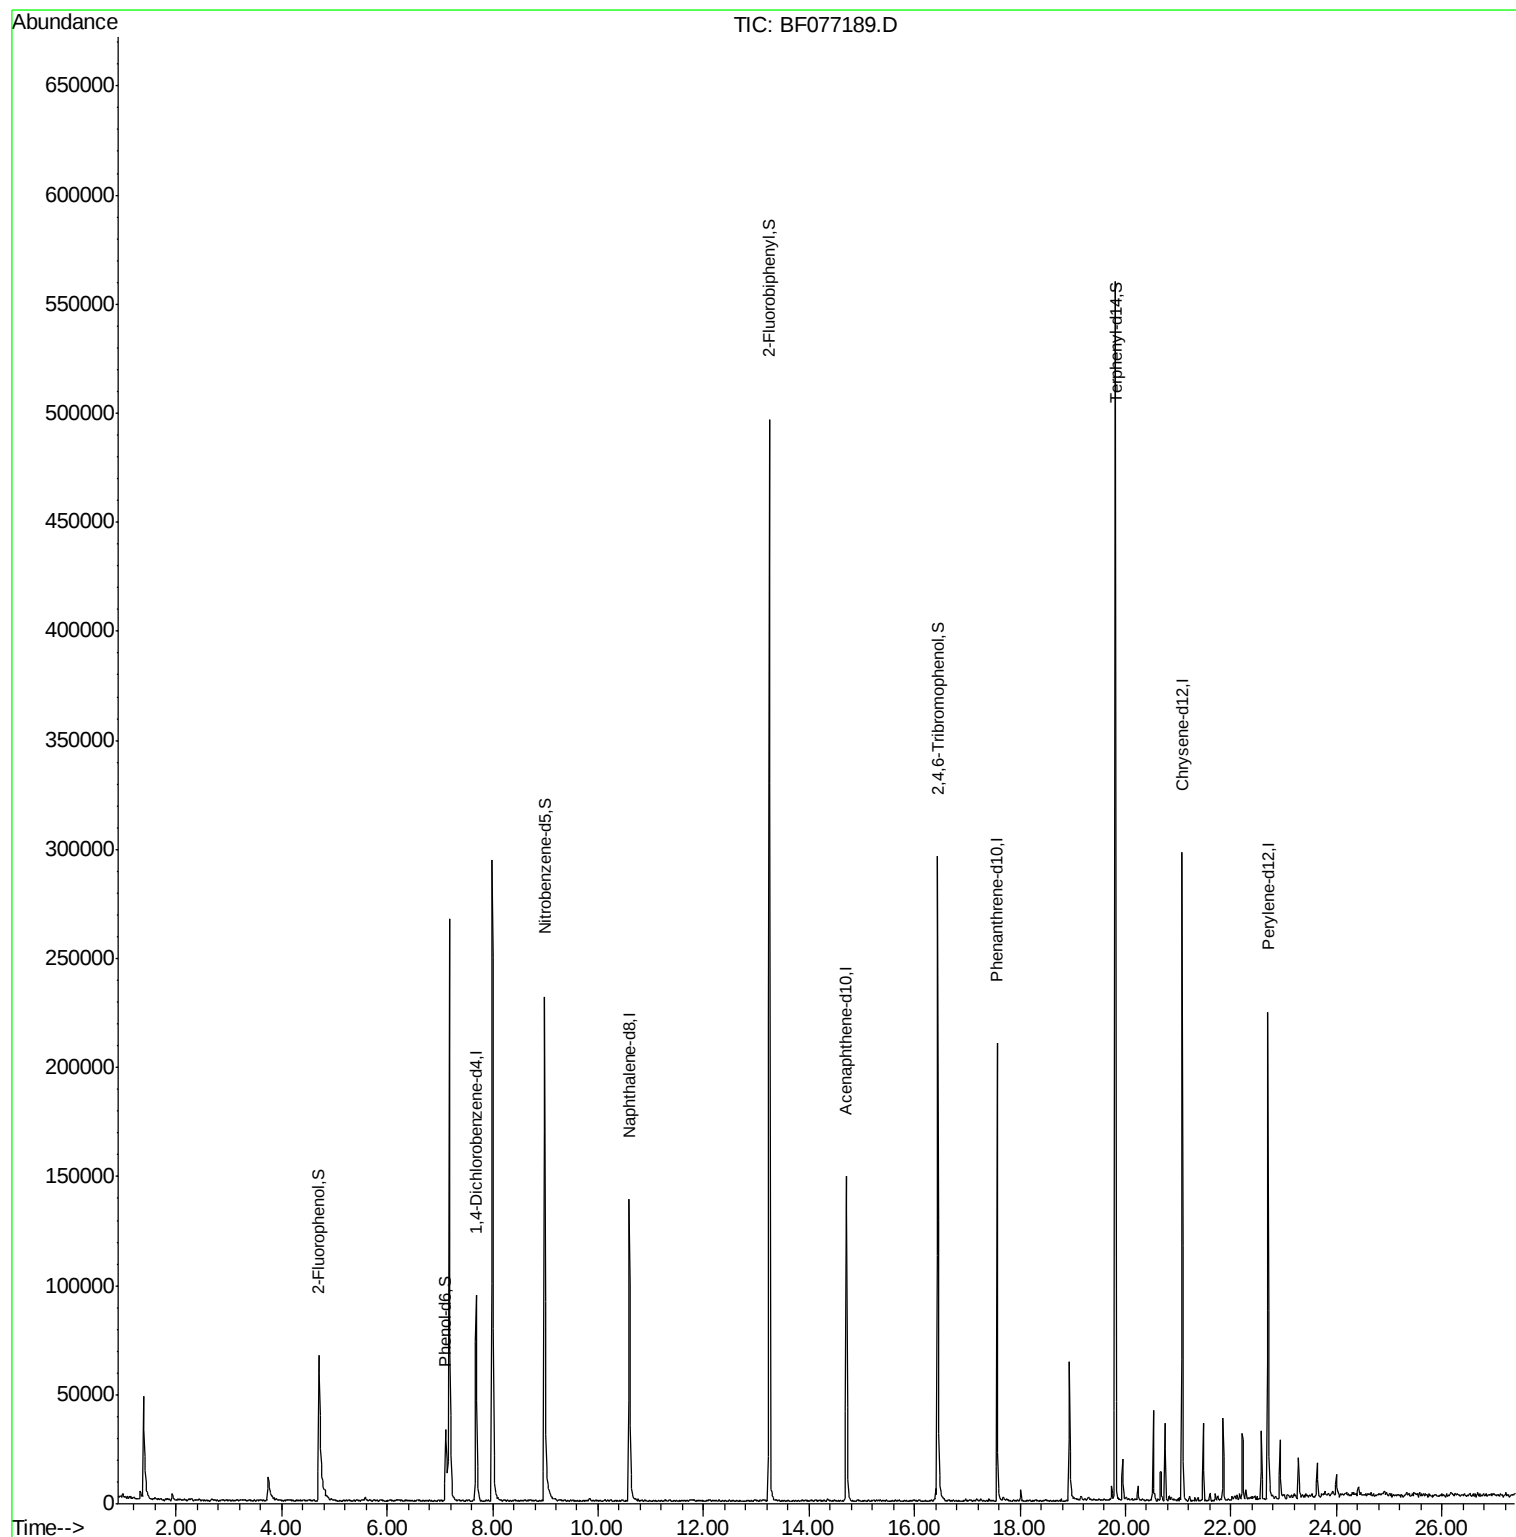



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 7.69 min Scan# 595

Delta R.T. -0.00 min

Lab File: BF077189.D

Acq: 5 Feb 2015 17:40

Instrument :

BNA_F

ClientSampleId :

DCW-RB02-2315


Tgt Ion:152 Resp: 29060

Ion Ratio Lower Upper

152 100

150 160.6 121.7 182.5



115 70.1 47.0 70.6



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

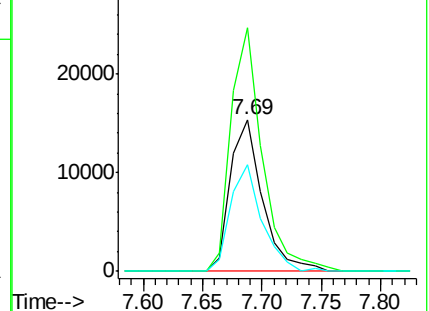

#5

2-Fluorophenol

Concen: 32.22 ng

RT: 4.70 min Scan# 334

Delta R.T. 0.01 min

Lab File: BF077189.D

Acq: 5 Feb 2015 17:40


Tgt Ion:112 Resp: 56951

Ion Ratio Lower Upper

112 100

64 69.7 54.2 81.4



63 40.6 28.4 42.6




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

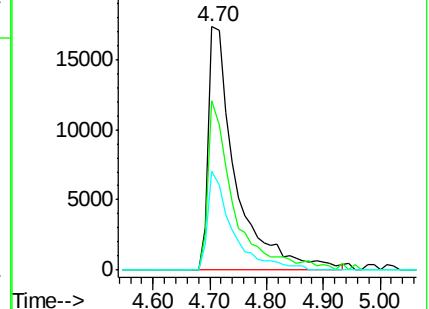

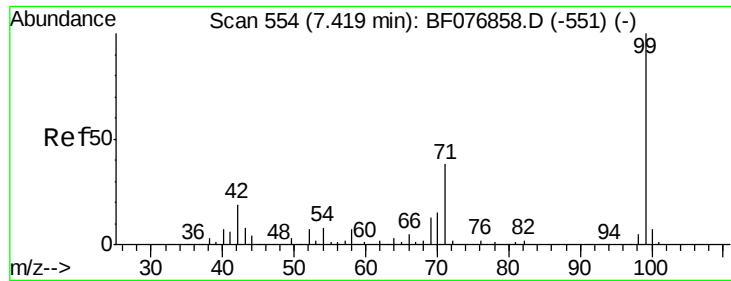

#7

Phenol-d6

Concen: 17.36 ng

RT: 7.10 min Scan# 544

Delta R.T. 0.02 min

Lab File: BF077189.D

Acq: 5 Feb 2015 17:40

Instrument :

BNA_F

ClientSampleId :

DCW-RB02-2315


Tgt Ion: 99 Resp: 38717

Ion Ratio Lower Upper

99 100

42 19.2 15.0 22.4




71 37.8 30.5 45.7

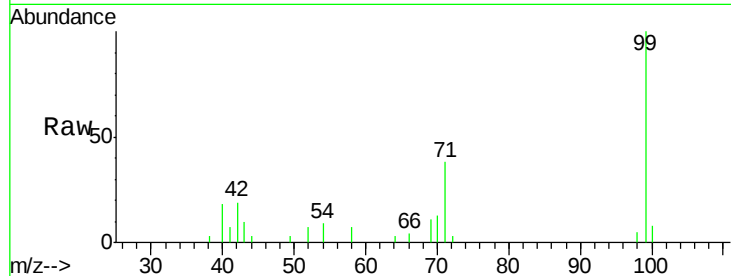

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

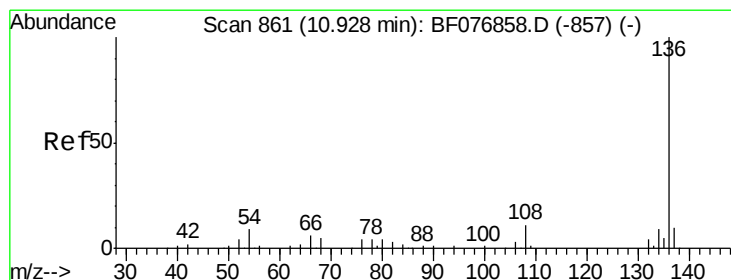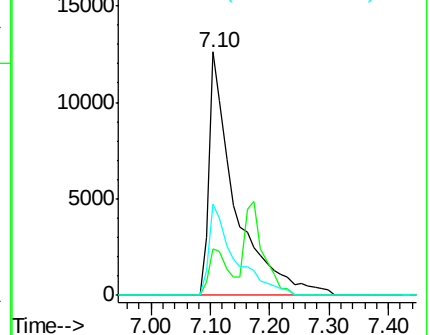

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.59 min Scan# 849

Delta R.T. -0.00 min

Lab File: BF077189.D

Acq: 5 Feb 2015 17:40

Tgt Ion: 136 Resp: 118711


Ion Ratio Lower Upper

136 100

137 11.4 8.1 12.1

54 9.1 7.0 10.4

68 4.5 3.7 5.5


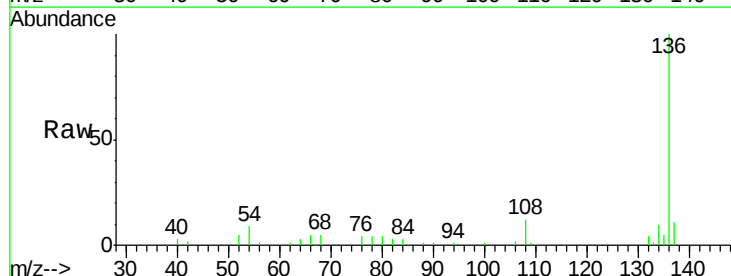


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



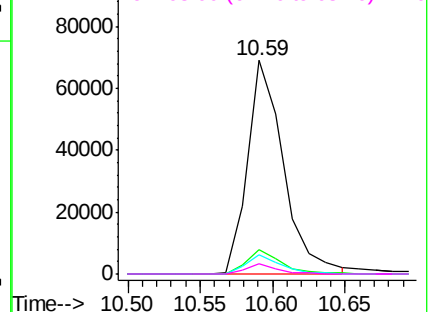




#23
 Nitrobenzene-d5
 Concen: 63.45 ng
 RT: 8.99 min Scan# 709
 Delta R.T. -0.00 min
 Lab File: BF077189.D
 Acq: 5 Feb 2015 17:40




Instrument :
 BNA_F
 ClientSampleId :
 DCW-RB02-2315

Tgt Ion: 82 Resp: 135965
 Ion Ratio Lower Upper
 82 100
 128 42.7 33.1 49.7
 54 55.1 48.3 72.5

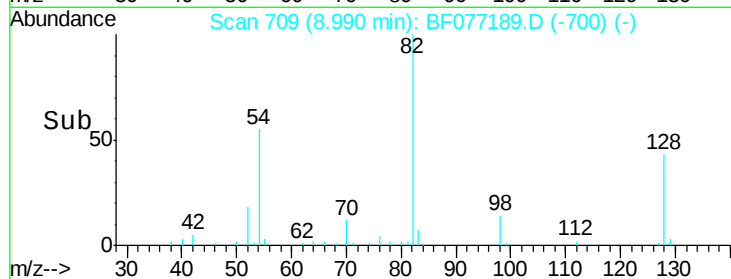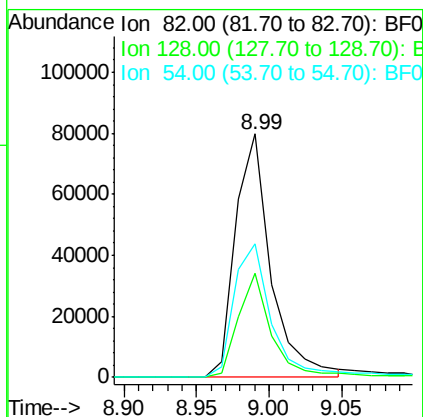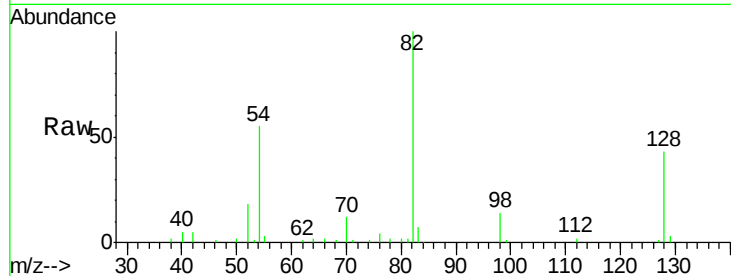

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.71 min Scan# 1209
 Delta R.T. -0.01 min
 Lab File: BF077189.D
 Acq: 5 Feb 2015 17:40

Tgt Ion: 164 Resp: 65178
 Ion Ratio Lower Upper
 164 100
 162 108.6 82.4 123.6
 160 45.5 34.8 52.2

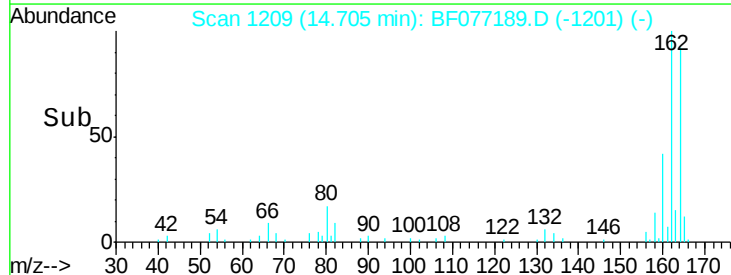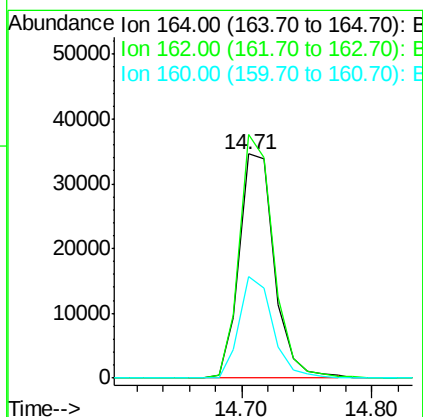



#41

2,4,6-Tribromophenol

Concen: 79.27 ng

RT: 16.44 min Scan# 1361

Delta R.T. -0.00 min

Lab File: BF077189.D

Acq: 5 Feb 2015 17:40

Instrument :

BNA_F

ClientSampleId :

DCW-RB02-2315


Tgt Ion:330 Resp: 41938

Ion Ratio Lower Upper

330 100

332 98.6 77.8 116.6




141 53.1 38.5 57.7



Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

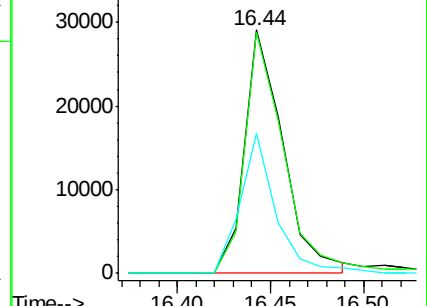

#44

2-Fluorobiphenyl

Concen: 64.63 ng

RT: 13.24 min Scan# 1081

Delta R.T. -0.00 min

Lab File: BF077189.D

Acq: 5 Feb 2015 17:40


Tgt Ion:172 Resp: 276804

Ion Ratio Lower Upper

172 100

171 34.5 26.6 40.0



170 23.5 18.0 27.0




Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

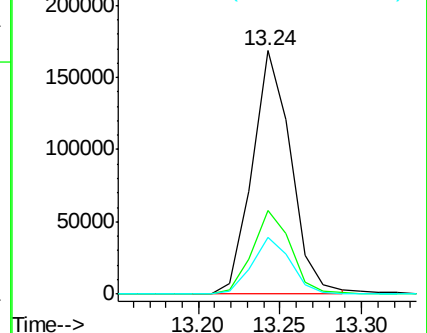






#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.56 min Scan# 1459
Delta R.T. -0.00 min
Lab File: BF077189.D
Acq: 5 Feb 2015 17:40

Instrument :
BNA_F
ClientSampleId :
DCW-RB02-2315

Tgt Ion:188 Resp: 112286
Ion Ratio Lower Upper
188 100
94 9.8 6.0 9.0#
80 9.8 6.9 10.3

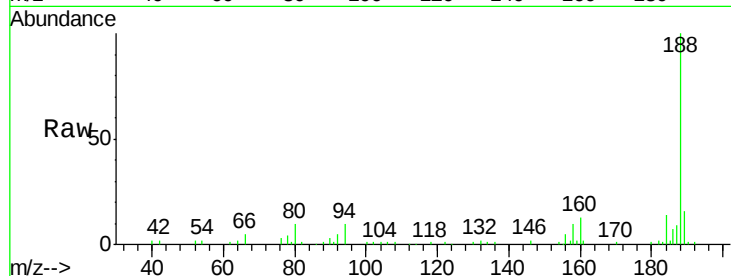


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0


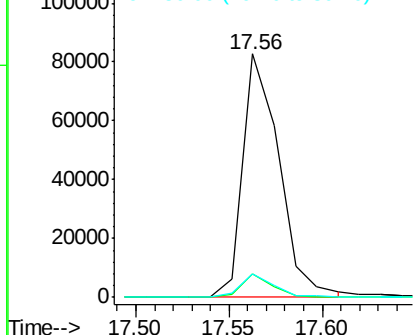


#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.07 min Scan# 1766
Delta R.T. -0.00 min
Lab File: BF077189.D
Acq: 5 Feb 2015 17:40

Tgt Ion:240 Resp: 121059
Ion Ratio Lower Upper
240 100
120 9.5 10.4 15.6#
236 24.7 20.2 30.2



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

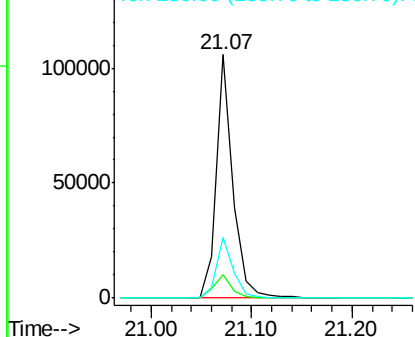







#78
 Terphenyl-d14
 Concen: 53.10 ng
 RT: 19.81 min Scan# 1656
 Delta R.T. -0.00 min
 Lab File: BF077189.D
 Acq: 5 Feb 2015 17:40

Instrument :
 BNA_F
 ClientSampleId :
 DCW-RB02-2315

Tgt Ion: 244 Resp: 279214
 Ion Ratio Lower Upper
 244 100
 212 7.0 6.3 9.5
 122 7.8 10.1 15.1#




Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

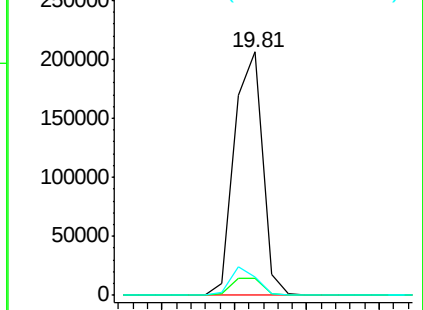

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 22.71 min Scan# 1909
 Delta R.T. -0.05 min
 Lab File: BF077189.D
 Acq: 5 Feb 2015 17:40

Tgt Ion: 264 Resp: 106358
 Ion Ratio Lower Upper
 264 100
 260 23.9 19.0 28.4
 265 21.7 18.1 27.1



Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

