

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020515\
 Data File : BF077192.D
 Acq On : 5 Feb 2015 19:23
 Operator : TP/IZ
 Sample : G1212-01
 Misc : S
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FK-BPM-01-A1A-A2A-A3A-A4A

Quant Time: Feb 06 01:00:28 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 06 00:49:29 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	31706	20.00	ng	0.00
21) Naphthalene-d8	10.59	136	125796	20.00	ng	0.00
38) Acenaphthene-d10	14.71	164	70803	20.00	ng	-0.01
63) Phenanthrene-d10	17.56	188	114192	20.00	ng	0.00
75) Chrysene-d12	21.07	240	116985	20.00	ng	0.00
86) Perylene-d12	22.72	264	107962	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	4.70	112	147786	76.64	ng	0.01
7) Phenol-d6	7.08	99	184102	75.68	ng	-0.01
23) Nitrobenzene-d5	8.99	82	106200	46.77	ng	0.00
41) 2,4,6-Tribromophenol	16.44	330	36328	63.21	ng	0.00
44) 2-Fluorobiphenyl	13.24	172	213578	45.91	ng	0.00
78) Terphenyl-d14	19.81	244	226303	44.53	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020515\
Data File : BF077192.D
Acq On : 5 Feb 2015 19:23
Operator : TP/IZ
Sample : G1212-01
Misc : S
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-BPM-01-A1A-A2A-A3A-A4A

Quant Time: Feb 06 01:00:28 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 06 00:49:29 2015
Response via : Initial Calibration

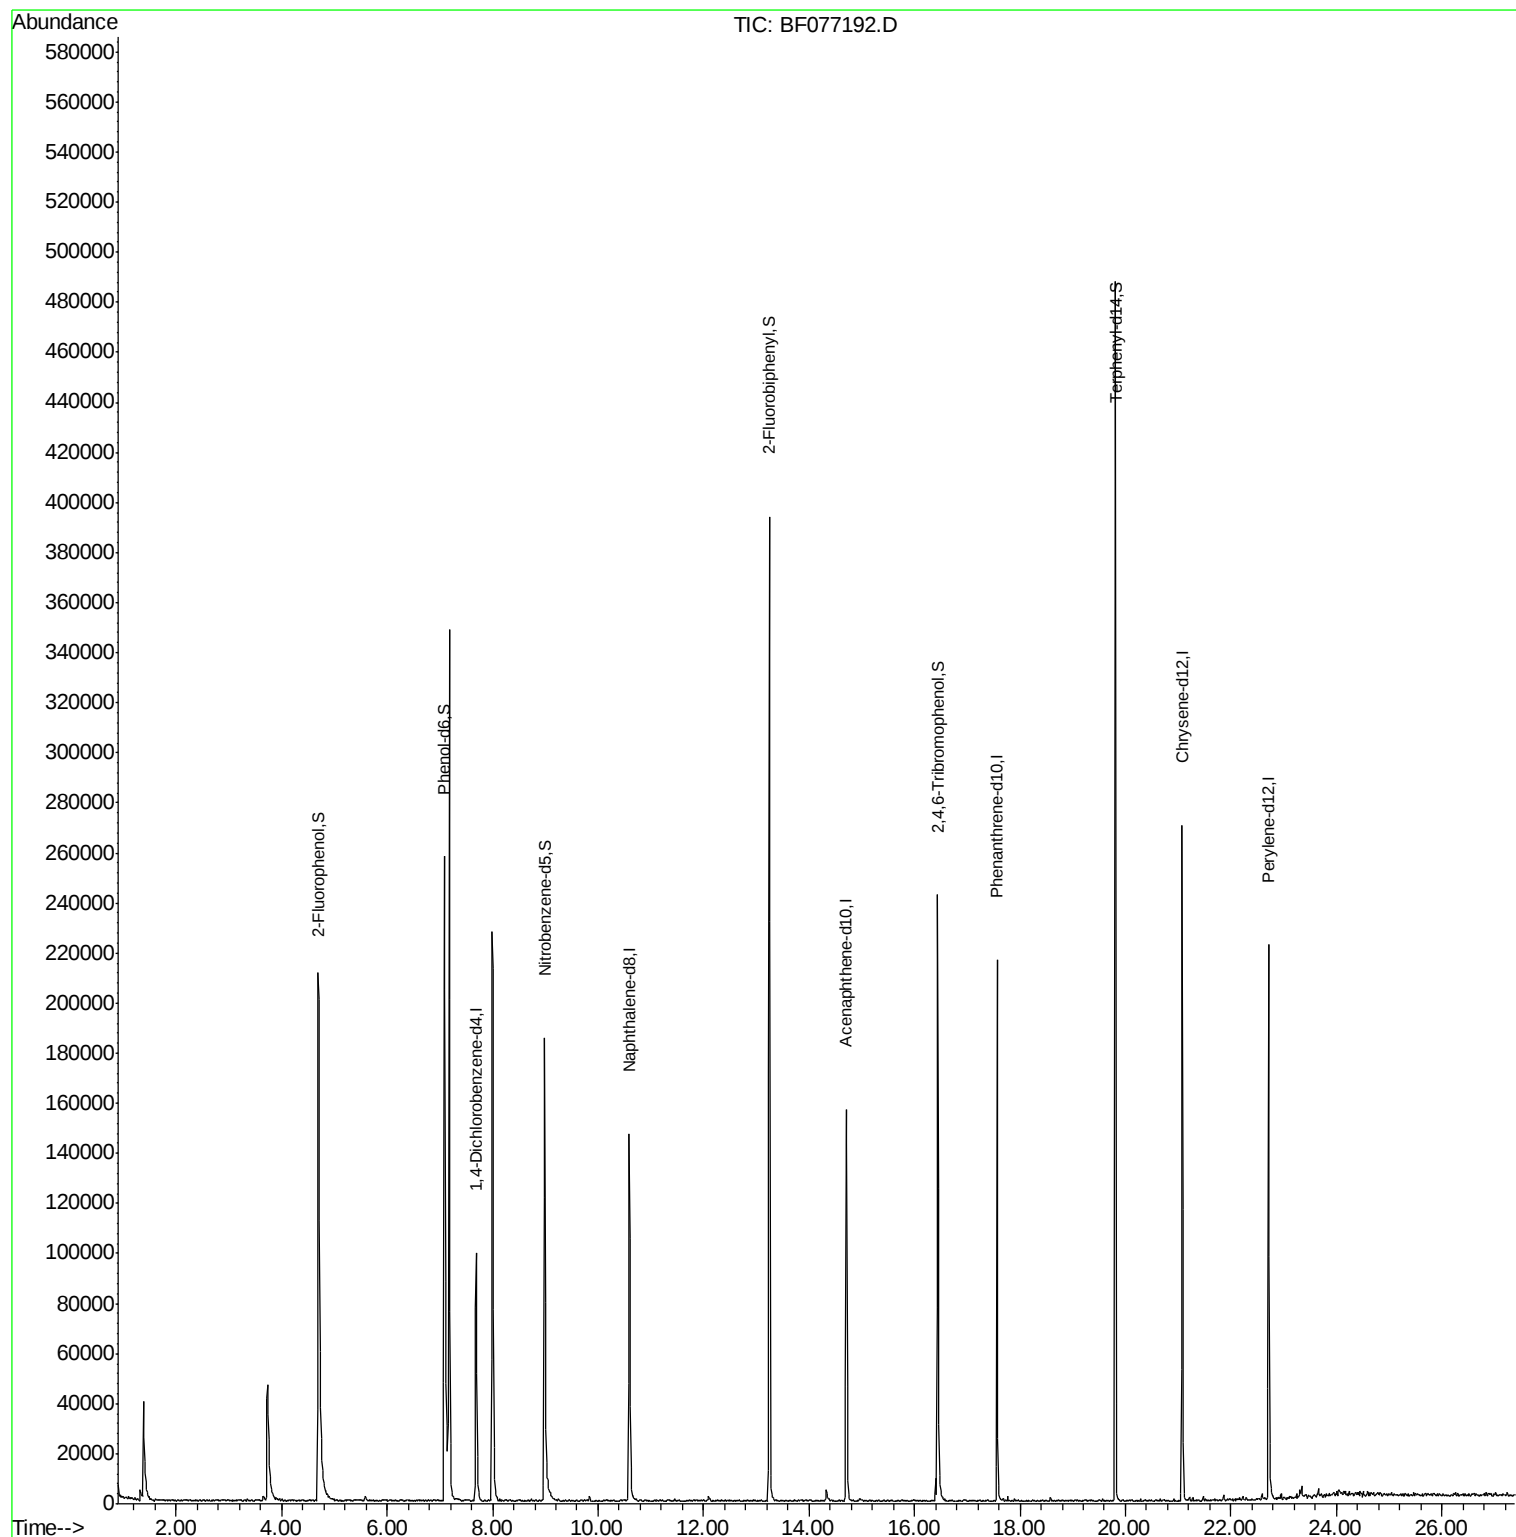

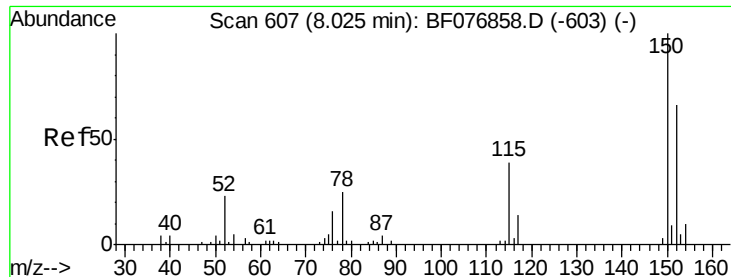

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 7.69 min Scan# 595

Delta R.T. -0.00 min

Lab File: BF077192.D

Acq: 5 Feb 2015 19:23

Instrument :

BNA_F

ClientSampleId :

FK-BPM-01-A1A-A2A-A3A-A4A


Tgt Ion:152 Resp: 31706

Ion Ratio Lower Upper

152 100

150 150.6 121.7 182.5




115 59.7 47.0 70.6



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

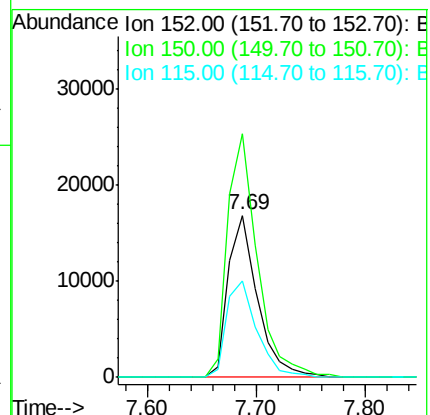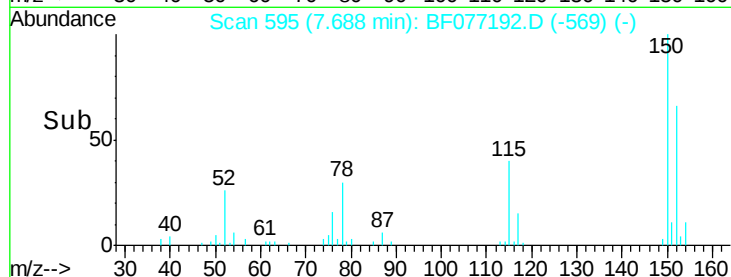

#5

2-Fluorophenol

Concen: 76.64 ng

RT: 4.70 min Scan# 334

Delta R.T. 0.01 min

Lab File: BF077192.D

Acq: 5 Feb 2015 19:23


Tgt Ion:112 Resp: 147786

Ion Ratio Lower Upper

112 100

64 63.7 54.2 81.4



63 34.1 28.4 42.6




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

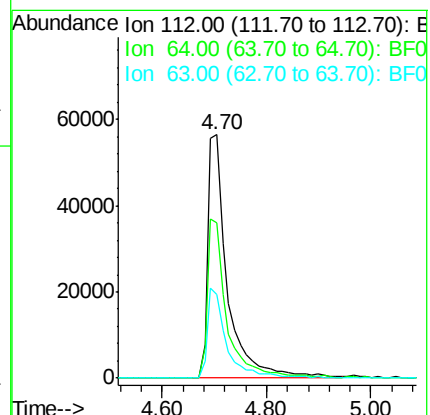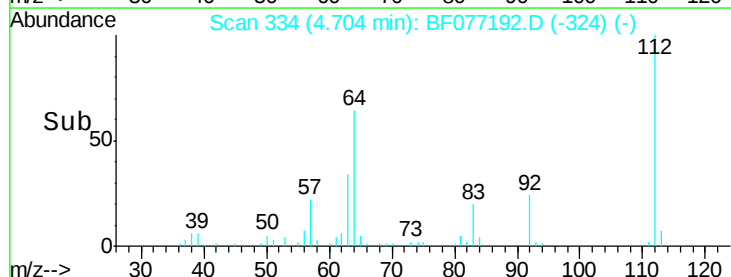

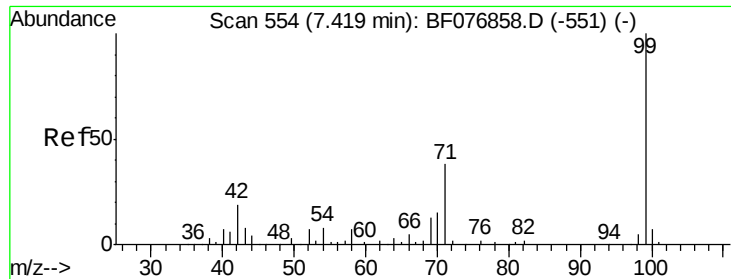

#7

Phenol-d6

Concen: 75.68 ng

RT: 7.08 min Scan# 542

Delta R.T. -0.01 min

Lab File: BF077192.D

Acq: 5 Feb 2015 19:23

Instrument :

BNA_F

ClientSampleId :

FK-BPM-01-A1A-A2A-A3A-A4A


Tgt Ion: 99 Resp: 184102

Ion Ratio Lower Upper

99 100

42 18.8 15.0 22.4




71 38.7 30.5 45.7



Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

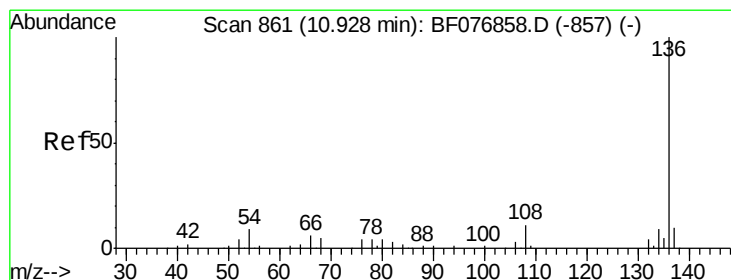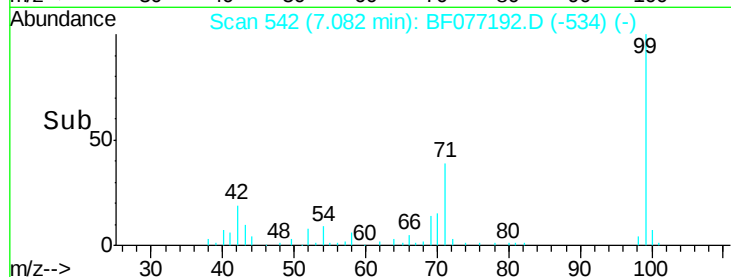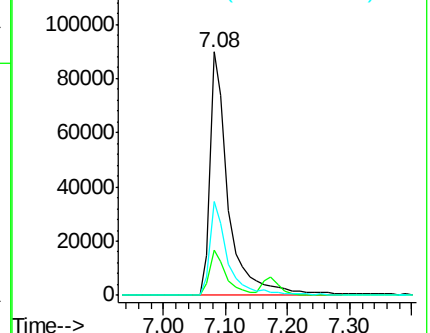

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.59 min Scan# 849

Delta R.T. -0.00 min

Lab File: BF077192.D

Acq: 5 Feb 2015 19:23

Tgt Ion: 136 Resp: 125796


Ion Ratio Lower Upper

136 100

137 10.6 8.1 12.1

54 8.9 7.0 10.4

68 4.2 3.7 5.5






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



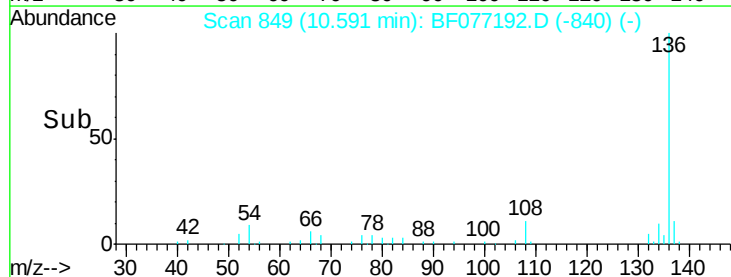
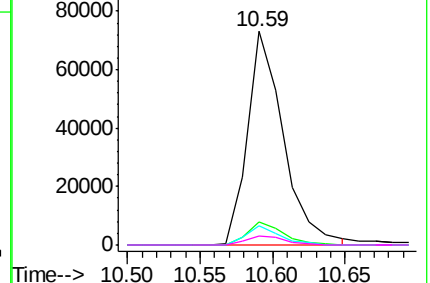


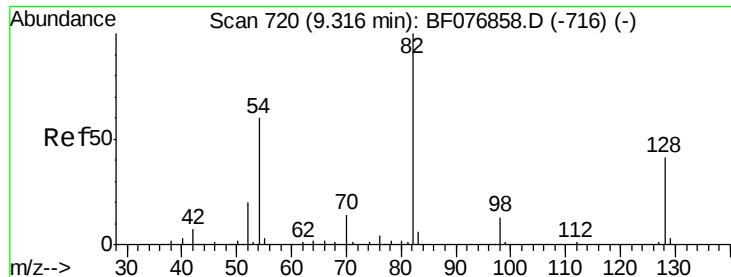

#23
 Nitrobenzene-d5
 Concen: 46.77 ng
 RT: 8.99 min Scan# 709
 Delta R.T. -0.00 min
 Lab File: BF077192.D
 Acq: 5 Feb 2015 19:23




Instrument :
 BNA_F
 ClientSampleId :
 FK-BPM-01-A1A-A2A-A3A-A4A


Tgt Ion: 82 Resp: 106200
 Ion Ratio Lower Upper
 82 100
 128 38.7 33.1 49.7
 54 55.9 48.3 72.5

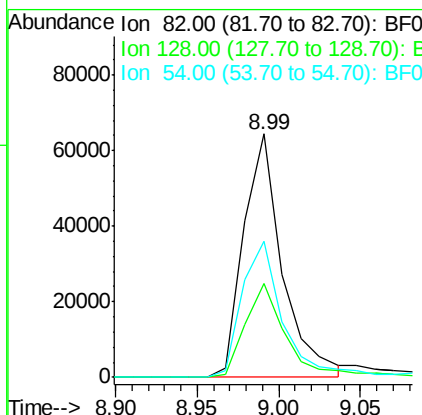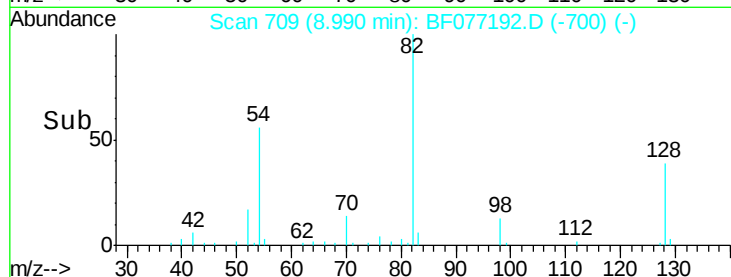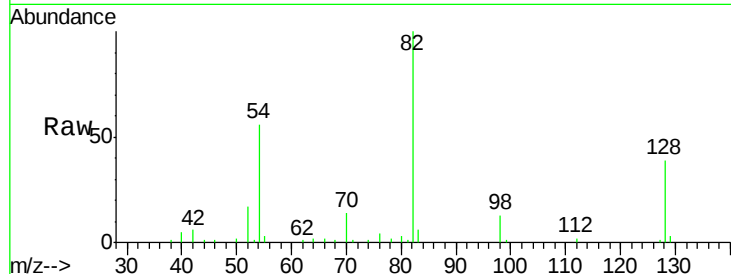

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.71 min Scan# 1209
 Delta R.T. -0.01 min
 Lab File: BF077192.D
 Acq: 5 Feb 2015 19:23

Tgt Ion: 164 Resp: 70803
 Ion Ratio Lower Upper
 164 100
 162 96.0 82.4 123.6
 160 41.5 34.8 52.2


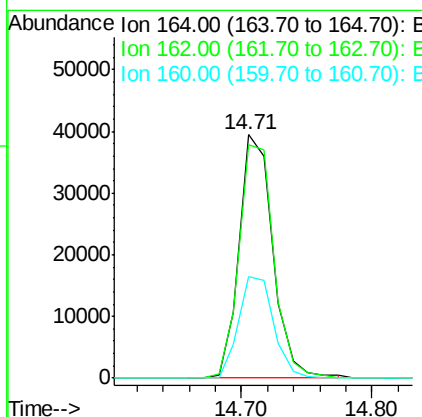
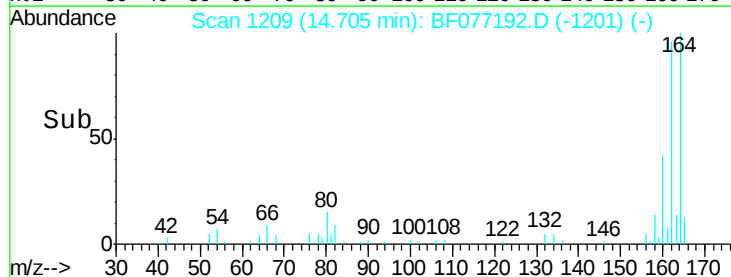



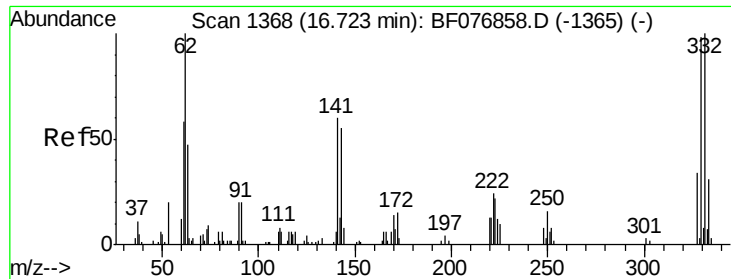

#41
 2,4,6-Tribromophenol
 Concen: 63.21 ng
 RT: 16.44 min Scan# 1361
 Delta R.T. -0.00 min
 Lab File: BF077192.D
 Acq: 5 Feb 2015 19:23




Instrument :
 BNA_F
 ClientSampleId :
 FK-BPM-01-A1A-A2A-A3A-A4A


Tgt Ion:330 Resp: 36328
 Ion Ratio Lower Upper
 330 100
 332 98.7 77.8 116.6
 141 52.8 38.5 57.7

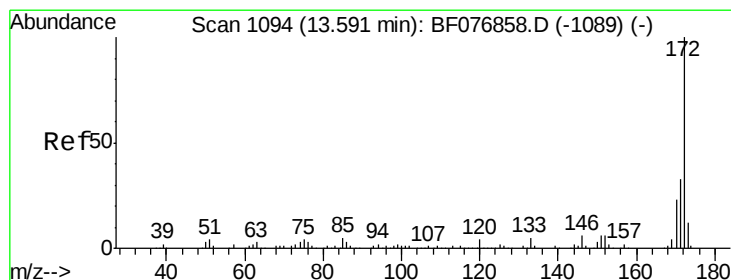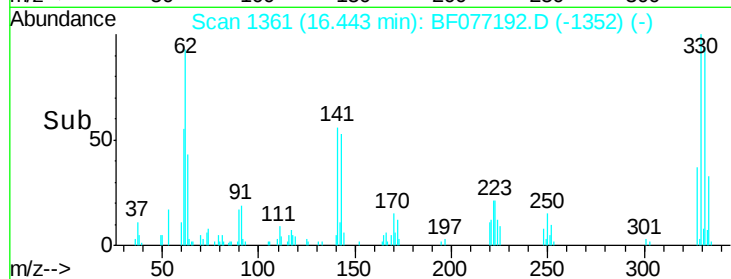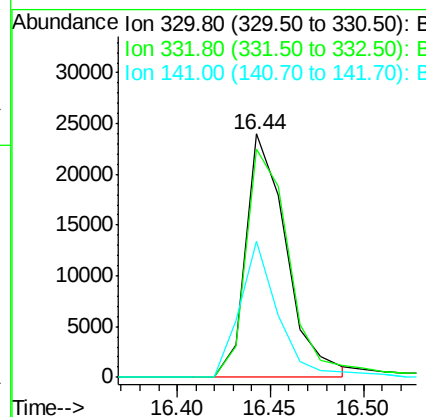

#44
 2-Fluorobiphenyl
 Concen: 45.91 ng
 RT: 13.24 min Scan# 1081
 Delta R.T. -0.00 min
 Lab File: BF077192.D
 Acq: 5 Feb 2015 19:23

Tgt Ion:172 Resp: 213578
 Ion Ratio Lower Upper
 172 100
 171 35.0 26.6 40.0
 170 23.5 18.0 27.0


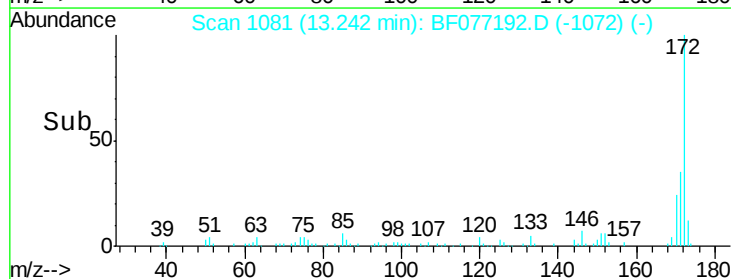
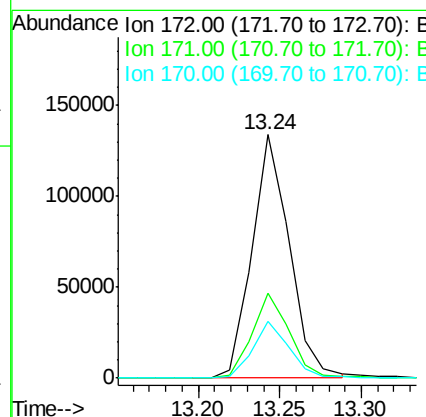
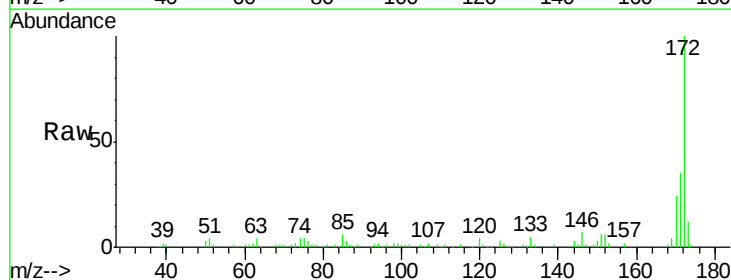


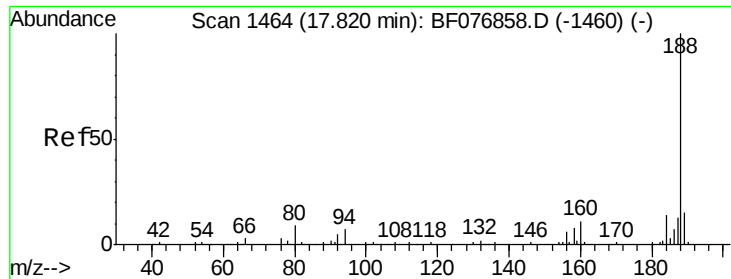

#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 17.56 min Scan# 1459
 Delta R.T. -0.00 min
 Lab File: BF077192.D
 Acq: 5 Feb 2015 19:23




Instrument :
 BNA_F
 ClientSampleId :
 FK-BPM-01-A1A-A2A-A3A-A4A


Tgt Ion:188 Resp: 114192
 Ion Ratio Lower Upper
 188 100
 94 10.6 6.0 9.0#
 80 10.8 6.9 10.3#

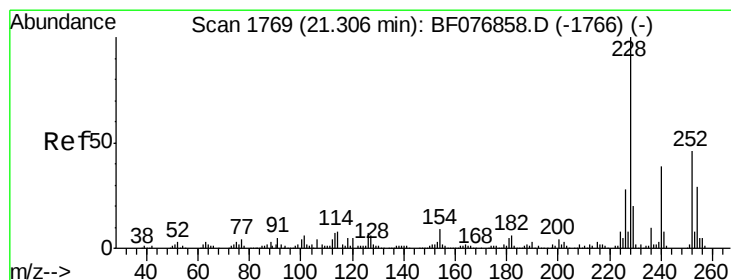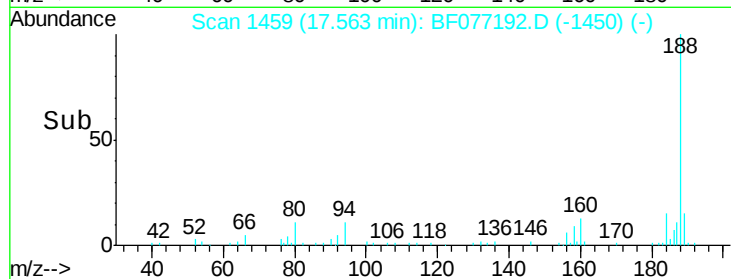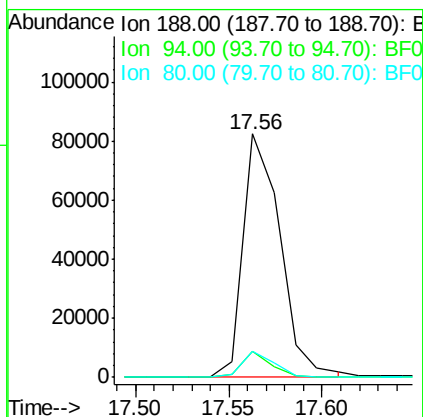

#75
 Chrysene-d12
 Concen: 20.00 ng
 RT: 21.07 min Scan# 1766
 Delta R.T. -0.00 min
 Lab File: BF077192.D
 Acq: 5 Feb 2015 19:23

Tgt Ion:240 Resp: 116985
 Ion Ratio Lower Upper
 240 100
 120 10.8 10.4 15.6
 236 24.1 20.2 30.2


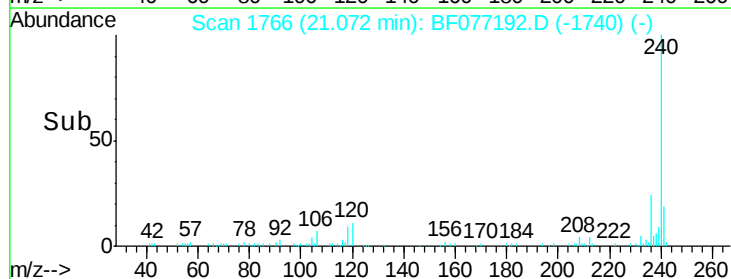
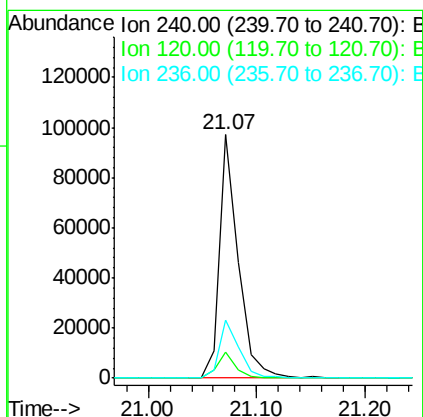
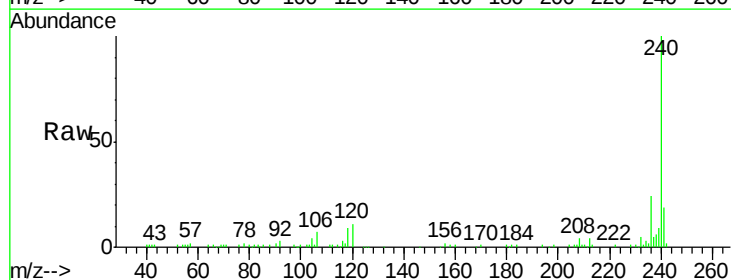


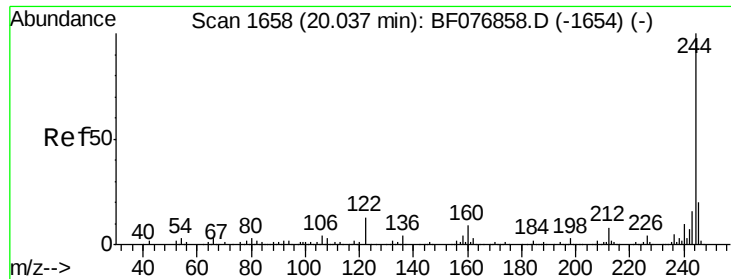

#78
 Terphenyl-d14
 Concen: 44.53 ng
 RT: 19.81 min Scan# 1656
 Delta R.T. -0.00 min
 Lab File: BF077192.D
 Acq: 5 Feb 2015 19:23

Instrument :
 BNA_F
 ClientSampleId :
 FK-BPM-01-A1A-A2A-A3A-A4A

Tgt Ion	Ratio	Lower	Upper
244	100		
212	6.9	6.3	9.5
122	9.3	10.1	15.1#

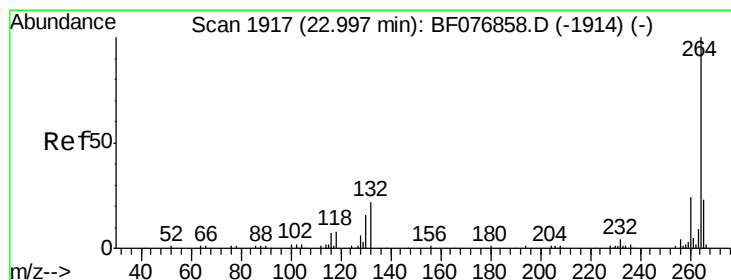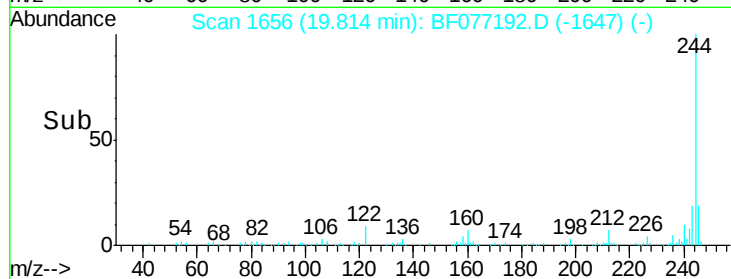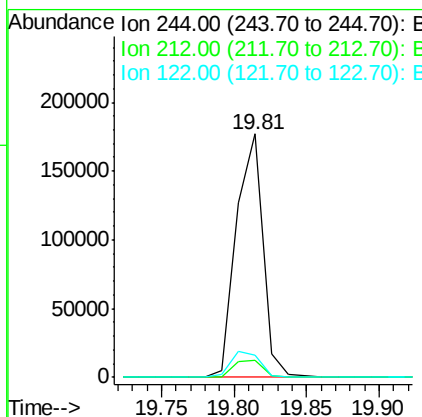

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 22.72 min Scan# 1910
 Delta R.T. -0.03 min
 Lab File: BF077192.D
 Acq: 5 Feb 2015 19:23

Tgt Ion	Ratio	Lower	Upper
264	100		
260	23.7	19.0	28.4
265	21.1	18.1	27.1

