

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020515\
 Data File : BF077188.D
 Acq On : 5 Feb 2015 17:06
 Operator : TP/IZ
 Sample : G1215-02
 Misc : W/DOD
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DCW-WW-056-2315

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.378	41	43	53	rVB	41979	74712	6.81%	1.195%
2	3.744	247	250	261	rBV	15597	47620	4.34%	0.762%
3	4.704	332	334	348	rBV	85976	223811	20.41%	3.581%
4	7.105	541	544	547	rBV	43483	95445	8.71%	1.527%
5	7.173	547	550	559	rVB	302092	594942	54.27%	9.518%
6	7.687	592	595	603	rBV	98462	179202	16.35%	2.867%
7	7.996	619	622	635	rBV	344612	599238	54.66%	9.587%
8	8.990	706	709	721	rBV	266278	449325	40.98%	7.188%
9	10.591	846	849	860	rBV	150654	246365	22.47%	3.941%
10	13.242	1078	1081	1087	rBV	597098	943083	86.02%	15.087%
11	14.328	1174	1176	1182	rBV	6708	13004	1.19%	0.208%
12	14.705	1206	1209	1217	rVB	154424	280187	25.56%	4.482%
13	16.443	1359	1361	1372	rVB	327508	474298	43.26%	7.588%
14	17.563	1457	1459	1464	rBV	215487	290183	26.47%	4.642%
15	19.814	1653	1656	1658	rBV	883423	1096327	100.00%	17.539%
16	21.072	1763	1766	1773	rBV	291632	355440	32.42%	5.686%
17	22.718	1907	1910	1918	rBV	221707	287613	26.23%	4.601%


Sum of corrected areas: 6250795

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020515\
Data File : BF077188.D
Acq On : 5 Feb 2015 17:06
Operator : TP/IZ
Sample : G1215-02
Misc : W/DOD
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DCW-WW-056-2315

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

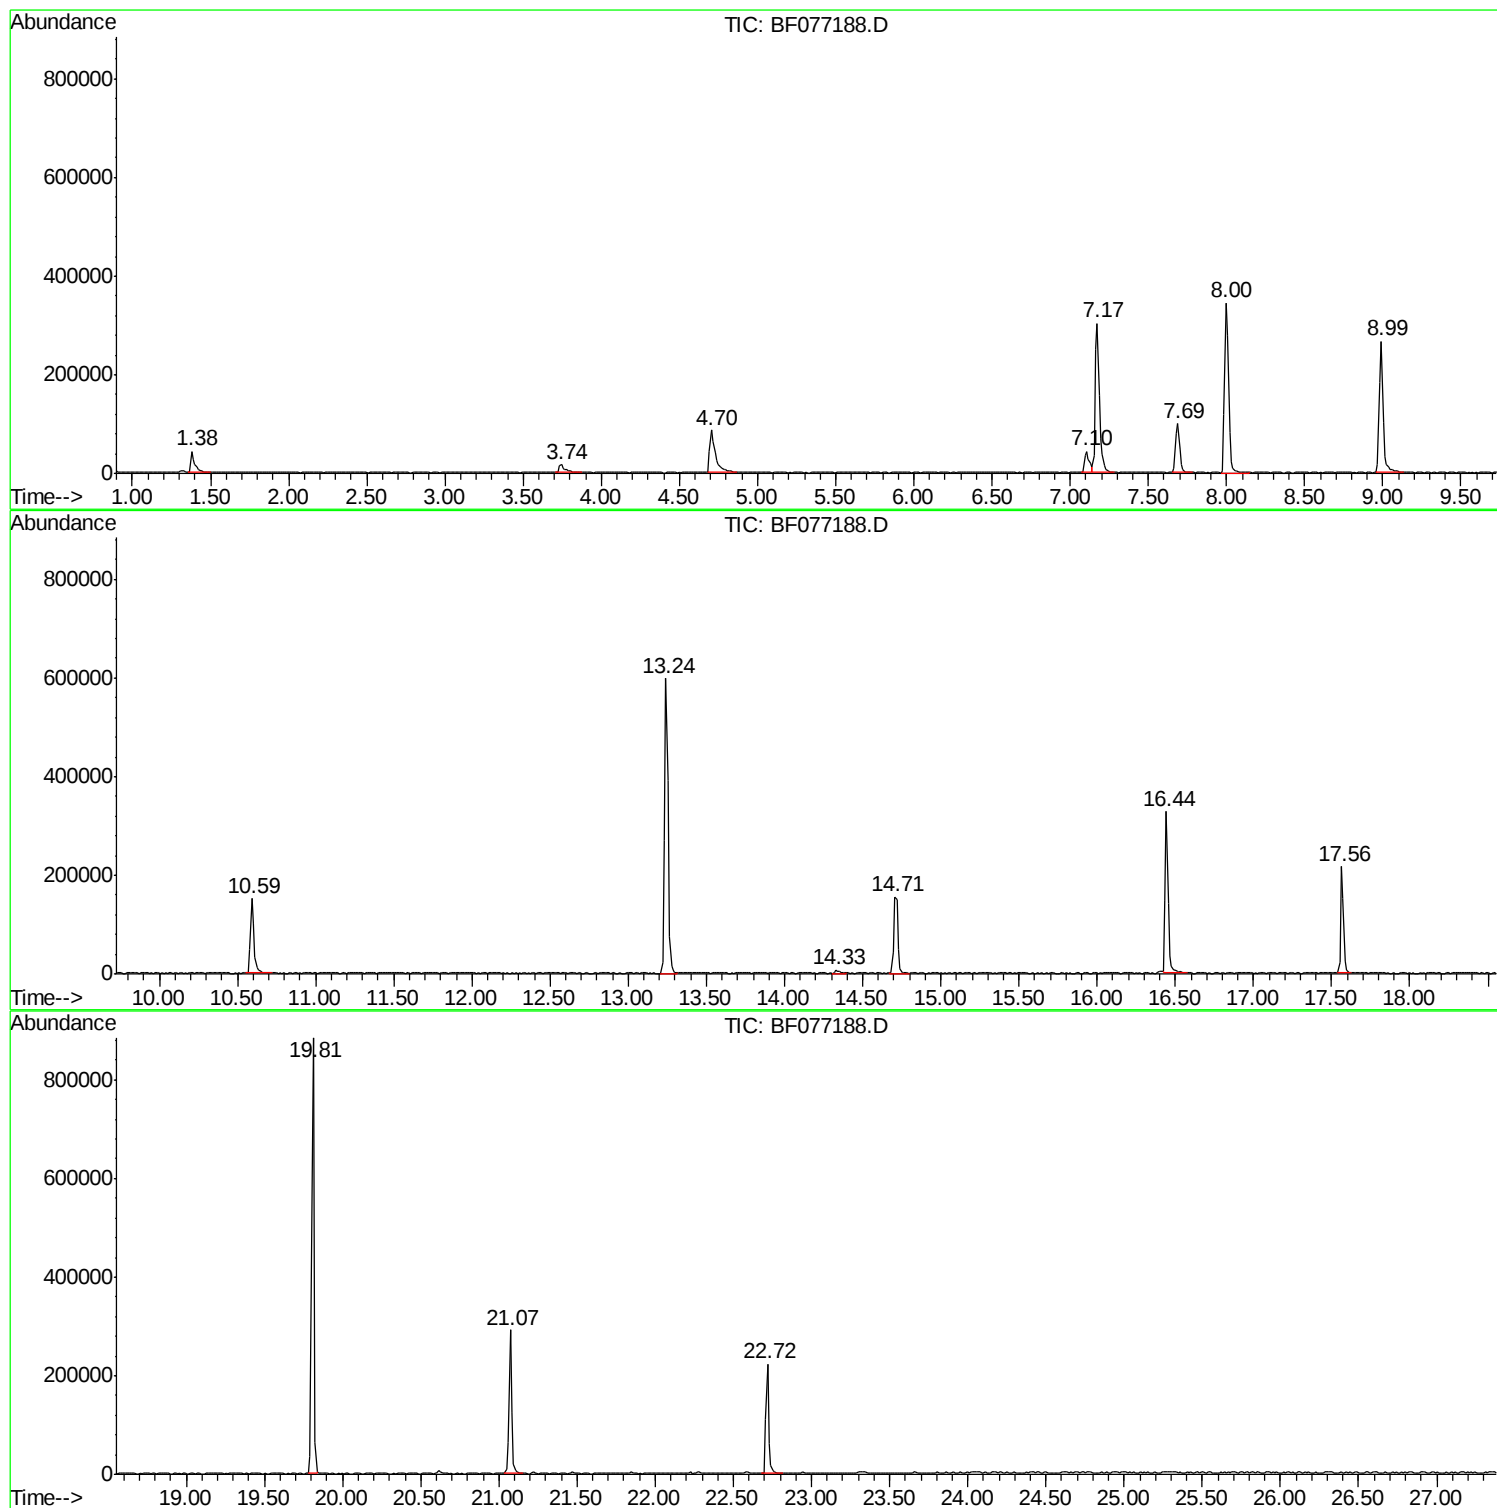

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020515\
Data File : BF077188.D
Acq On : 5 Feb 2015 17:06
Operator : TP/IZ
Sample : G1215-02
Misc : W/DOD
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DCW-WW-056-2315










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 unknown7.17 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.17	66.40 ng	594942	1,4-Dichlorobenzene-d4	7.69

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	17
3		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
4		5-Aminoindole	132	C8H8N2	005192-03-0	12
5		(5-METHYL-2-PYRIDYL)ACETONITRILE	132	C8H8N2	1000241-93-9	10

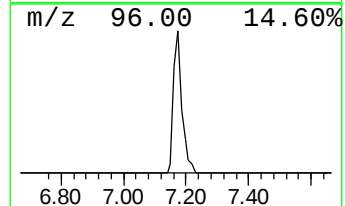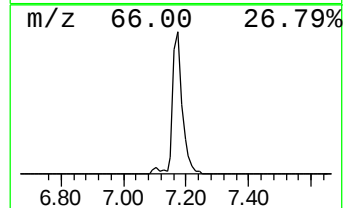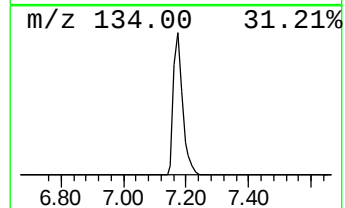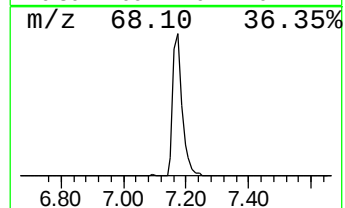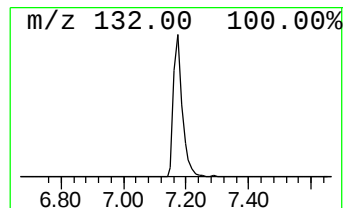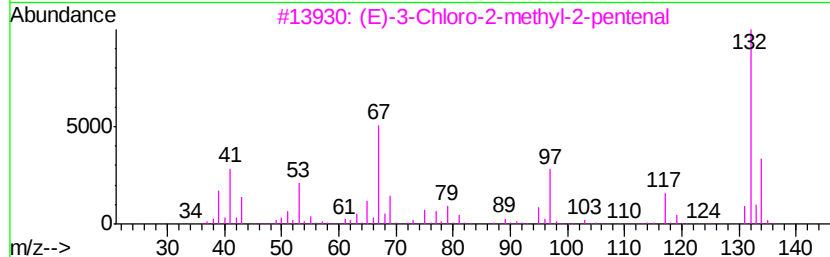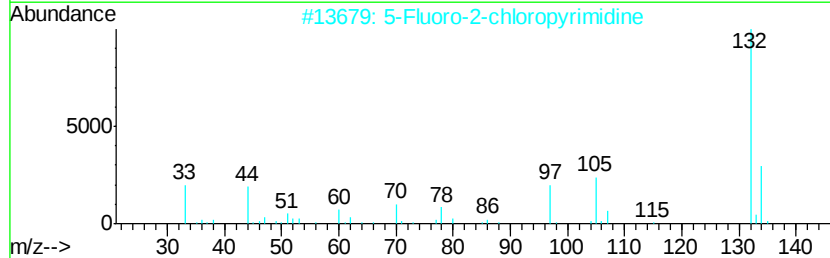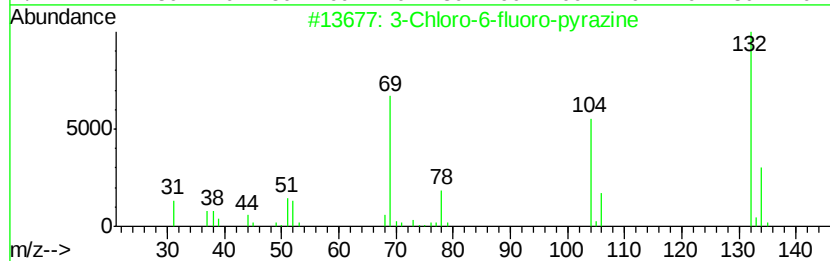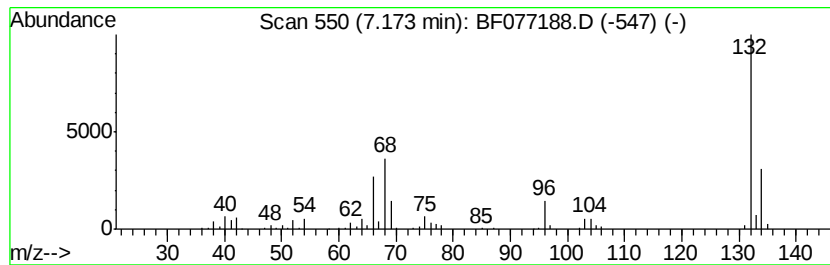

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020515\
Data File : BF077188.D
Acq On : 5 Feb 2015 17:06
Operator : TP/IZ
Sample : G1215-02
Misc : W/DOD
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DCW-WW-056-2315

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.17	7.17	66.4	ng	594942	1	7.69	179202	20.0