

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020515\
 Data File : BF077192.D
 Acq On : 5 Feb 2015 19:23
 Operator : TP/IZ
 Sample : G1212-01
 Misc : S
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FK-BPM-01-A1A-A2A-A3A-A4A

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	36	37	41	rBV	4253	10773	1.65%	0.186%
2	1.378	41	43	54	rVB	39199	76851	11.79%	1.329%
3	3.733	246	249	262	rBV	46237	130935	20.08%	2.264%
4	4.693	331	333	347	rBV	211055	512096	78.53%	8.855%
5	7.082	540	542	547	rBV	257591	475769	72.96%	8.226%
6	7.173	547	550	556	rVB	346906	616114	94.49%	10.653%
7	7.688	592	595	602	rVB	98668	178850	27.43%	3.092%
8	7.996	619	622	633	rVB	227635	421537	64.65%	7.289%
9	8.990	706	709	726	rBV	184634	325097	49.86%	5.621%
10	10.591	846	849	860	rBV	146126	244673	37.52%	4.231%
11	13.242	1078	1081	1090	rBV	393186	601546	92.25%	10.401%
12	14.328	1172	1176	1182	rVB2	4796	9782	1.50%	0.169%
13	14.705	1206	1209	1216	rBV	156740	279609	42.88%	4.835%
14	16.397	1355	1357	1359	rBV	9198	14229	2.18%	0.246%
15	16.443	1359	1361	1370	rVB	241859	341708	52.40%	5.908%
16	17.563	1457	1459	1464	rBV	215893	281033	43.10%	4.859%
17	19.814	1653	1656	1658	rBV	486725	652074	100.00%	11.275%
18	21.072	1763	1766	1772	rBV	270188	328746	50.42%	5.684%
19	22.718	1908	1910	1919	rBV	221287	274947	42.16%	4.754%
20	24.043	2024	2026	2030	rBV2	2549	7075	1.08%	0.122%


Sum of corrected areas: 5783444

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020515\
Data File : BF077192.D
Acq On : 5 Feb 2015 19:23
Operator : TP/IZ
Sample : G1212-01
Misc : S
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-BPM-01-A1A-A2A-A3A-A4A

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

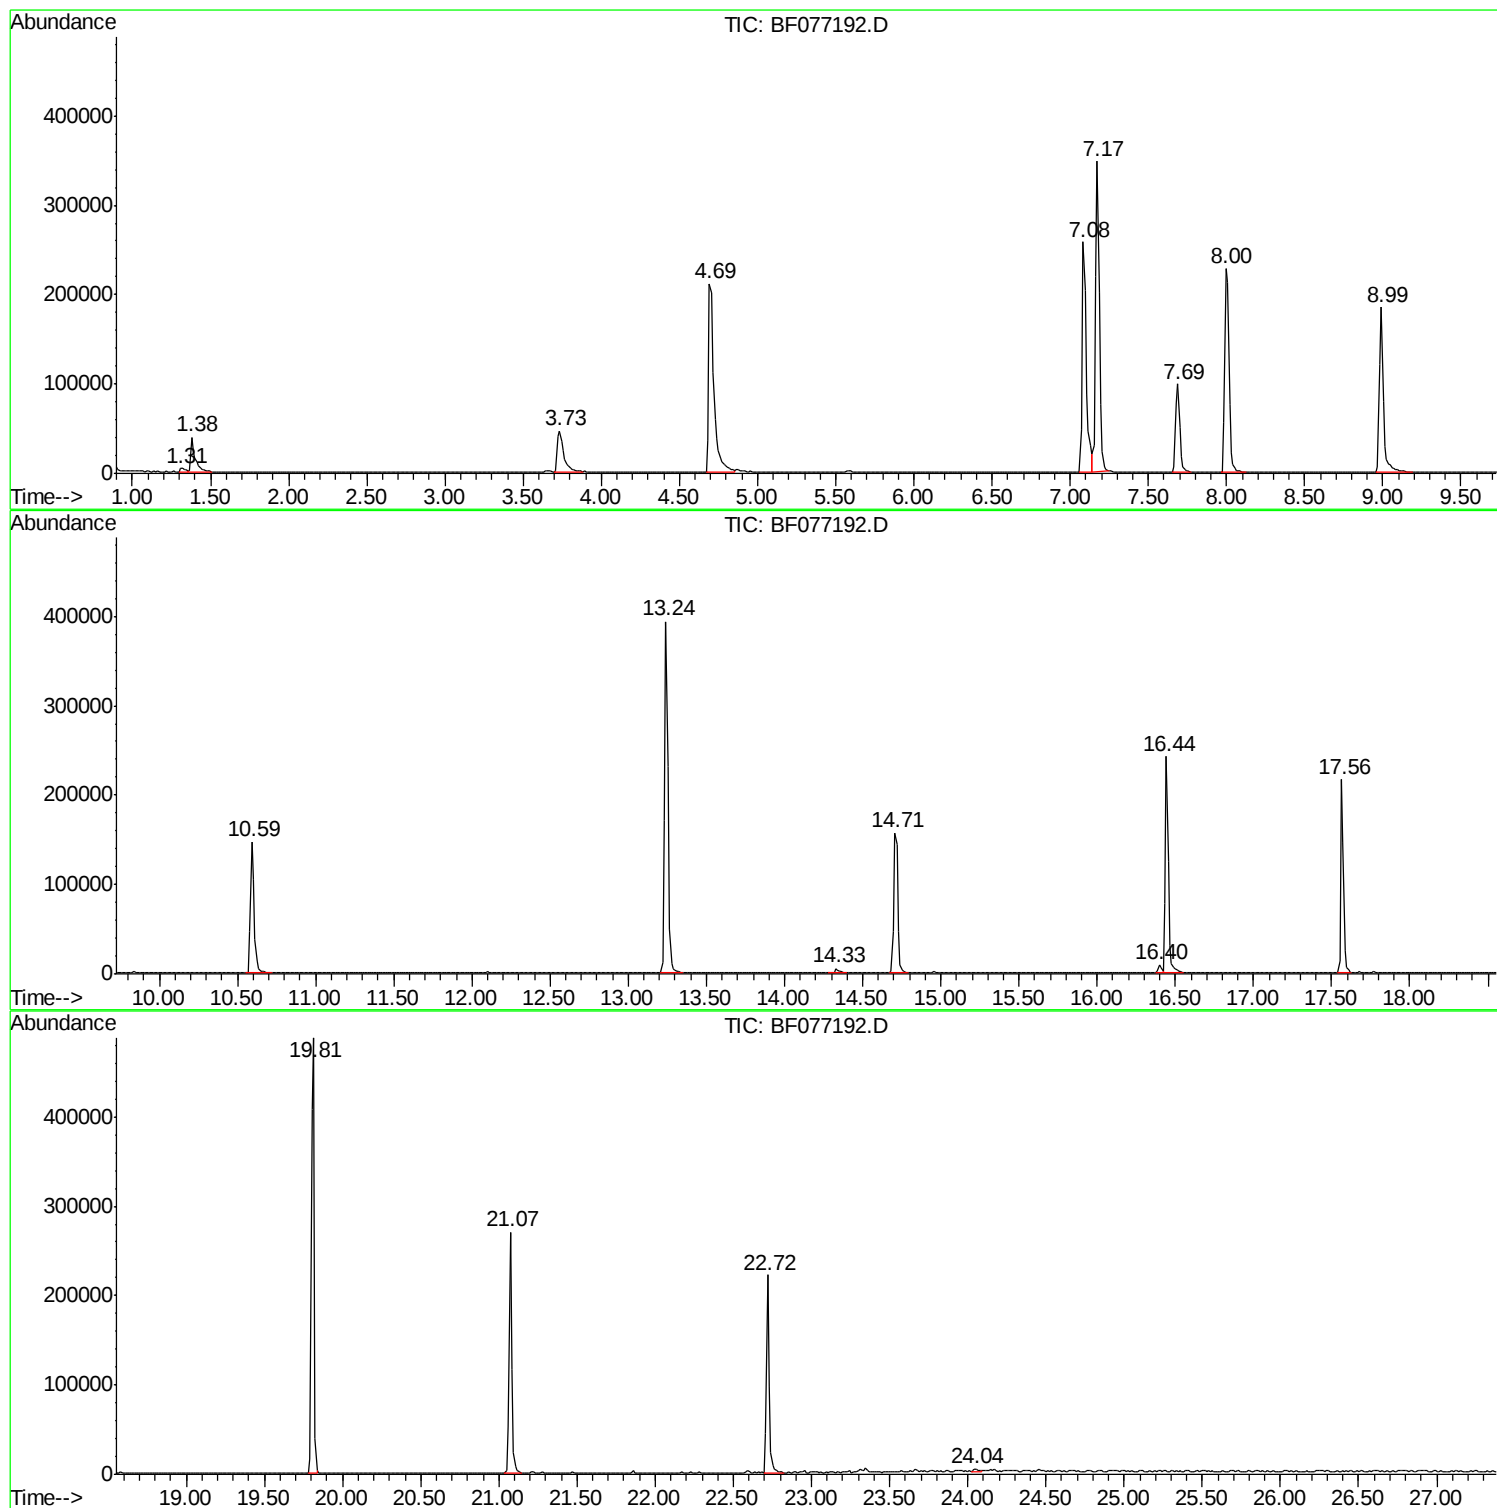

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020515\
Data File : BF077192.D
Acq On : 5 Feb 2015 19:23
Operator : TP/IZ
Sample : G1212-01
Misc : S
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-BPM-01-A1A-A2A-A3A-A4A










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.73	14.64 ng	130935	1,4-Dichlorobenzene-d4	7.69

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	59
2			Guanidine	59	CH5N3	000113-00-8	47
3			3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	36
4			2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	36
5			1,8-Nonanediol, 8-methyl-	174	C10H22O2	054725-73-4	28

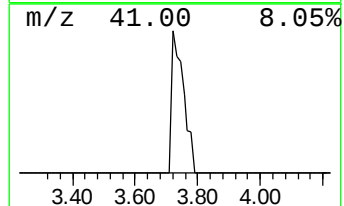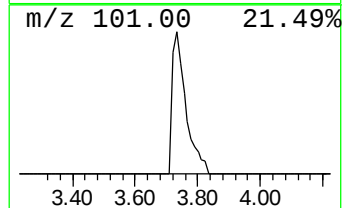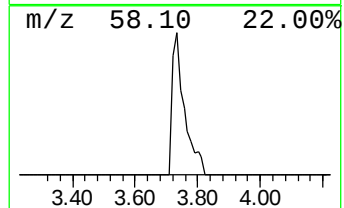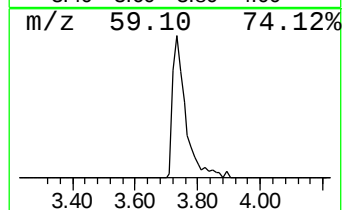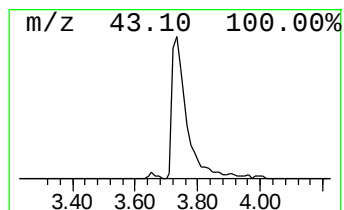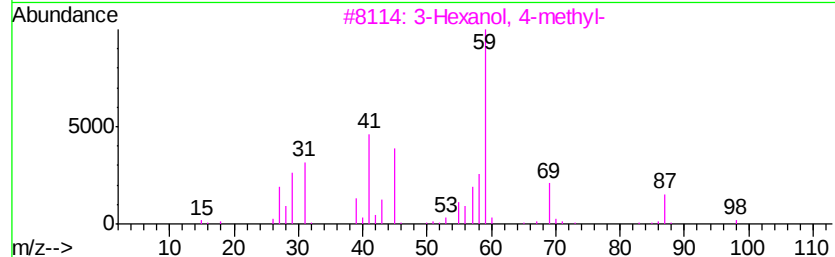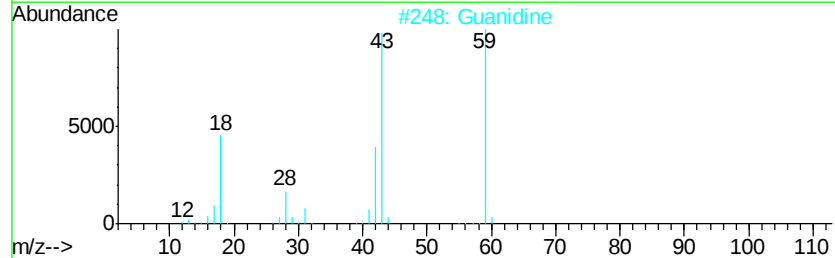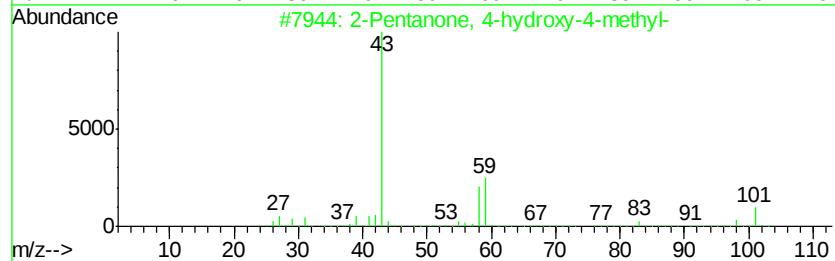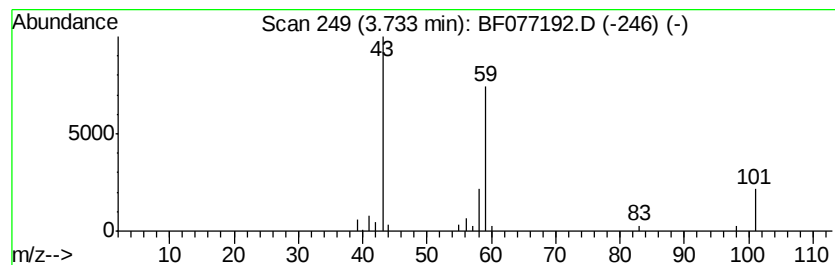

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF077192.D
Data File : BF077192.D
Acq On : 5 Feb 2015 19:23
Operator : TP/IZ
Sample : G1212-01
Misc : S
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-BPM-01-A1A-A2A-A3A-A4A










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 unknown7.17 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.17	68.90 ng	616114	1,4-Dichlorobenzene-d4	7.69

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
3		(5-METHYL-2-PYRIDYL)ACETONITRILE	132	C8H8N2	1000241-93-9	10
4		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	10
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

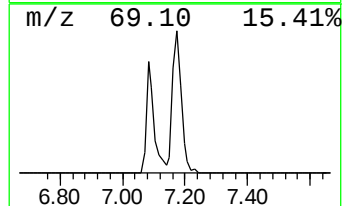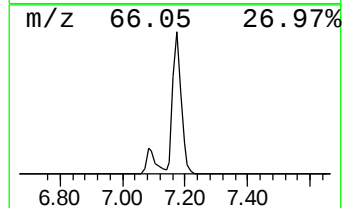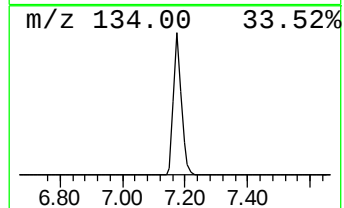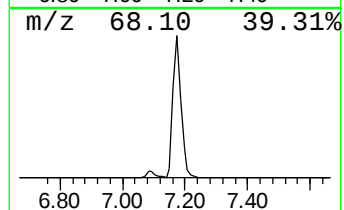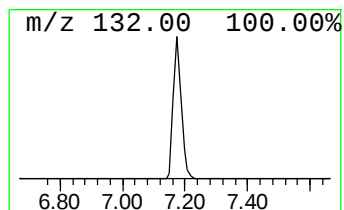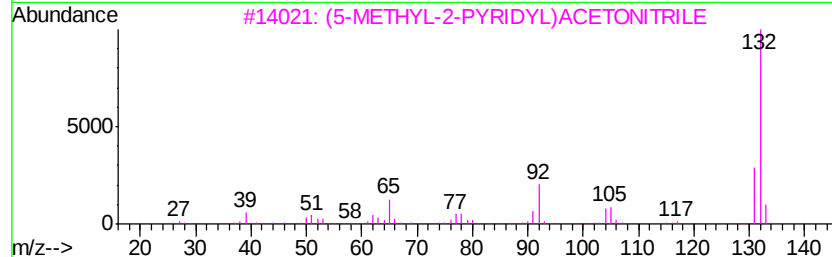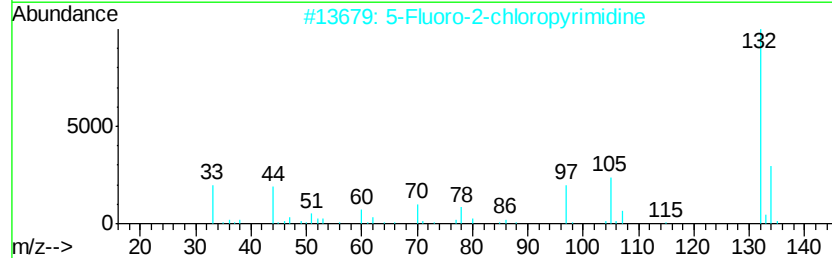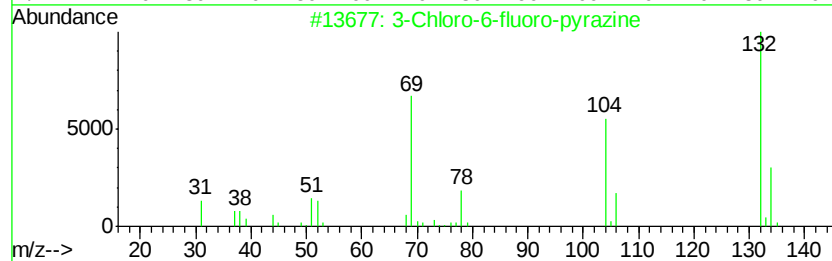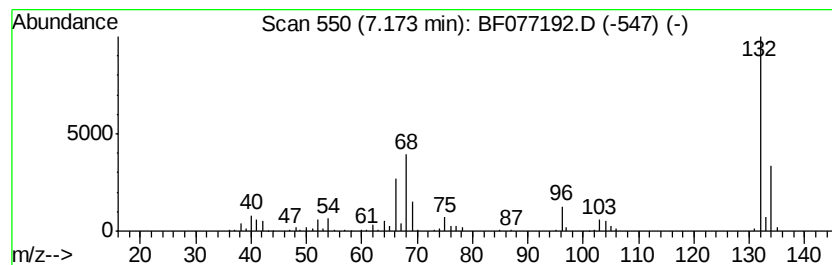

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020515\
Data File : BF077192.D
Acq On : 5 Feb 2015 19:23
Operator : TP/IZ
Sample : G1212-01
Misc : S
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-BPM-01-A1A-A2A-A3A-A4A

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	3.73	14.6	ng	130935	1	7.69	178850	20.0
unknown7.17	7.17	68.9	ng	616114	1	7.69	178850	20.0