


Data Path : Z:\HPCHEM1\BNA_F\Data\BF020515\
Data File : BF077183.D
Acq On : 5 Feb 2015 10:23
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jan 30 22:48:24 2015

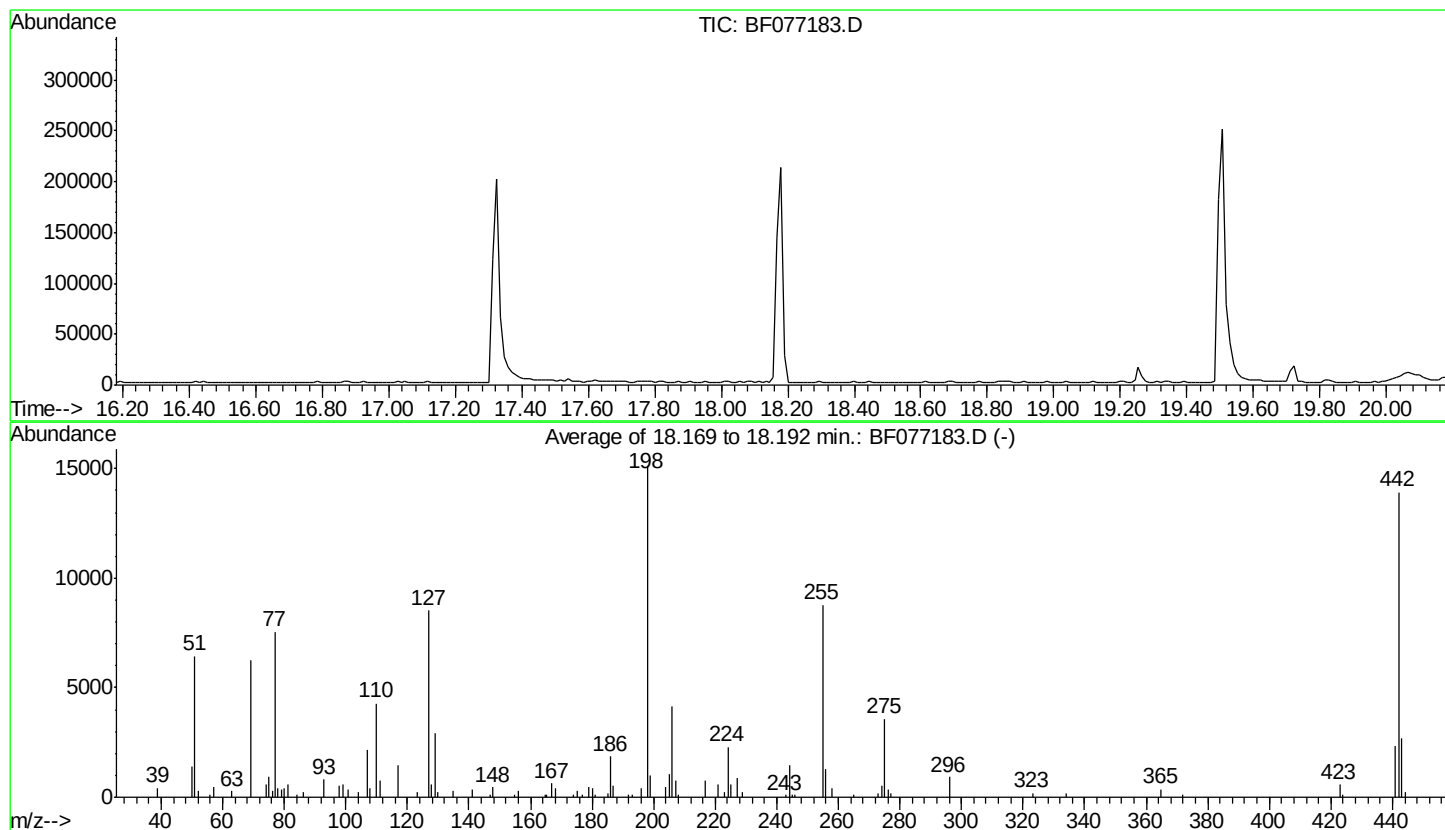

AutoFind: Scans 1512, 1513, 1514; Background Corrected with Scan 1508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.5	6435	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	41.2	6234	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	56.2	8508	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	15139	PASS
199	198	5	9	6.5	977	PASS
275	198	10	60	23.6	3575	PASS
365	198	1	100	2.4	369	PASS
441	442	0.01	24	16.6	2317	PASS
442	198	50	100	92.1	13940	PASS
443	442	15	24	19.4	2707	PASS