


Data Path : Z:\HPCHEM1\BNA_F\Data\BF020515\
 Data File : BF077196.D
 Acq On : 5 Feb 2015 21:41
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 30 22:48:24 2015

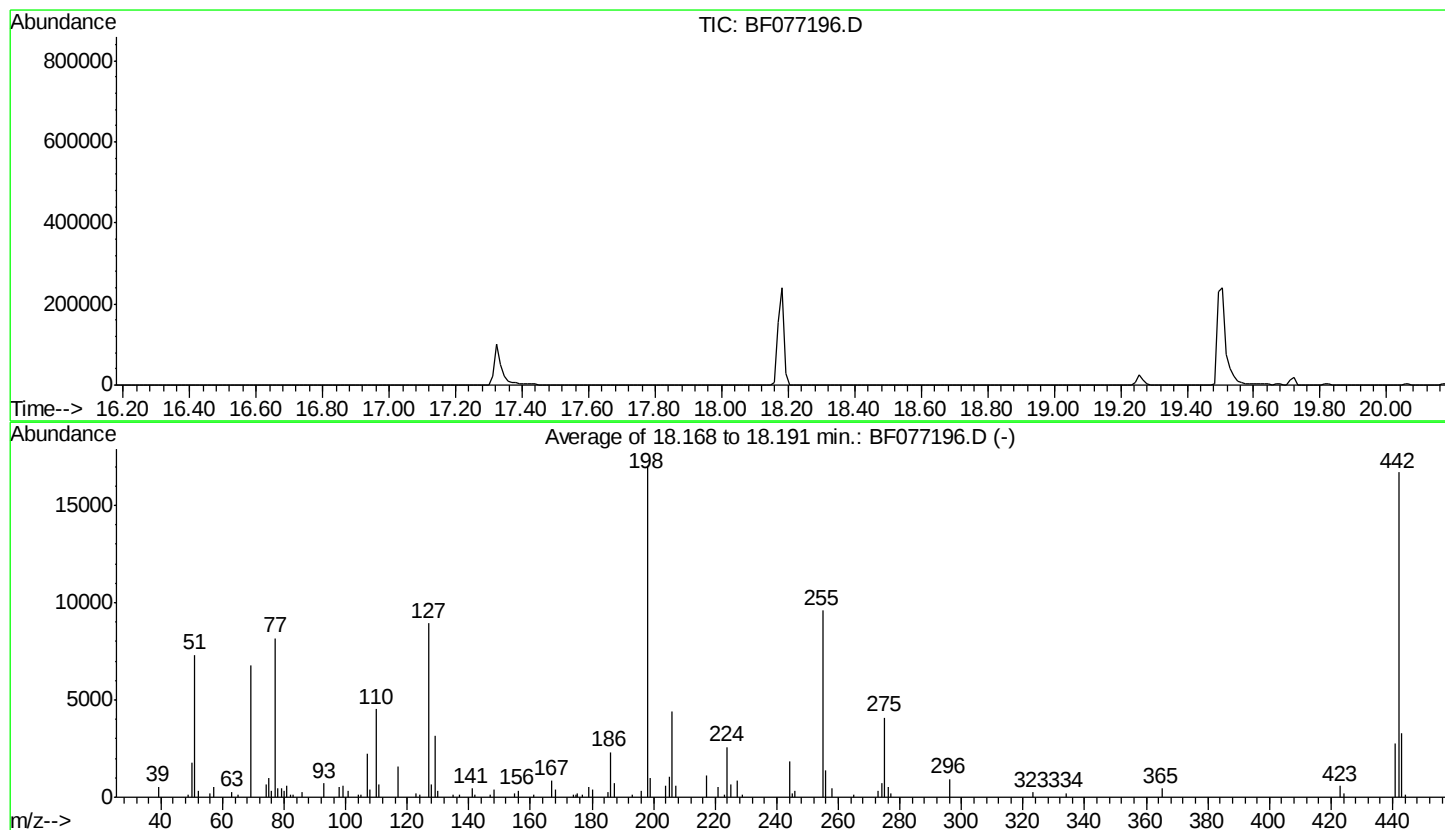

AutoFind: Scans 1512, 1513, 1514; Background Corrected with Scan 1508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.9	7310	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	39.7	6772	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.5	8943	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	17047	PASS
199	198	5	9	5.9	1001	PASS
275	198	10	60	24.0	4085	PASS
365	198	1	100	2.7	456	PASS
441	442	0.01	24	16.7	2793	PASS
442	198	50	100	98.0	16711	PASS
443	442	15	24	19.6	3270	PASS