

Data Path : Z:\HPCHEM1\BNA F\DATA\BF020516\
 Data File : BF084879.D
 Acq On : 6 Feb 2016 00:14
 Operator : SJ/IZ
 Sample : H1311-04 5X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SUP-B018(10-11)

Manual Integrations
 APPROVED

UMANGI
 2/8/2016 3:03:08 PM

Quant Time: Feb 06 03:48:20 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 03 14:16:01 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.66	152	174482	20.00	ng	-0.02
21) Naphthalene-d8	7.95	136	740926	20.00	ng	-0.02
38) Acenaphthene-d10	9.70	164	315495	20.00	ng	-0.03
63) Phenanthrene-d10	11.17	188	556872	20.00	ng	-0.03
75) Chrysene-d12	13.80	240	367963	20.00	ng	-0.03
86) Perylene-d12	15.17	264	313285	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.24	112	256569	22.90	ng	-0.03
7) Phenol-d6	6.30	99	346942	24.98	ng	-0.03
23) Nitrobenzene-d5	7.23	82	200376	15.23	ng	-0.03
41) 2,4,6-Tribromophenol	10.48	330	51459	15.64	ng	-0.05
44) 2-Fluorobiphenyl	9.02	172	382744	15.26	ng	-0.03
78) Terphenyl-d14	12.75	244	247294	15.23	ng	-0.05
Target Compounds						Qvalue
49) Dimethylphthalate	9.42	163	54623	2.27	ng	# 90
70) Phenanthrene	11.20	178	209399	6.78	ng	99
74) Fluoranthene	12.37	202	176327	5.64	ng	97
77) Pyrene	12.60	202	155365	5.51	ng	97
79) Butylbenzylphthalate	13.24	149	40452	3.17	ng	# 89
80) Benzo(a)anthracene	13.79	228	58069	2.54	ng	99
87) Benzo(b)fluoranthene	14.80	252	50749m	2.41	ng	
89) Benzo(a)pyrene	15.12	252	36813	2.05	ng	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA F\DATA\BF020516\
Data File : BF084879.D
Acq On : 6 Feb 2016 00:14
Operator : SJ/IZ
Sample : H1311-04 5X
Misc :
ALS Vial : 24 Sample Multiplier: 1


Instrument :
BNA_F
ClientSampleId :
SUP-B018(10-11)

Manual Integrations
APPROVED

UMANGI
2/8/2016 3:03:08 PM

Quant Time: Feb 06 03:48:20 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 03 14:16:01 2016
Response via : Initial Calibration

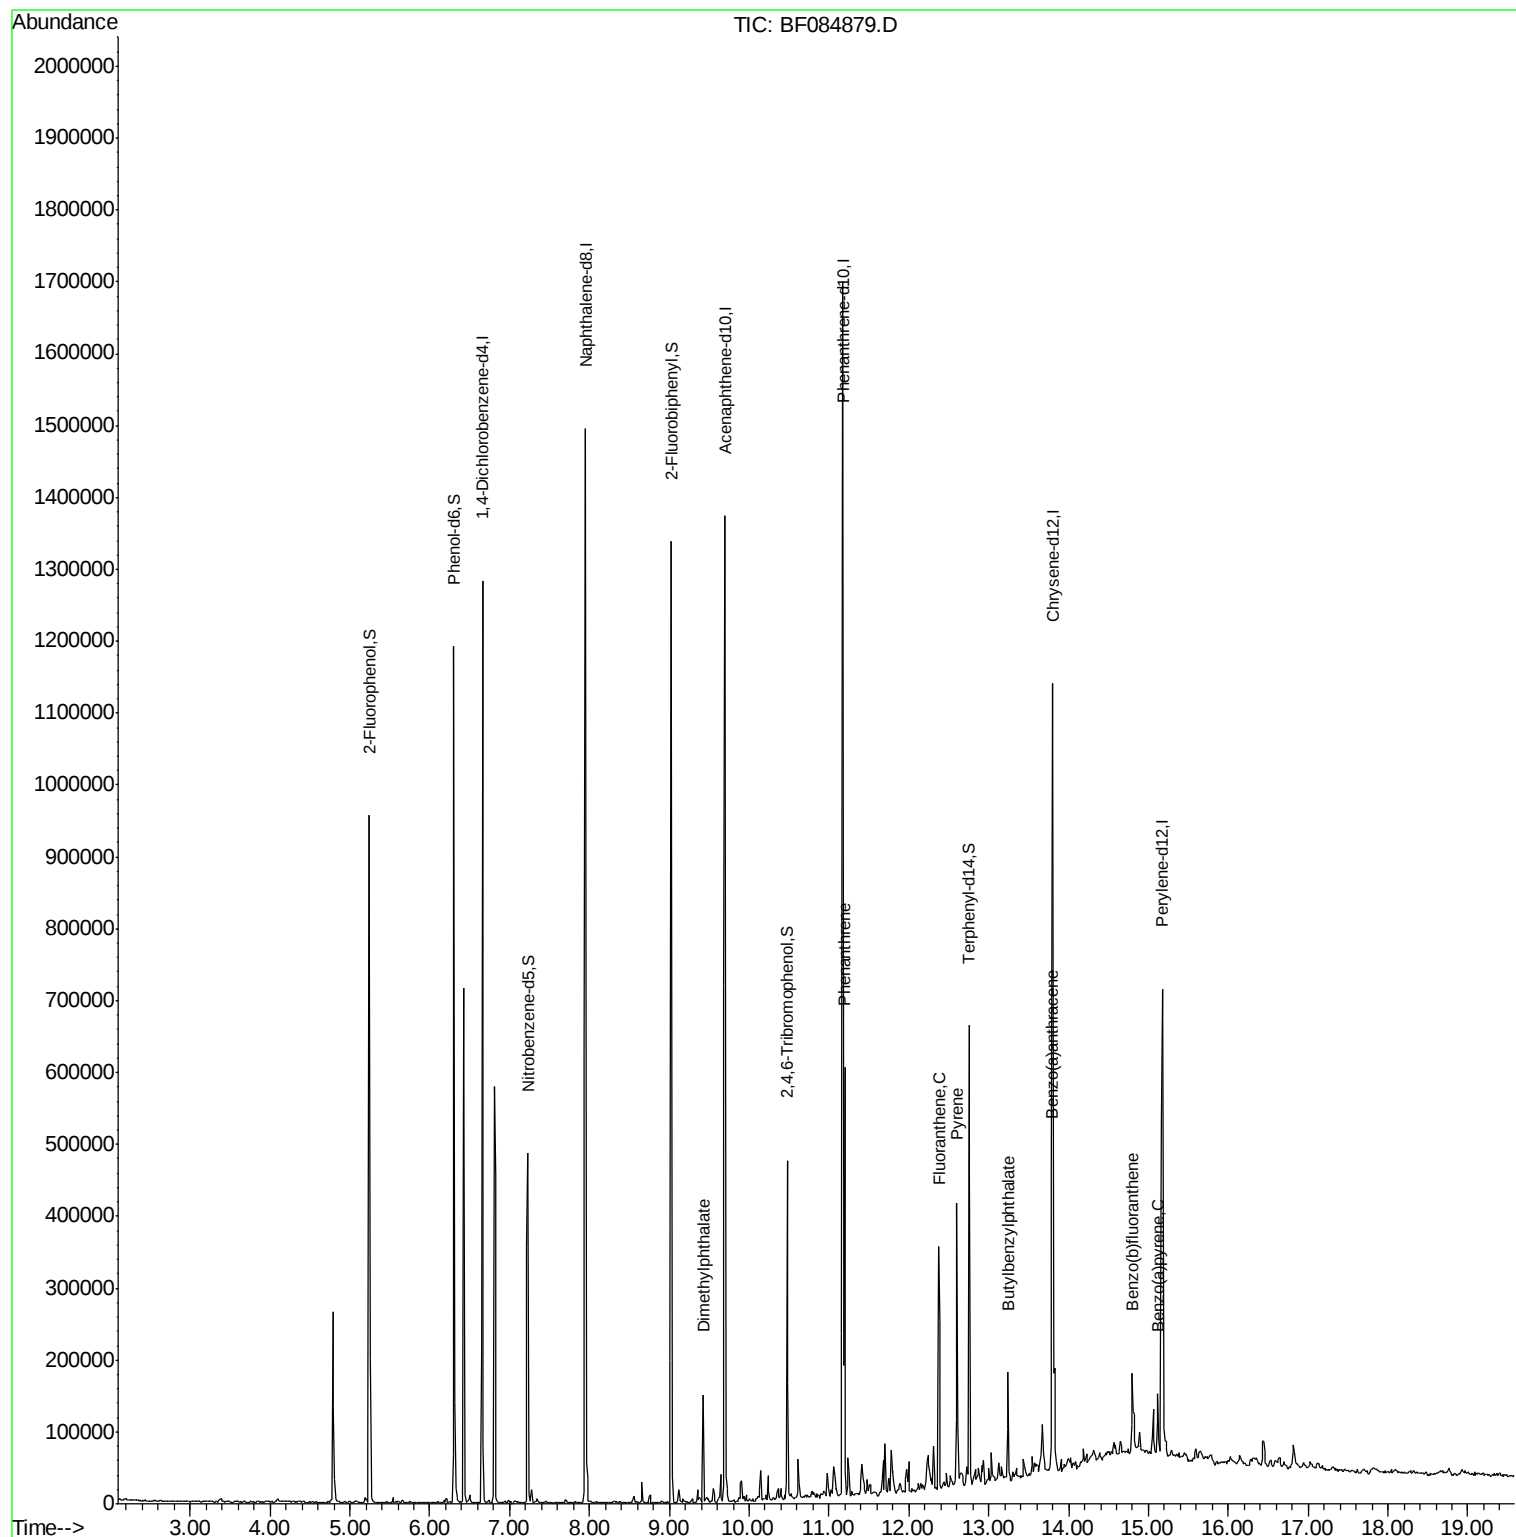

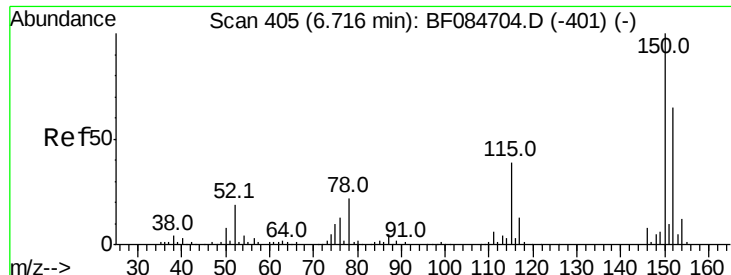

#1





1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.66 min Scan# 400
Delta R.T. -0.02 min
Lab File: BF084879.D
Acq: 6 Feb 2016 00:14

Instrument :
BNA_F
ClientSampleId :
SUP-B018(10-11)

Tot Ion	Ratio	Lower	Upper
152	100		
150	158.0	123.0	184.4
115	63.8	51.4	77.2

Manual Integrations
APPROVED




UMANGI
2/8/2016 3:03:08 PM

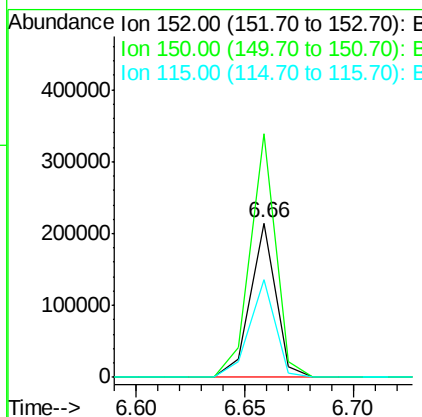


#5

2-Fluorophenol
Concen: 22.90 ng
RT: 5.24 min Scan# 276
Delta R.T. -0.03 min
Lab File: BF084879.D
Acq: 6 Feb 2016 00:14

Tgt Ion	Ratio	Lower	Upper
112	100		
64	58.7	36.6	55.0#
63	30.7	19.4	29.0#

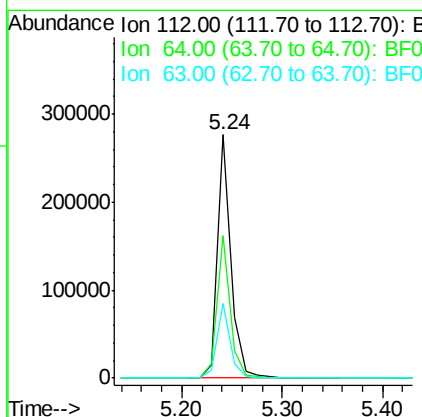

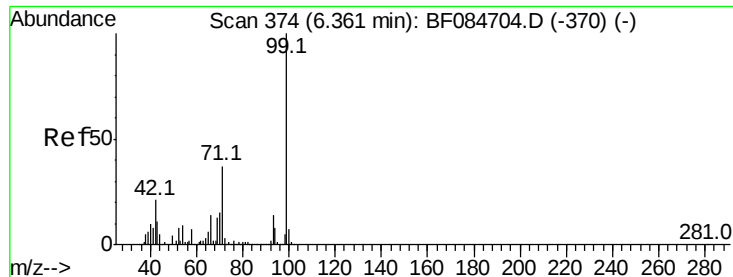

#7

Phenol-d6

Concen: 24.98 ng

RT: 6.30 min Scan# 369

Delta R.T. -0.03 min

Lab File: BF084879.D

Acq: 6 Feb 2016 00:14

Instrument :

BNA_F





ClientSampleId :

SUP-B018(10-11)

Tot Ion	99	Resp	346942
Ion Ratio	Lower	Upper	
99	100		
42	20.1	12.8	19.2#
71	36.1	30.9	46.3

Manual Integrations
APPROVED

UMANGI
2/8/2016 3:03:08 PM

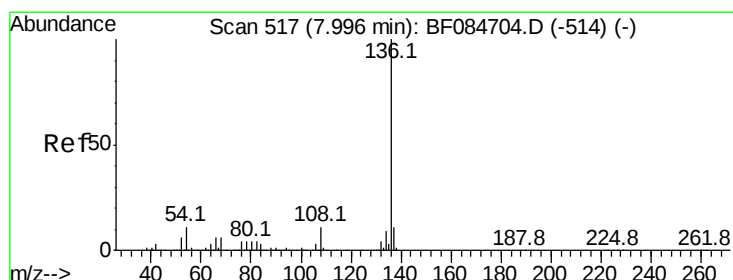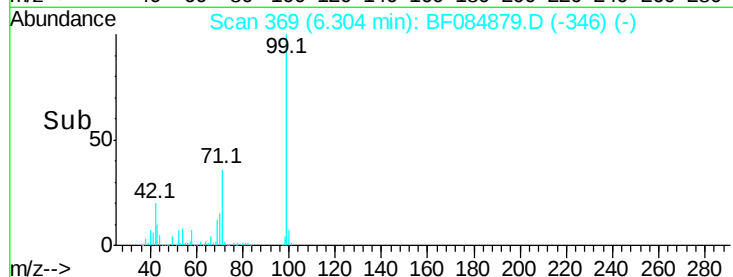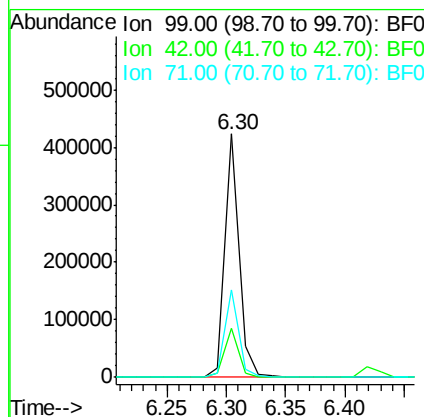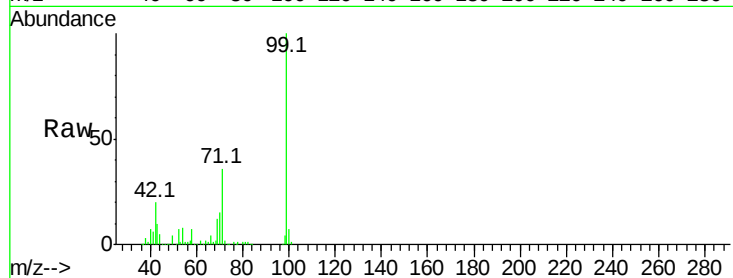

#21

Naphthalene-d8

Concen: 20.00 ng




RT: 7.95 min Scan# 513


Delta R.T. -0.02 min

Lab File: BF084879.D

Acq: 6 Feb 2016 00:14

Tgt Ion	136	Resp	740926
Ion Ratio	Lower	Upper	
136	100		
137	10.7	8.7	13.1
54	6.5	5.8	8.8
68	4.0	4.2	6.2#

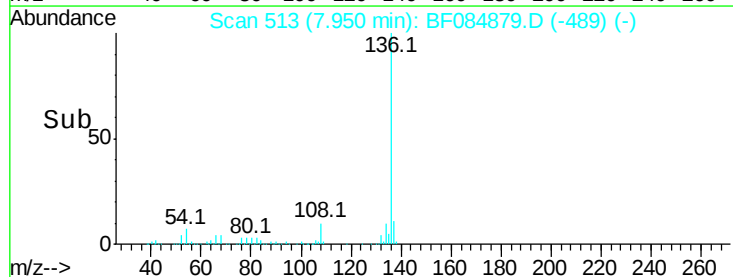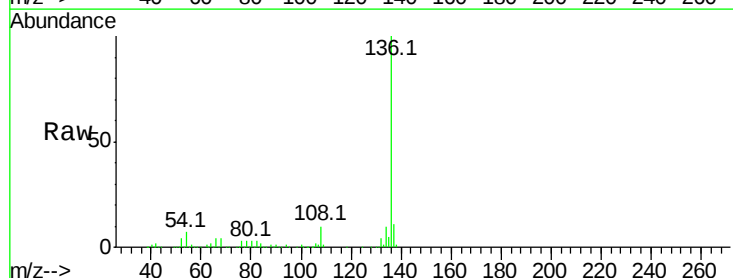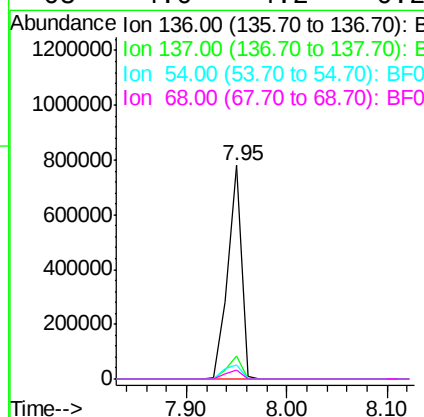

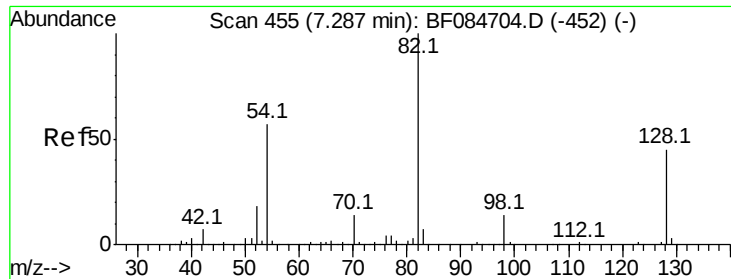

#23

Nitrobenzene-d5

Concen: 15.23 ng

RT: 7.23 min Scan# 450

Delta R.T. -0.03 min

Lab File: BF084879.D

Acq: 6 Feb 2016 00:14

Instrument :

BNA_F

ClientSampleId :


SUP-B018(10-11)

Tot Ion: 82 Resp: 200376
Ion Ratio Lower Upper




82	100		
128	54.9	34.6	51.8#
54	48.4	38.4	57.6

Manual Integrations
APPROVED

UMANGI
2/8/2016 3:03:08 PM



Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

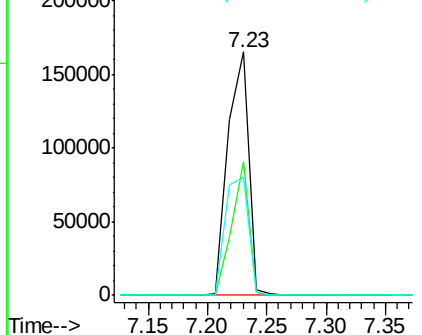

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.70 min Scan# 666


Delta R.T. -0.03 min

Lab File: BF084879.D



Acq: 6 Feb 2016 00:14


Tgt Ion:164 Resp: 315495
Ion Ratio Lower Upper

164	100		
162	104.9	85.1	127.7
160	49.1	37.5	56.3



Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

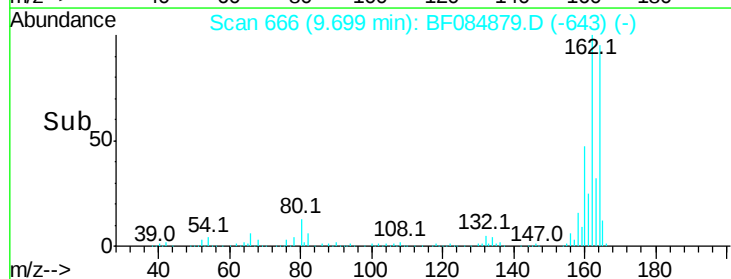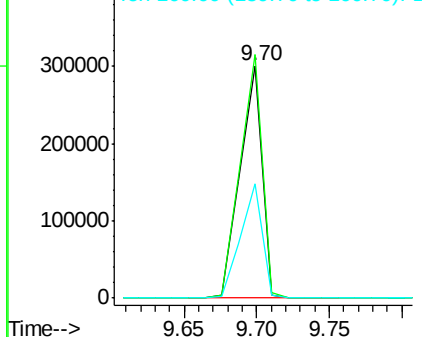

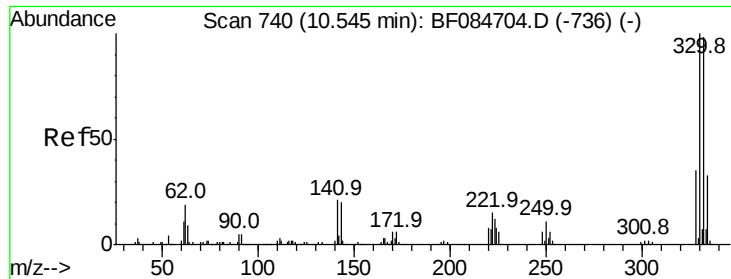


#41
 2,4,6-Tribromophenol
 Concen: 15.64 ng
 RT: 10.48 min Scan# 734
 Delta R.T. -0.05 min
 Lab File: BF084879.D
 Acq: 6 Feb 2016 00:14

Instrument :
 BNA_F
 ClientSampleId :
 SUP-B018(10-11)




Tot Ion	Ratio	Lower	Upper
330	100		
332	97.6	76.6	114.8
141	40.7	27.8	41.6

Manual Integrations
 APPROVED

UMANGI
 2/8/2016 3:03:08 PM




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

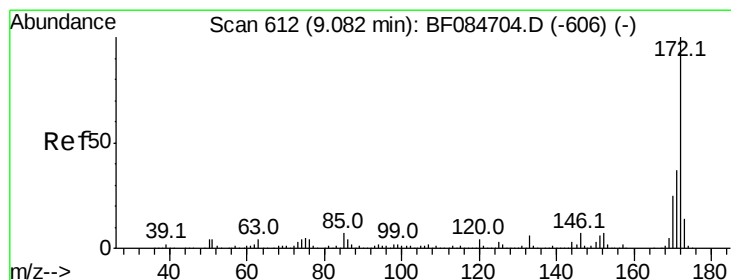
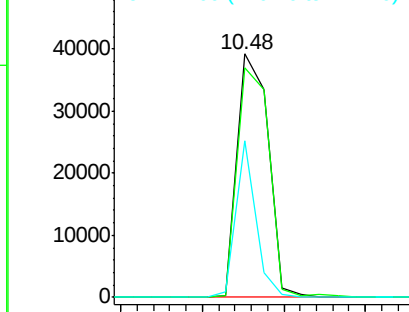



#44
 2-Fluorobiphenyl
 Concen: 15.26 ng
 RT: 9.02 min Scan# 607
 Delta R.T. -0.03 min
 Lab File: BF084879.D
 Acq: 6 Feb 2016 00:14

Tgt Ion	Ratio	Lower	Upper
172	100		
171	34.4	28.9	43.3
170	23.6	18.6	27.8

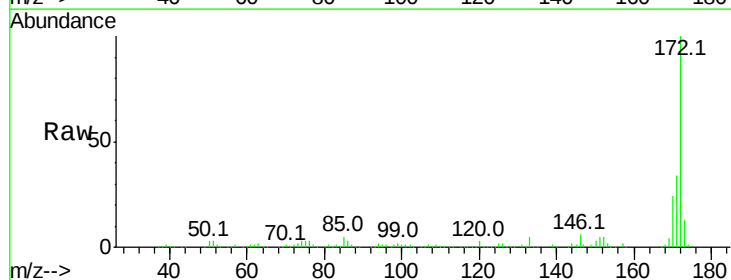

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

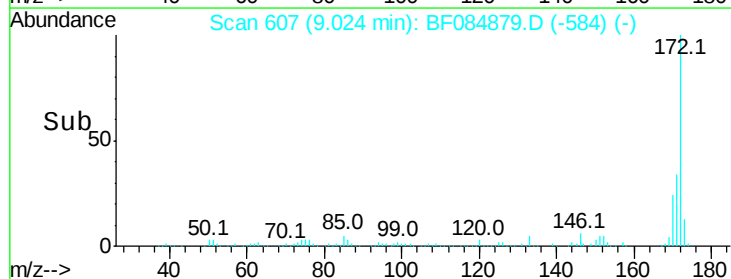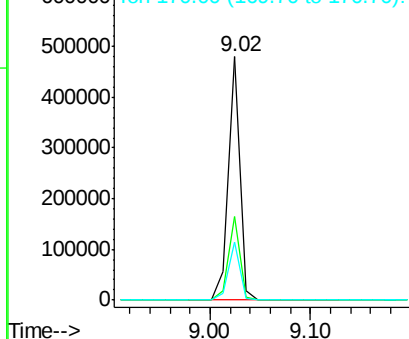

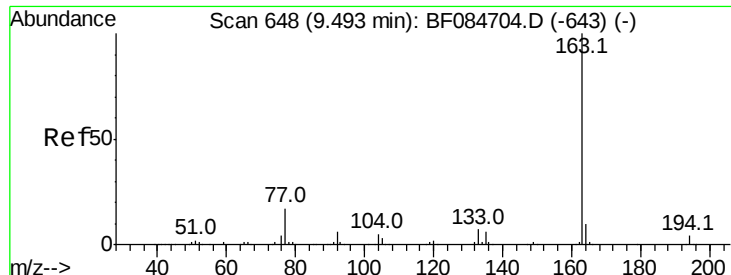


#49
Dimethylphthalate
Concen: 2.27 ng
RT: 9.42 min Scan# 642
Delta R.T. -0.05 min
Lab File: BF084879.D
Acq: 6 Feb 2016 00:14

Instrument :
BNA_F
ClientSampleId :
SUP-B018(10-11)




Tot Ion	Ratio	Resp	Lower	Upper
163	100	54623		
194	3.1	8.0	12.0#	
164	9.8	8.0	12.0	

Manual Integrations
APPROVED

UMANGI
2/8/2016 3:03:08 PM




Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

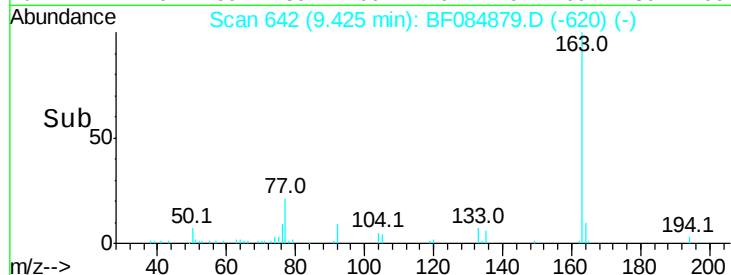
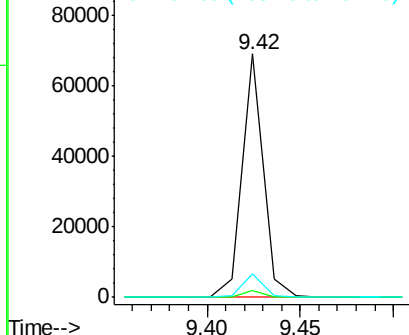



#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.17 min Scan# 795
Delta R.T. -0.03 min
Lab File: BF084879.D
Acq: 6 Feb 2016 00:14

Tgt Ion	Ratio	Resp	Lower	Upper
188	100	556872		
94	8.5	9.0	13.4#	
80	8.7	9.6	14.4#	



Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

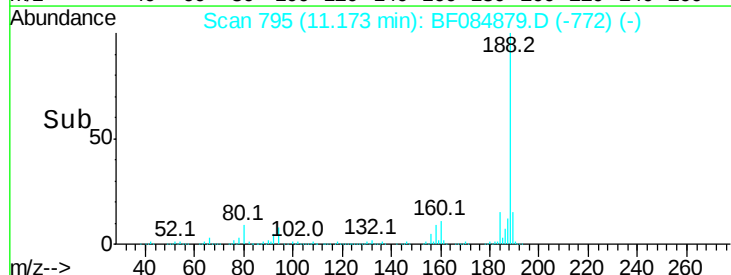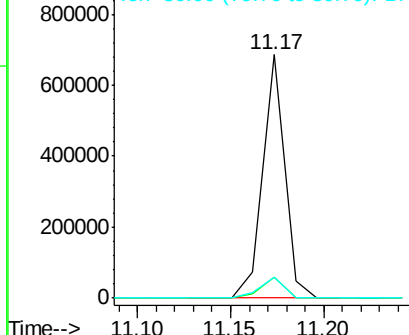

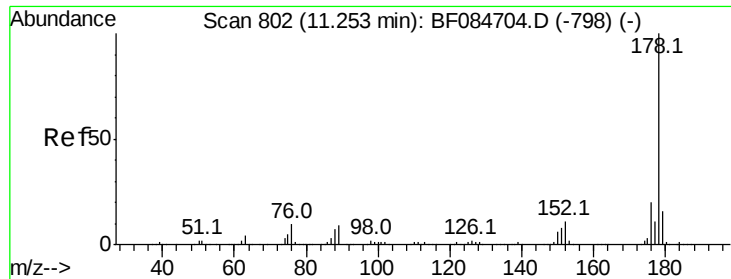





#70
Phenanthrene
Concen: 6.78 ng
RT: 11.20 min Scan# 797
Delta R.T. -0.03 min
Lab File: BF084879.D
Acq: 6 Feb 2016 00:14

Instrument :
BNA_F
ClientSampleId :
SUP-B018(10-11)

Tot Ion	Ratio	Lower	Upper
178	100		
176	18.7	15.3	22.9
179	15.2	12.0	18.0




Manual Integrations
APPROVED


UMANGI
2/8/2016 3:03:08 PM

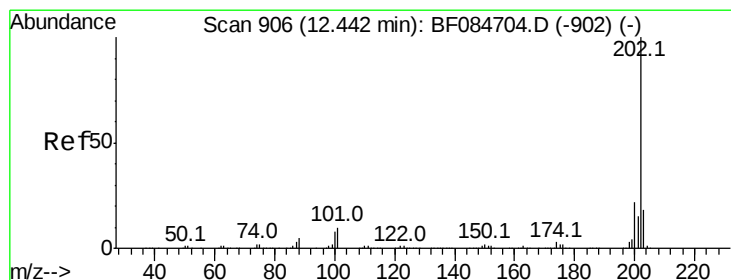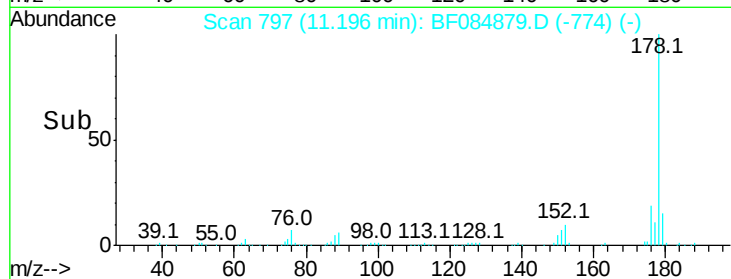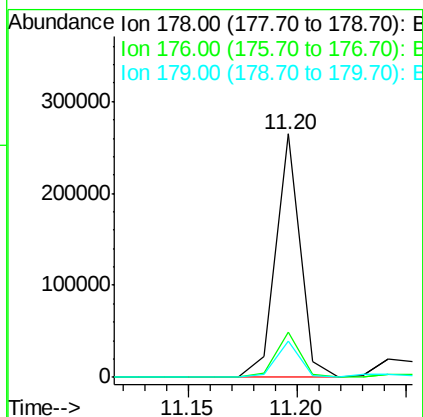

#74
Fluoranthene
Concen: 5.64 ng
RT: 12.37 min Scan# 900
Delta R.T. -0.05 min
Lab File: BF084879.D
Acq: 6 Feb 2016 00:14

Tgt Ion	Ratio	Lower	Upper
202	100		
101	15.1	0.0	32.8
203	17.6	0.0	37.9

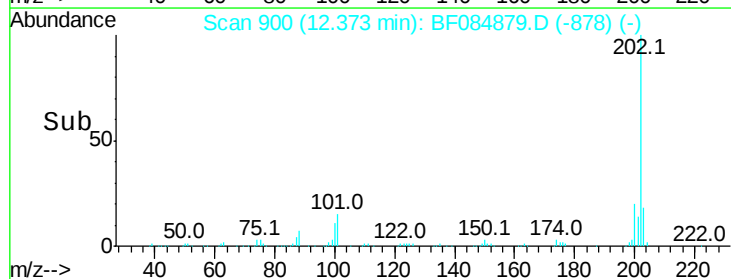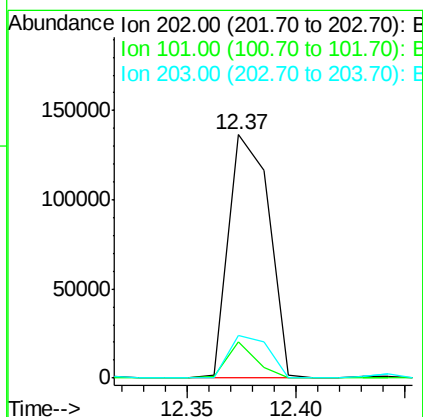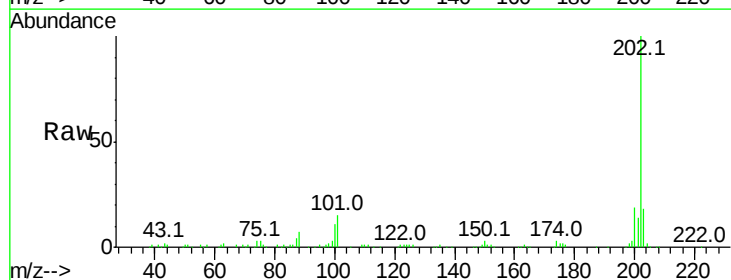



#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.80 min Scan# 1025

Delta R.T. -0.03 min

Lab File: BF084879.D

Acq: 6 Feb 2016 00:14

Instrument :

BNA_F





ClientSampleId :

SUP-B018(10-11)

Tot Ion	Ratio	Lower	Upper
240	100		
120	9.2	9.5	14.3#
236	25.3	20.6	31.0

Manual Integrations
APPROVED

UMANGI
2/8/2016 3:03:08 PM

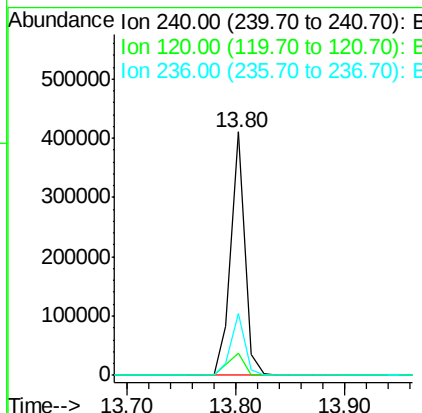

#77

Pyrene

Concen: 5.51 ng




RT: 12.60 min Scan# 920


Delta R.T. -0.03 min

Lab File: BF084879.D

Acq: 6 Feb 2016 00:14

Tgt Ion	Ratio	Lower	Upper
202	100		
200	20.2	17.2	25.8
203	16.9	14.3	21.5

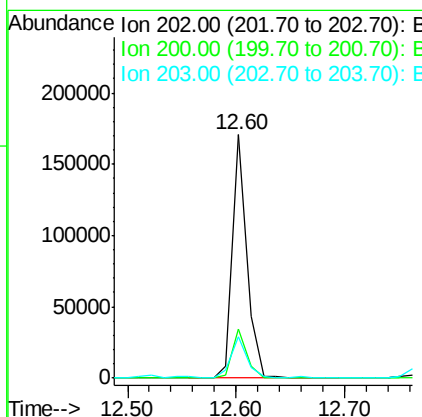

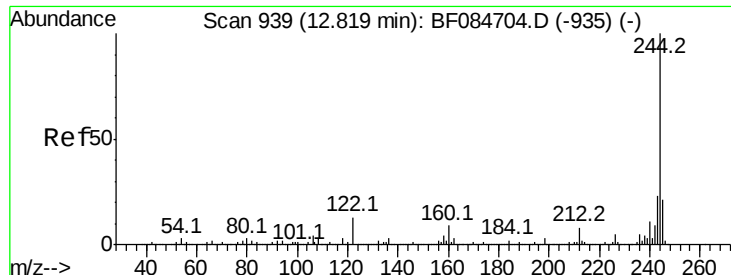





#78
 Terphenyl-d14
 Concen: 15.23 ng
 RT: 12.75 min Scan# 933
 Delta R.T. -0.05 min
 Lab File: BF084879.D
 Acq: 6 Feb 2016 00:14

Instrument :
 BNA_F
 ClientSampleId :
 SUP-B018(10-11)

Tot Ion	Ratio	Lower	Upper
244	100		
212	7.4	5.7	8.5
122	17.0	7.4	11.0




Manual Integrations
 APPROVED


UMANGI
 2/8/2016 3:03:08 PM

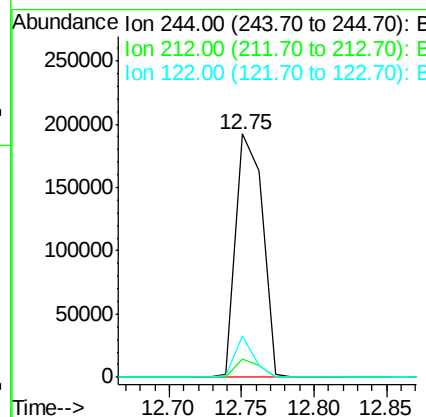

#79
 Butylbenzylphthalate
 Concen: 3.17 ng
 RT: 13.24 min Scan# 976
 Delta R.T. -0.03 min
 Lab File: BF084879.D
 Acq: 6 Feb 2016 00:14

Tgt Ion	Ratio	Lower	Upper
149	100		
91	62.4	57.6	86.4
206	20.0	13.2	19.8

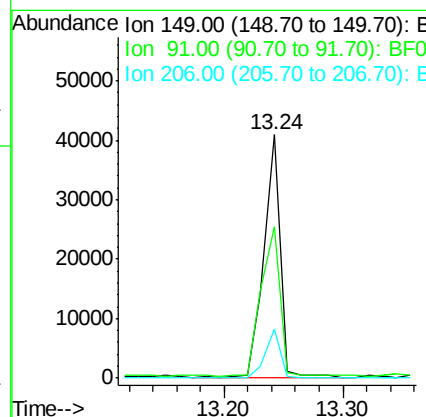







#80
 Benzo(a)anthracene
 Concen: 2.54 ng
 RT: 13.79 min Scan# 1024
 Delta R.T. -0.03 min
 Lab File: BF084879.D
 Acq: 6 Feb 2016 00:14

Instrument :
 BNA_F
 ClientSampleId :
 SUP-B018(10-11)

Tot Ion	Ratio	Lower	Upper
228	100		
226	28.3	21.8	32.6
229	19.6	15.8	23.8




Manual Integrations
 APPROVED


UMANGI
 2/8/2016 3:03:08 PM

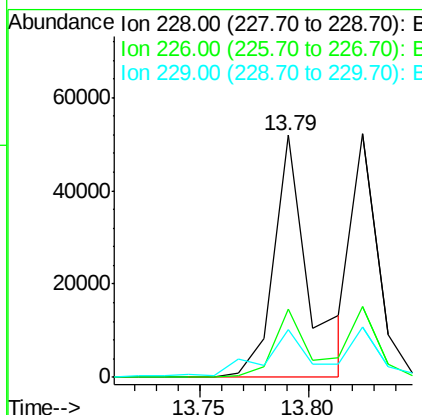

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.17 min Scan# 1145
 Delta R.T. -0.03 min
 Lab File: BF084879.D
 Acq: 6 Feb 2016 00:14

Tgt Ion	Ratio	Lower	Upper
264	100		
260	22.3	19.4	29.2
265	21.0	17.8	26.6

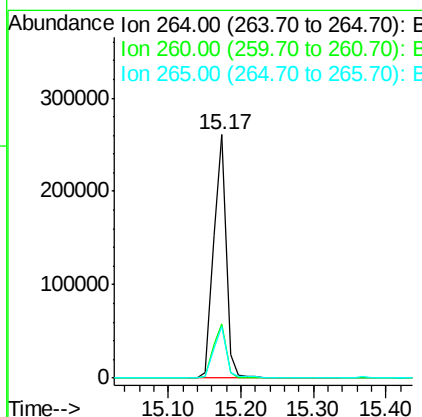

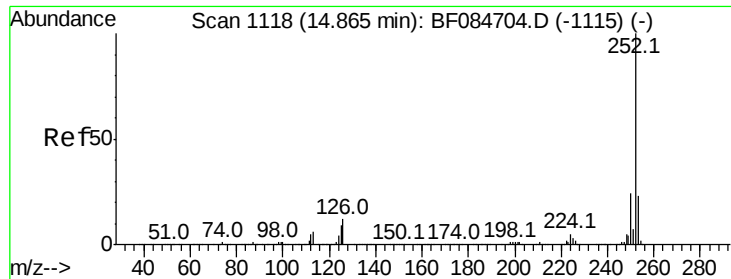





#87
Benzo(b)fluoranthene
Concen: 2.41 ng
RT: 14.80 min Scan# 1112
Delta R.T. -0.03 min
Lab File: BF084879.D
Acq: 6 Feb 2016 00:14

Instrument :
BNA_F
ClientSampleId :
SUP-B018(10-11)

Tot Ion	Ratio	Lower	Upper
252	100		
253	24.9	17.3	25.9
125	11.6	6.5	9.7

Manual Integrations
APPROVED

UMANGI
2/8/2016 3:03:08 PM

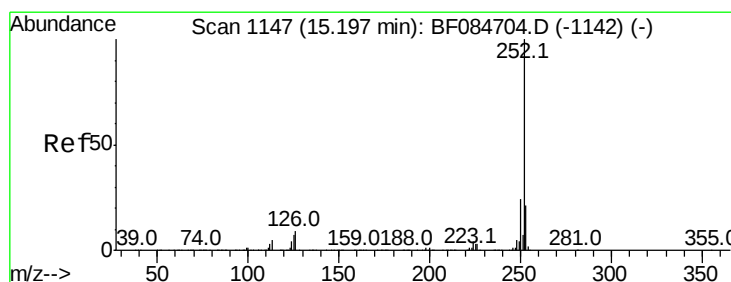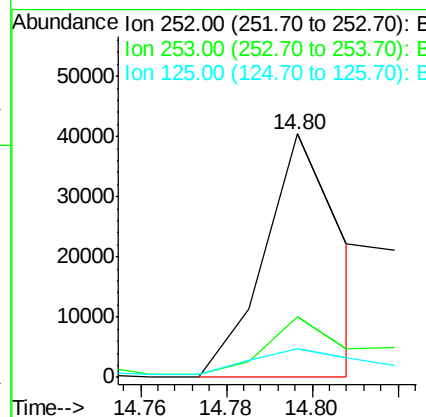

#89
Benzo(a)pyrene
Concen: 2.05 ng
RT: 15.12 min Scan# 1140
Delta R.T. -0.03 min
Lab File: BF084879.D
Acq: 6 Feb 2016 00:14

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.4	17.3	25.9
125	9.7	7.0	10.4

